

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102517\
 Data File : BE094530.D
 Acq On : 25 Oct 2017 12:50
 Operator : SJ/JU
 Sample : I5693-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EQB-2-100417

Manual Integrations
 APPROVED

Sohil
 10/27/2017 8:28:35 AM

Quant Time: Oct 25 18:34:04 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 25 17:03:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1132	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	6390	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4118	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	9182m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	8493	0.40	ng/ul	0.00
20) Perylene-d12	23.94	264	6387m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3793	0.37	ng/ul	-0.02
14) Fluoranthene-d10	19.27	212	9870	0.36	ng/ul	-0.02
Target Compounds						
8) Acenaphthene	14.58	153	463	0.035	ng/ul#	39
23) Benzo(a)pyrene	23.77	252	2329	0.130	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102517\
Data File : BE094530.D
Acq On : 25 Oct 2017 12:50
Operator : SJ/JU
Sample : I5693-09
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
EQB-2-100417

Manual Integrations
APPROVED

Sohil
10/27/2017 8:28:35 AM

Quant Time: Oct 25 18:34:04 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:03:27 2017
Response via : Initial Calibration

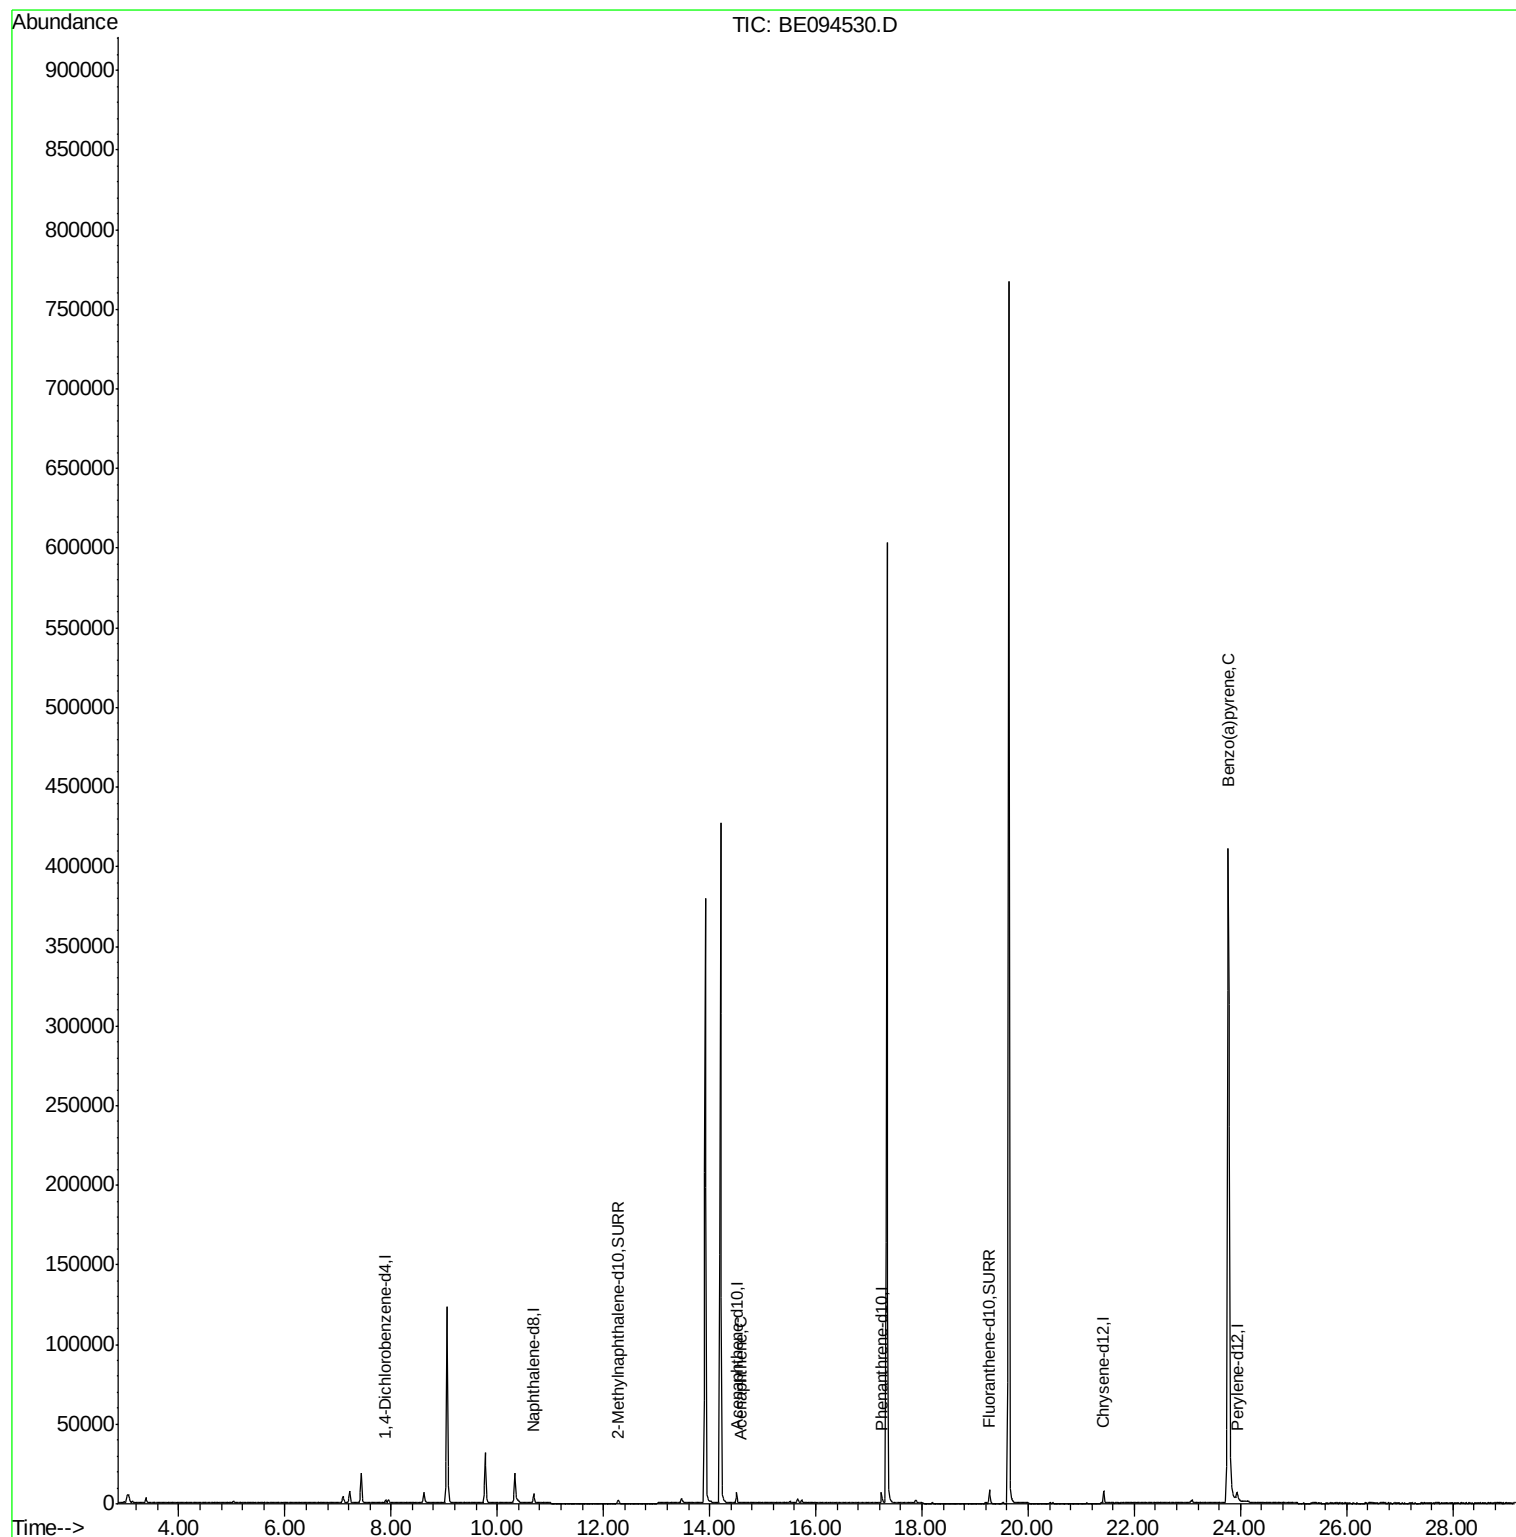

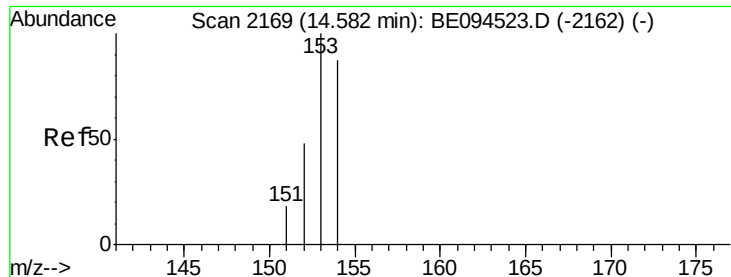

#8

Acenaphthene

Concen: 0.035 ng/ul

RT: 14.58 min Scan# 2169

Delta R.T. -0.00 min

Lab File: BE094530.D

Acq: 25 Oct 2017 12:50

Instrument :

BNA_E





ClientSampleId :

EQB-2-100417

Tgt Ion:	153	Resp:	463
Ion Ratio	Lower	Upper	
153	100		
152	18.4	40.3	60.5#
154	24.7	71.4	107.2#

Manual Integrations
APPROVED

Sohil
10/27/2017 8:28:35 AM

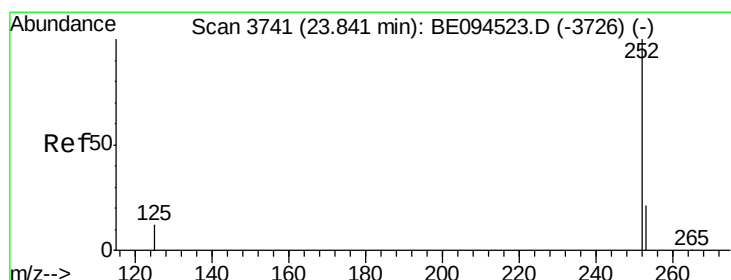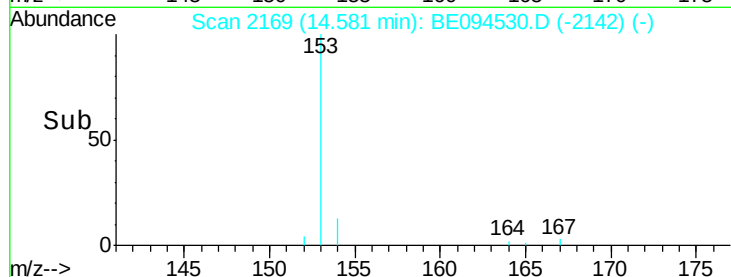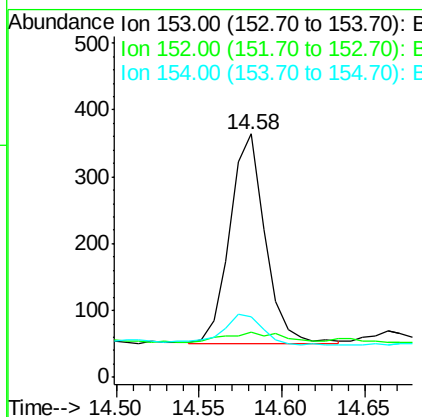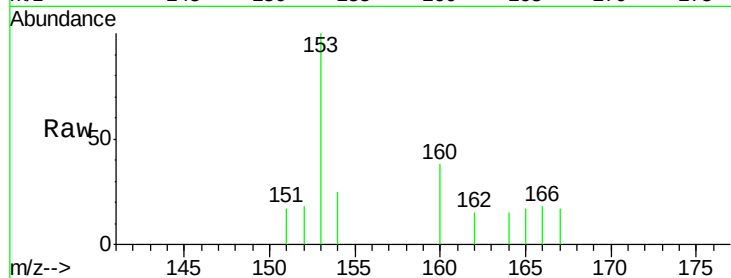

#23

Benzo(a)pyrene

Concen: 0.130 ng/ul

RT: 23.77 min Scan# 3726

Delta R.T. -0.07 min

Lab File: BE094530.D

Acq: 25 Oct 2017 12:50

Tgt Ion:	252	Resp:	2329
Ion Ratio	Lower	Upper	
252	100		
253	45.0	28.5	42.7#
125	39.8	18.1	27.1#

