


Data Path : Z:\HPCHEM1\BNA_E\Data\BE102714\
 Data File : BE088315.D
 Acq On : 27 Oct 2014 14:38
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102714.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 28 10:16:06 2014

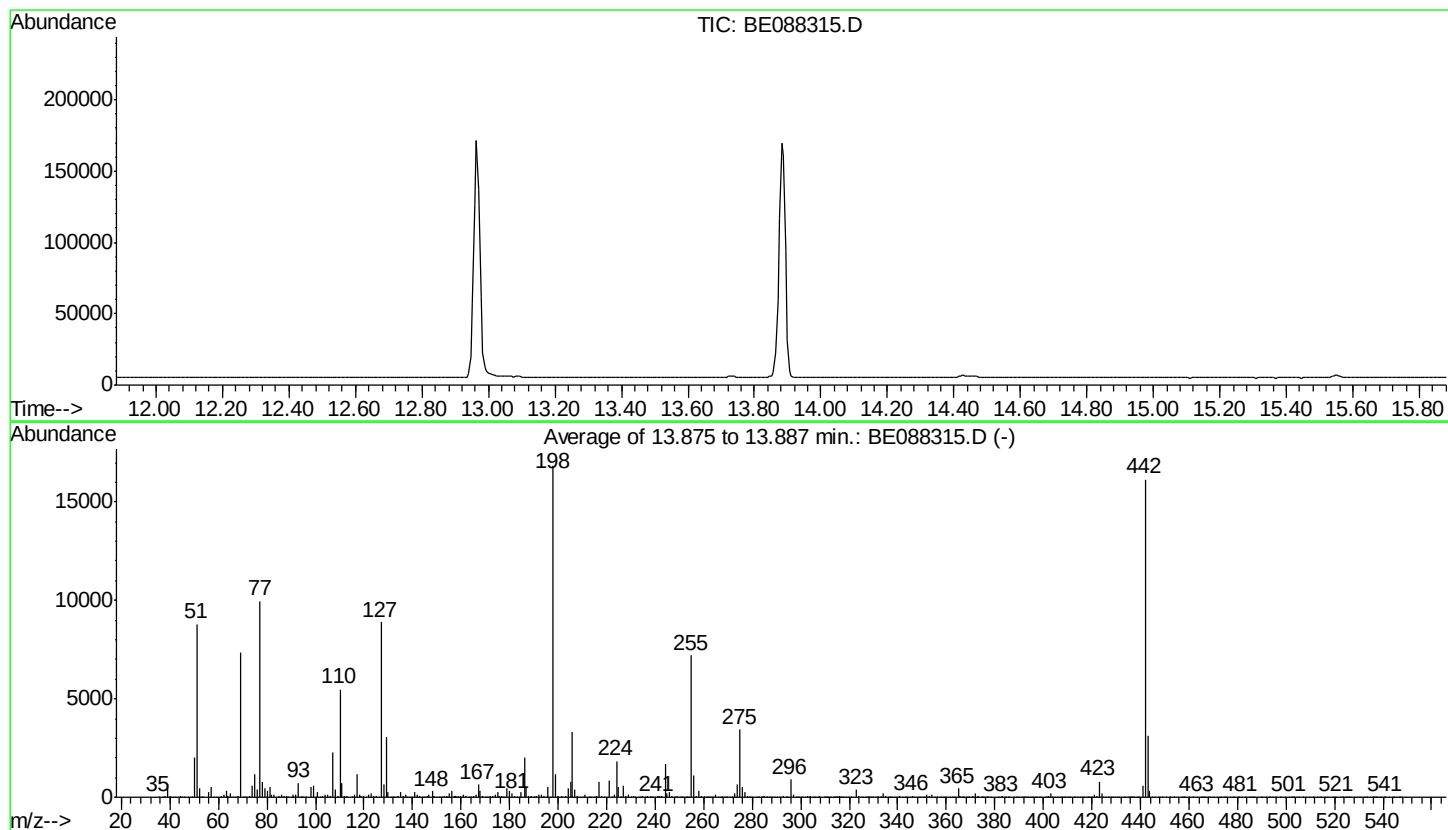

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	8806	PASS
68	69	0.00	2	0.9	68	PASS
69	198	0.00	100	43.5	7326	PASS
70	69	0.00	2	0.3	25	PASS
127	198	10	80	52.8	8892	PASS
197	198	0.00	2	0.2	32	PASS
198	198	100	100	100.0	16845	PASS
199	198	5	9	6.8	1146	PASS
275	198	10	60	20.4	3433	PASS
365	198	1	100	2.7	452	PASS
441	442	0.01	24	3.8	606	PASS
442	198	50	100	95.8	16133	PASS
443	442	15	24	19.2	3096	PASS