

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102715\
 Data File : BE091056.D
 Acq On : 27 Oct 2015 19:35
 Operator : UM/NP
 Sample : G4075-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JG9J0

Manual Integrations
 APPROVED

MmDadoda
 10/28/2015 6:36:52 PM

Quant Time: Oct 28 09:28:34 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 28 03:57:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	5136	0.40	ng/ul	-0.02
4) Naphthalene-d8	9.57	136	28569	0.40	ng/ul	-0.02
8) Acenaphthene-d10	13.41	164	17924	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.14	188	36607m	0.40	ng/ul	0.00
18) Chrysene-d12	20.30	240	34780m	0.40	ng/ul	0.00
22) Perylene-d12	22.20	264	32982m	0.40	ng/ul	0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.90	96	34049	9.22	ng/uL	-0.08
6) 2-Methylnaphthalene-d10	11.07	152	14397	0.37	ng/ul	-0.02
16) Fluoranthene-d10	18.13	212	36049	0.35	ng/ul	0.00
Target Compounds						
21) Chrysene	20.33	228	12224m	0.12	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE102715\
Data File : BE091056.D
Acq On : 27 Oct 2015 19:35
Operator : UM/NP
Sample : G4075-12
Misc :
ALS Vial : 7 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
JG9J0

Manual Integrations
APPROVED

MmDadoda
10/28/2015 6:36:52 PM

Quant Time: Oct 28 09:28:34 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 28 03:57:22 2015
Response via : Initial Calibration

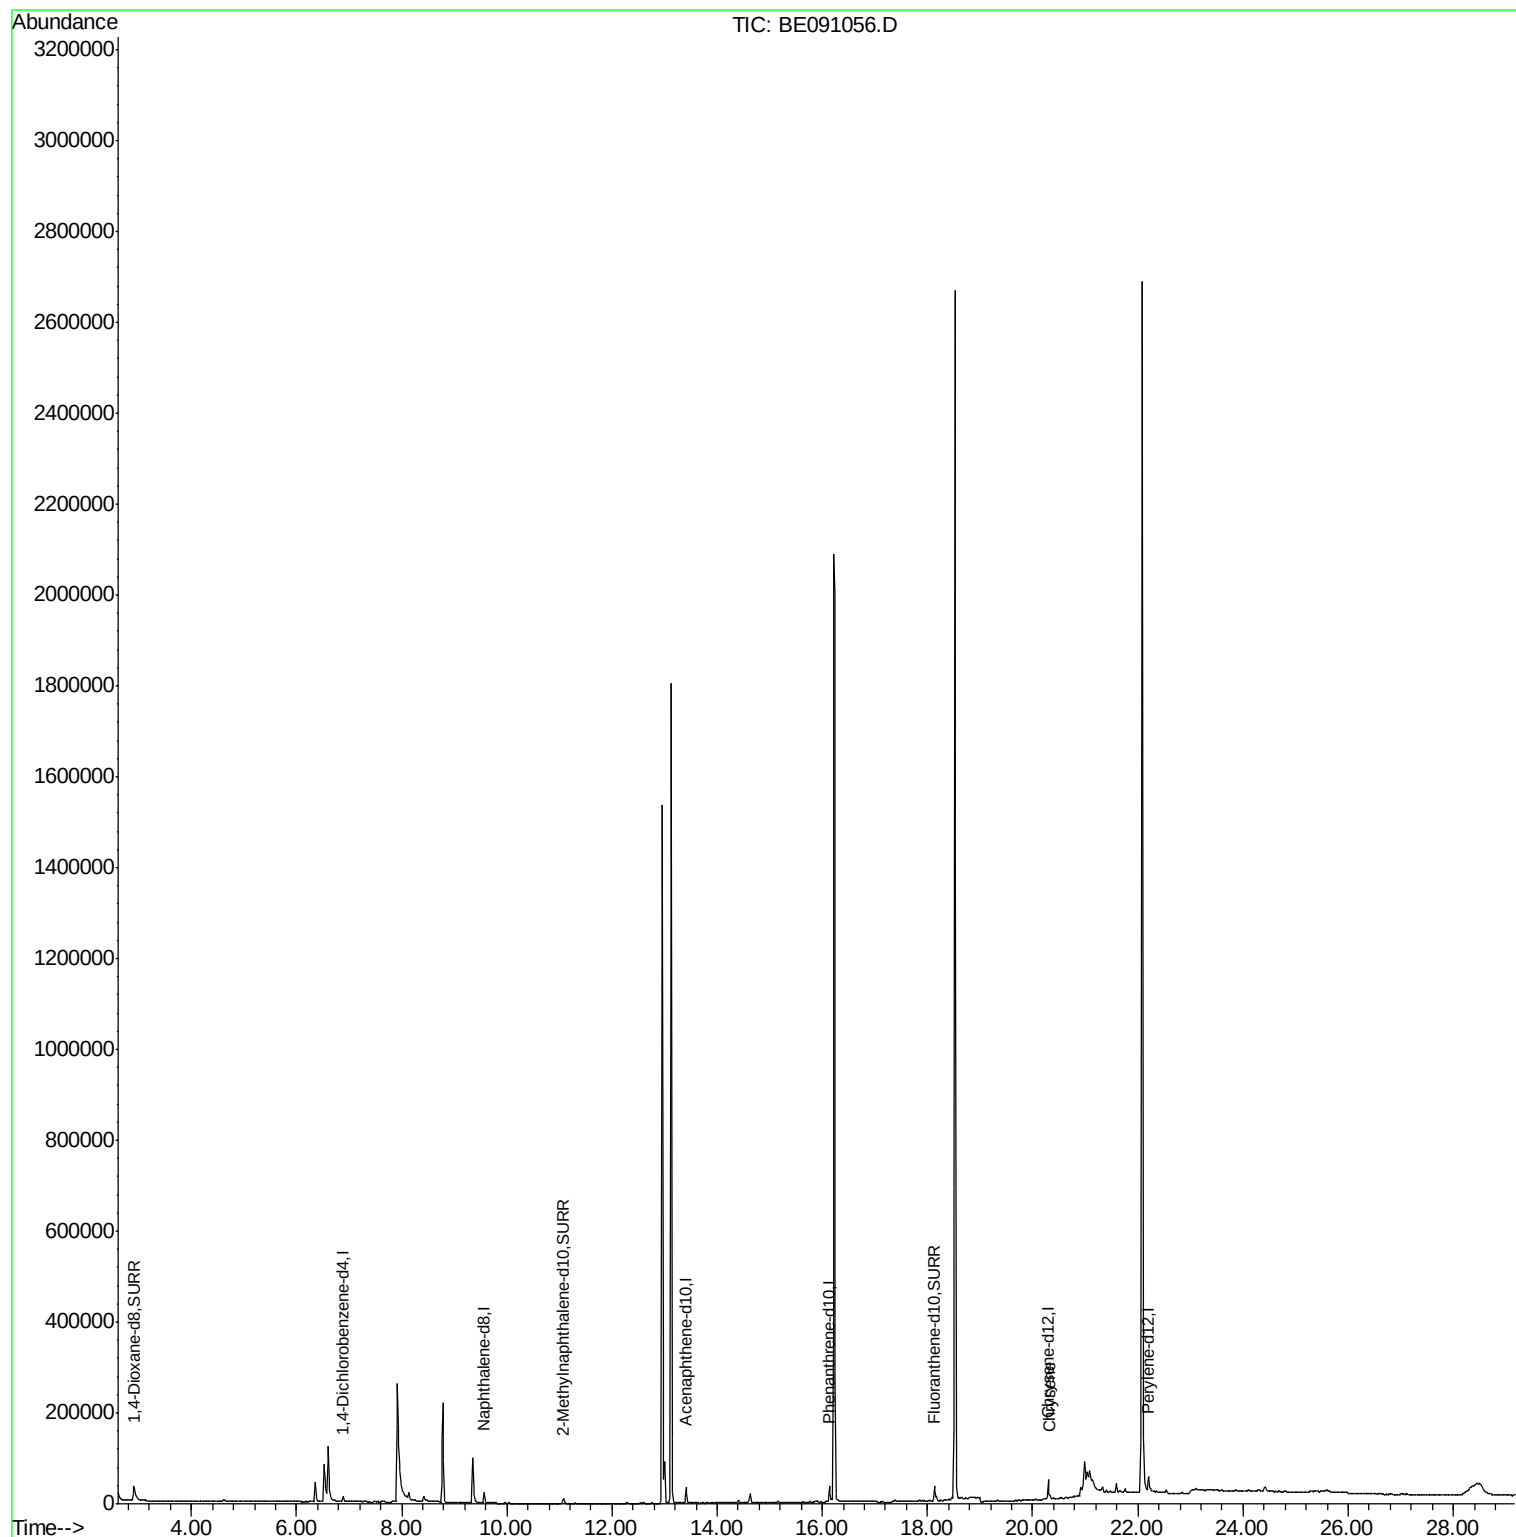

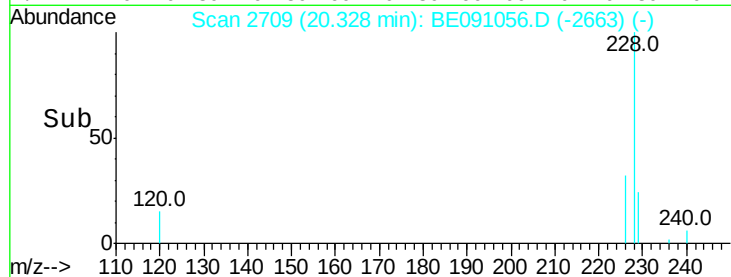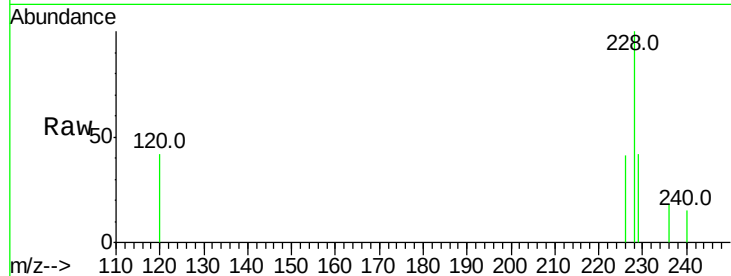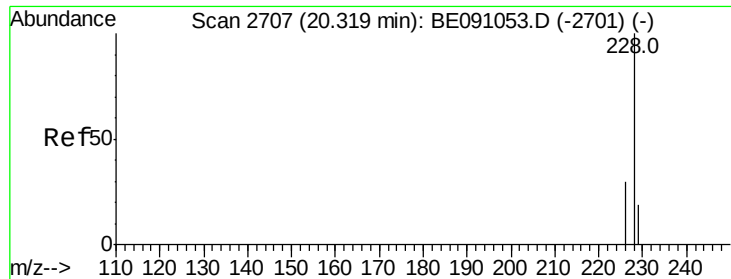

#21

Chrysene

Concen: 0.12 ng/ul m

RT: 20.33 min Scan# 2709

Delta R.T. 0.01 min

Lab File: BE091056.D

Acq: 27 Oct 2015 19:35

Instrument :

BNA_E

ClientSampleId :

JG9J0

Tot Ion:	228	Resp:	12224
Ion Ratio	Lower	Upper	
228	100		
226	41.4	25.7	38.5#
229	42.1	15.2	22.8#

Manual Integrations
APPROVED

MmDadoda
10/28/2015 6:36:52 PM

