

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094601.D
 Acq On : 27 Oct 2017 18:16
 Operator : SJ/JU
 Sample : PB103508BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK09

Quant Time: Oct 30 01:11:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1145	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6811	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4026	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	8038	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	456845	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3125	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	7172	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	873	0.06	ng/ul#	28
17) Pyrene	19.65	202	1319	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103508BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Quant Time: Oct 30 01:11:39 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration




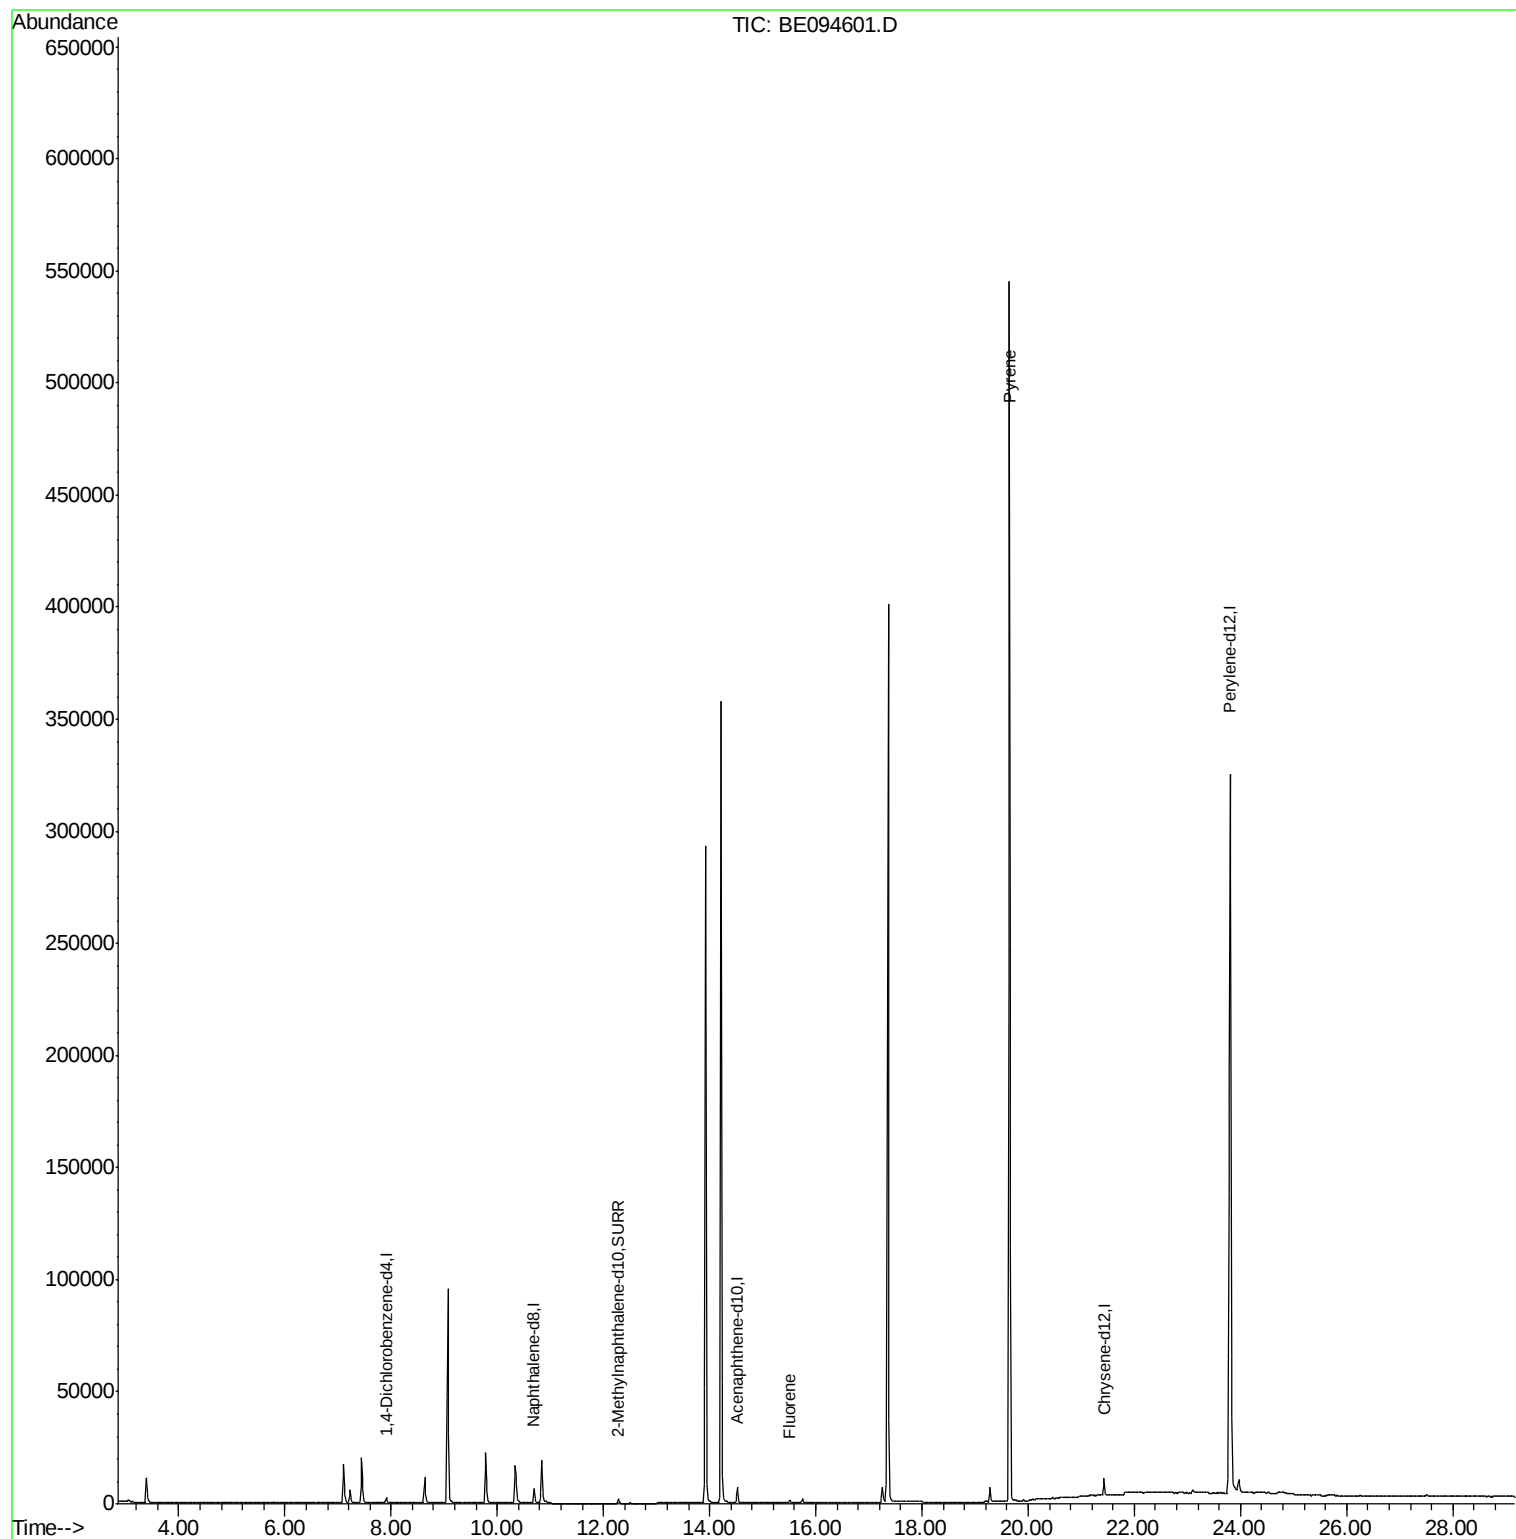


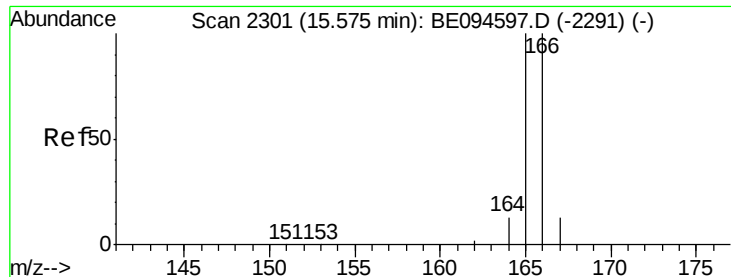

#9
Fluorene
 Concen: 0.06 ng/ul
 RT: 15.51 min Scan# 2293
 Delta R.T. -0.06 min
 Lab File: BE094601.D
 Acq: 27 Oct 2017 18:16

Instrument :
 BNA_E
 ClientSampleId :
 SBLK09

Tot Ion:166 Resp: 873
 Ion Ratio Lower Upper
 166 100
 165 18.5 73.4 110.2#
 167 39.2 14.6 22.0#

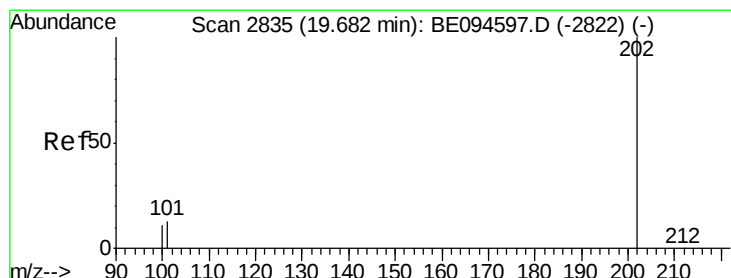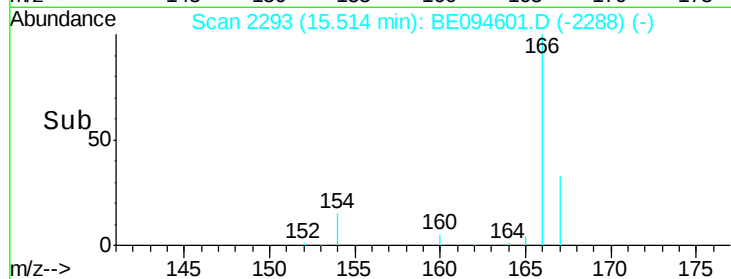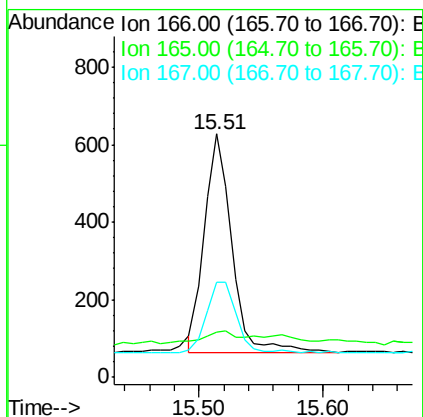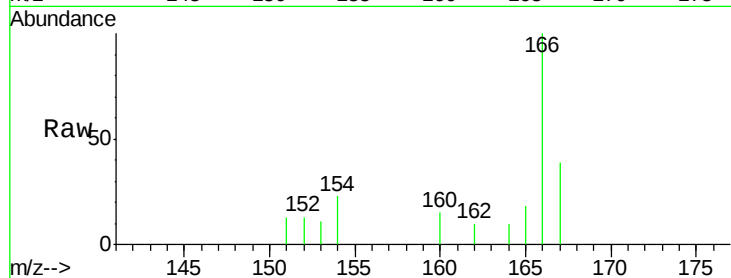

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.65 min Scan# 2828
 Delta R.T. -0.03 min
 Lab File: BE094601.D
 Acq: 27 Oct 2017 18:16

Tgt Ion:202 Resp: 1319
 Ion Ratio Lower Upper
 202 100
 101 120.7 18.2 27.4#
 100 566.0 15.6 23.4#

