

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094602.D
 Acq On : 27 Oct 2017 18:52
 Operator : SJ/JU
 Sample : I5842-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Quant Time: Oct 30 01:11:49 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1113	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6613	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	3837	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	7849	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	433877	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2536	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	6845	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.65	202	1135	0.05	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094602.D
Acq On : 27 Oct 2017 18:52
Operator : SJ/JU
Sample : I5842-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Quant Time: Oct 30 01:11:49 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

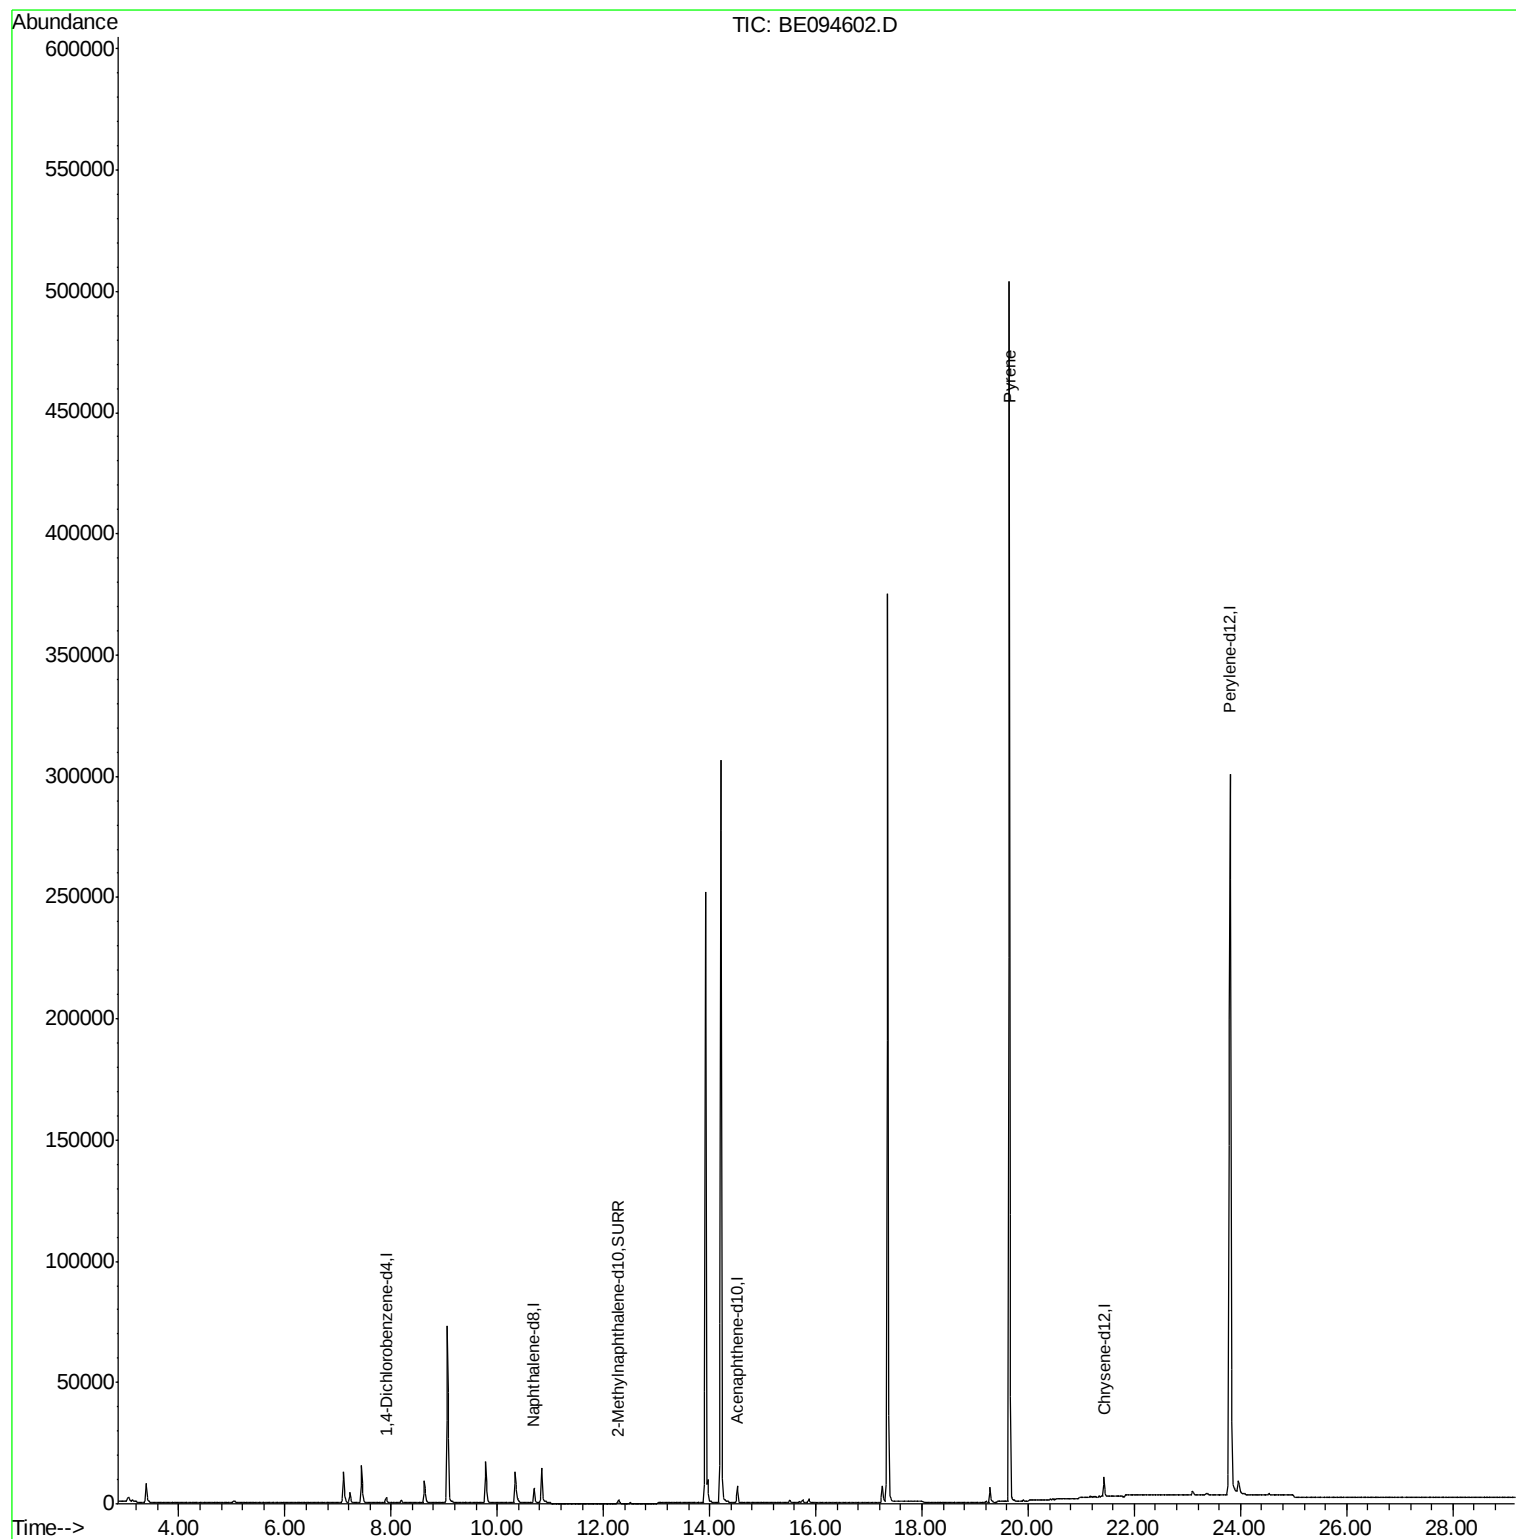

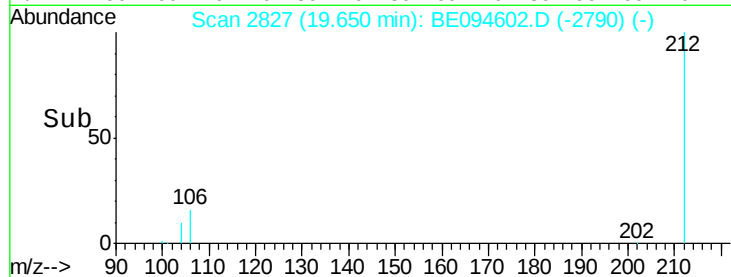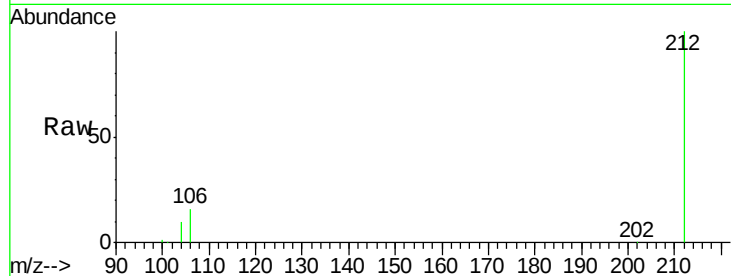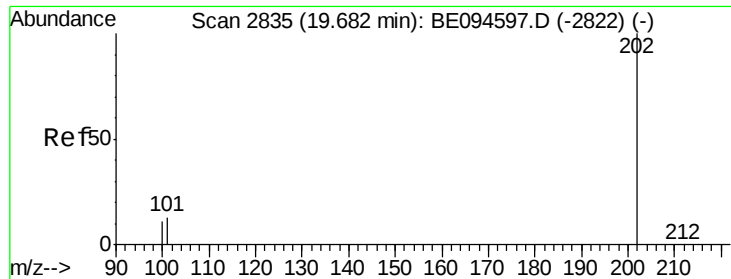

#17
 Pvrene
 Concen: 0.05 ng/ul
 RT: 19.65 min Scan# 2827
 Delta R.T. -0.03 min
 Lab File: BE094602.D
 Acq: 27 Oct 2017 18:52

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Tot Ion	Ratio	Lower	Upper
202	100		
101	128.3	18.2	27.4#
100	616.4	15.6	23.4#

