

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094604.D
 Acq On : 27 Oct 2017 20:07
 Operator : SJ/JU
 Sample : I5842-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Quant Time: Oct 30 01:12:01 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1106	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	6583	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	3829	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	7790	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	410525	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2565	0.24	ng/ul	-0.01
14) Fluoranthene-d10	19.29	212	6646	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.65	202	1087	0.05	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094604.D
Acq On : 27 Oct 2017 20:07
Operator : SJ/JU
Sample : I5842-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB6

Quant Time: Oct 30 01:12:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

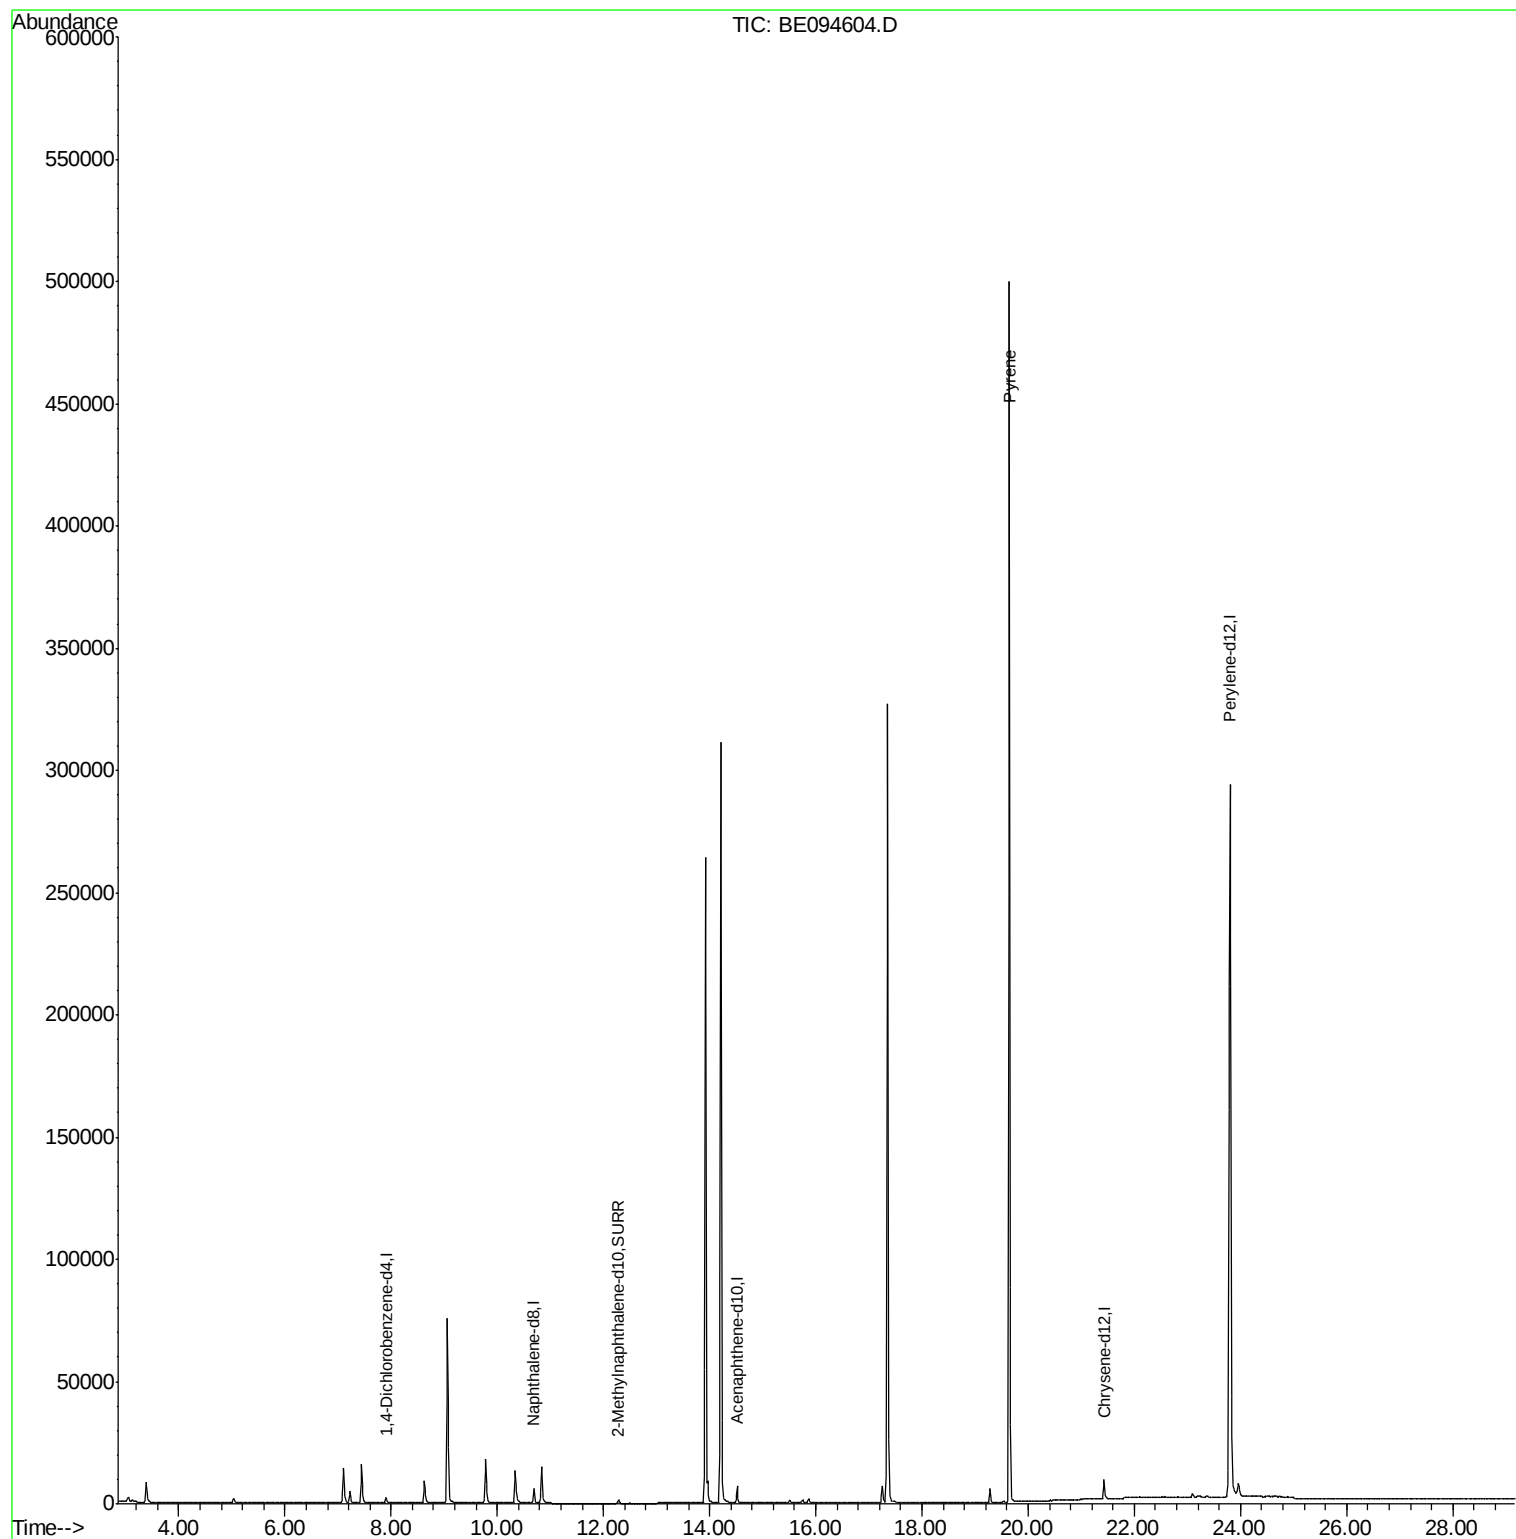

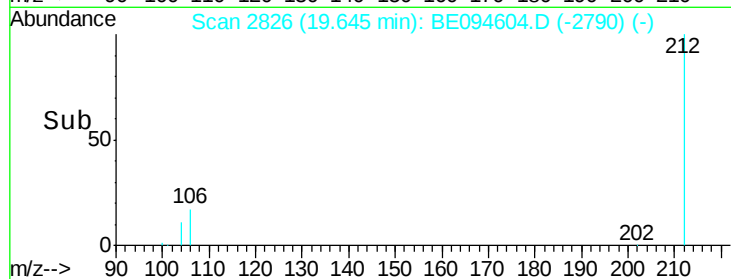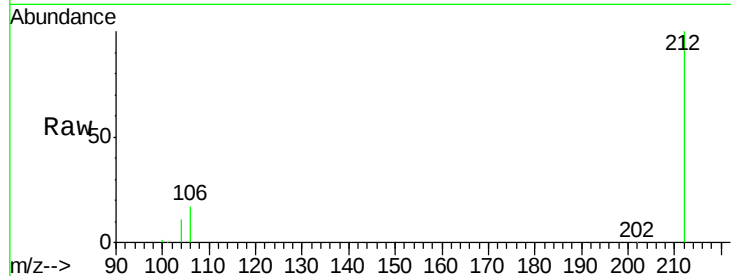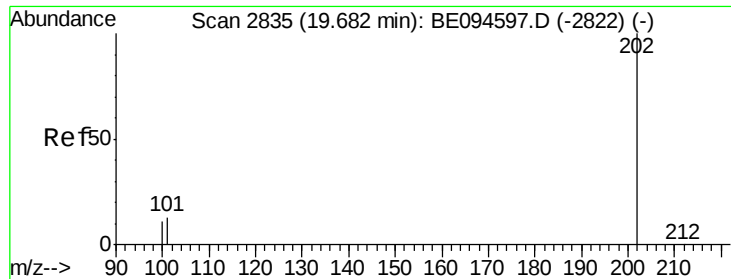

#17

Pvrene

Concen: 0.05 ng/ul

RT: 19.65 min Scan# 2826

Delta R.T. -0.04 min

Lab File: BE094604.D

Acq: 27 Oct 2017 20:07

Instrument :

BNA_E

ClientSampleId :

C0AB6

Tot Ion:202 Resp: 1087

Ion Ratio Lower Upper

202 100

101 141.0 18.2 27.4#

100 758.9 15.6 23.4#

