




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103509BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Manual Integrations
APPROVED

Sohil
10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:11:39 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

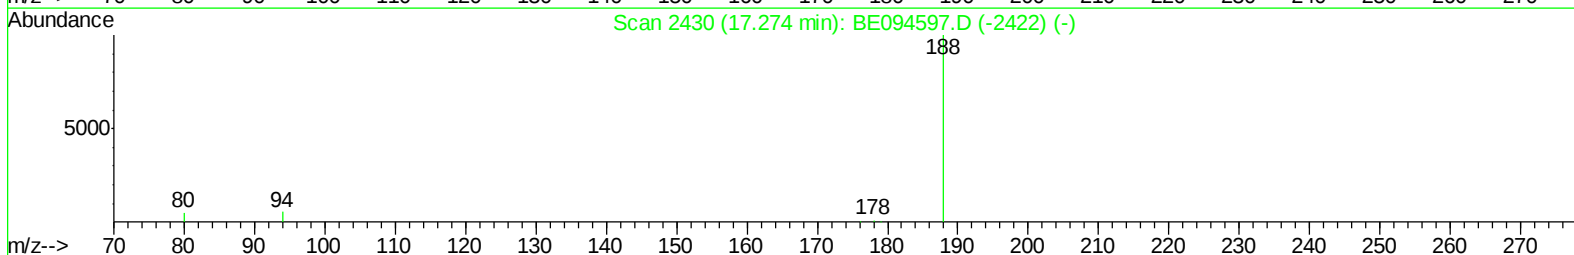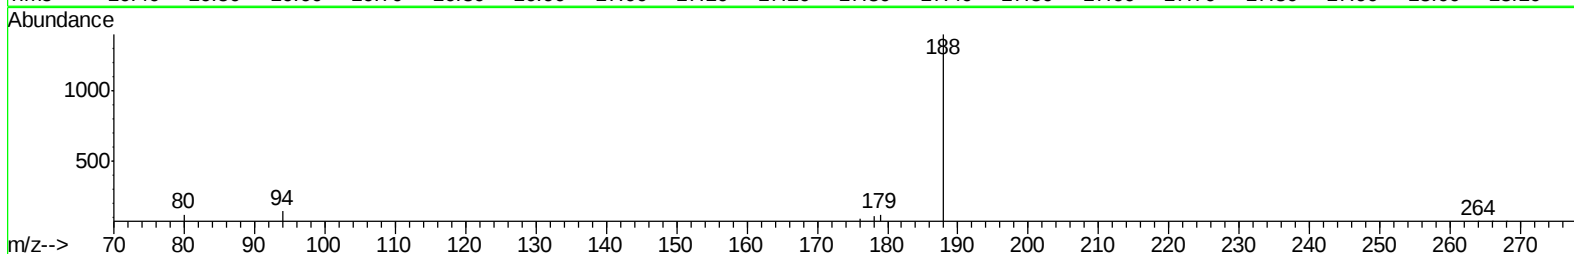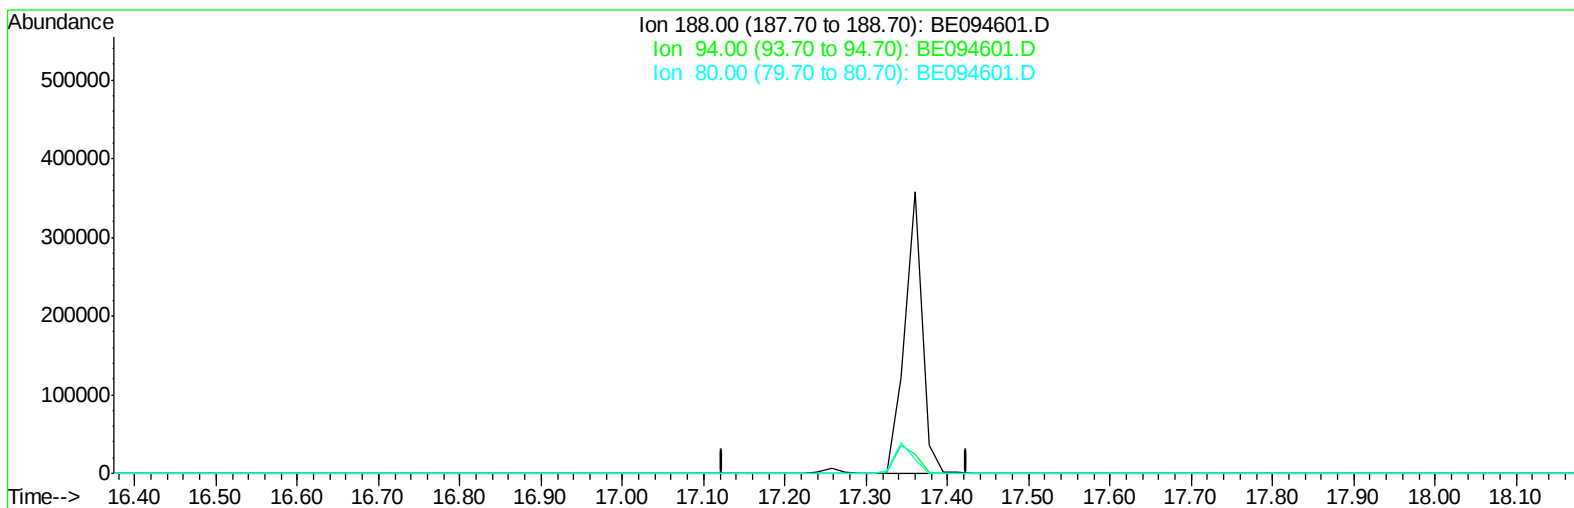

TIC: BE094601.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103509BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Manual Integrations
APPROVED

Sohil
10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:11:39 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

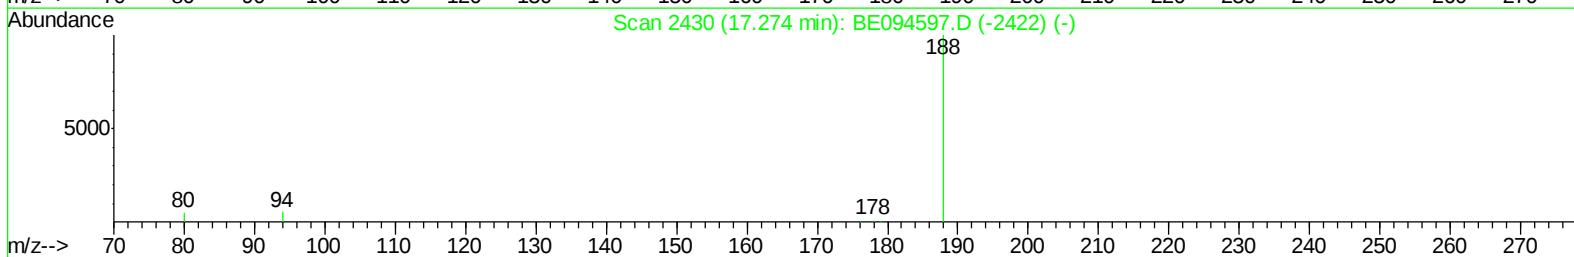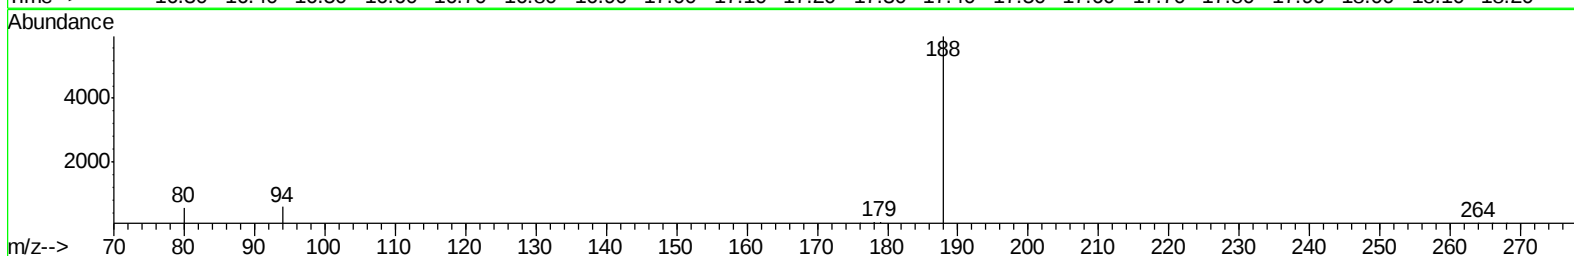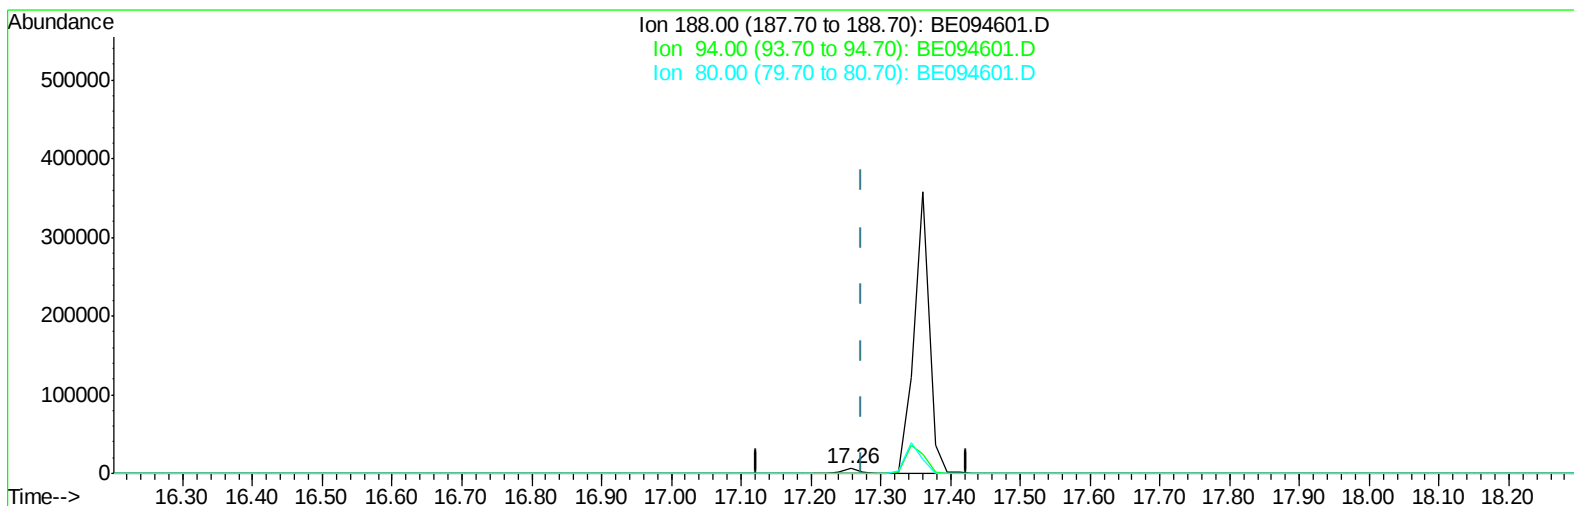

TIC: BE094601.D

(10) Phenanthrene-d10 (I)

17.257min (-0.017) 0.40ng/ul m

response 8545

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.03
80.00	11.80	9.43#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103509BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Manual Integrations
APPROVED

Sohil
10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:32:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

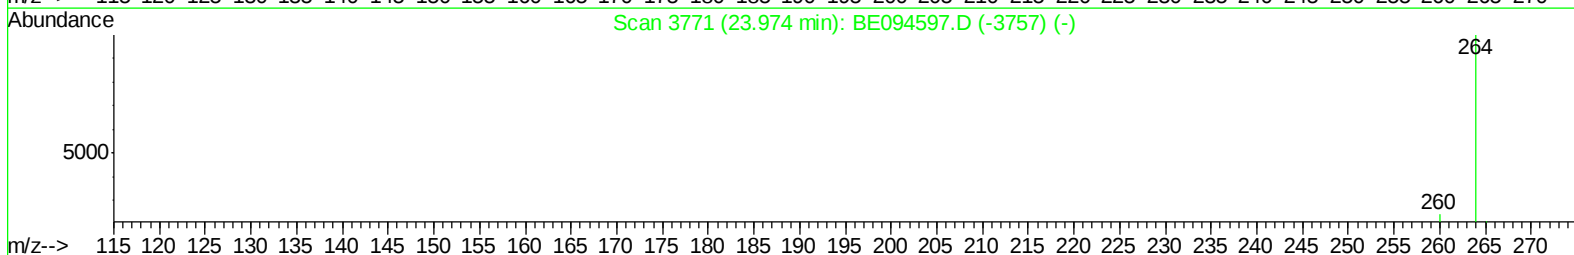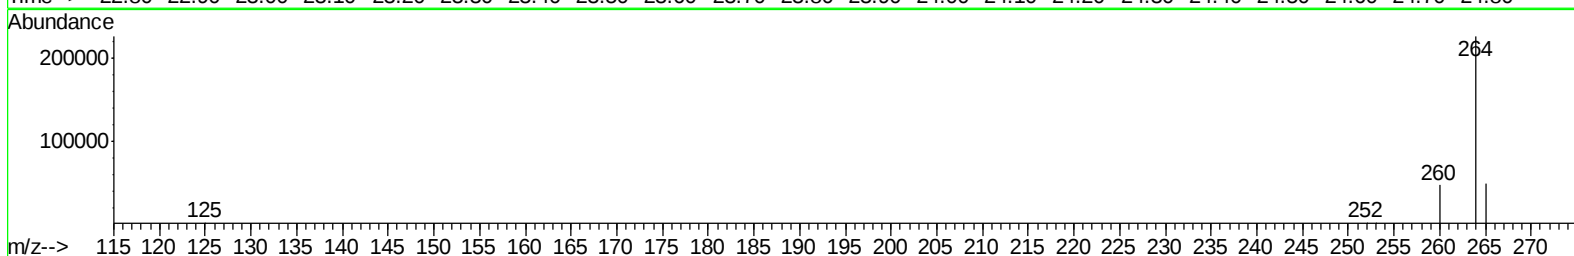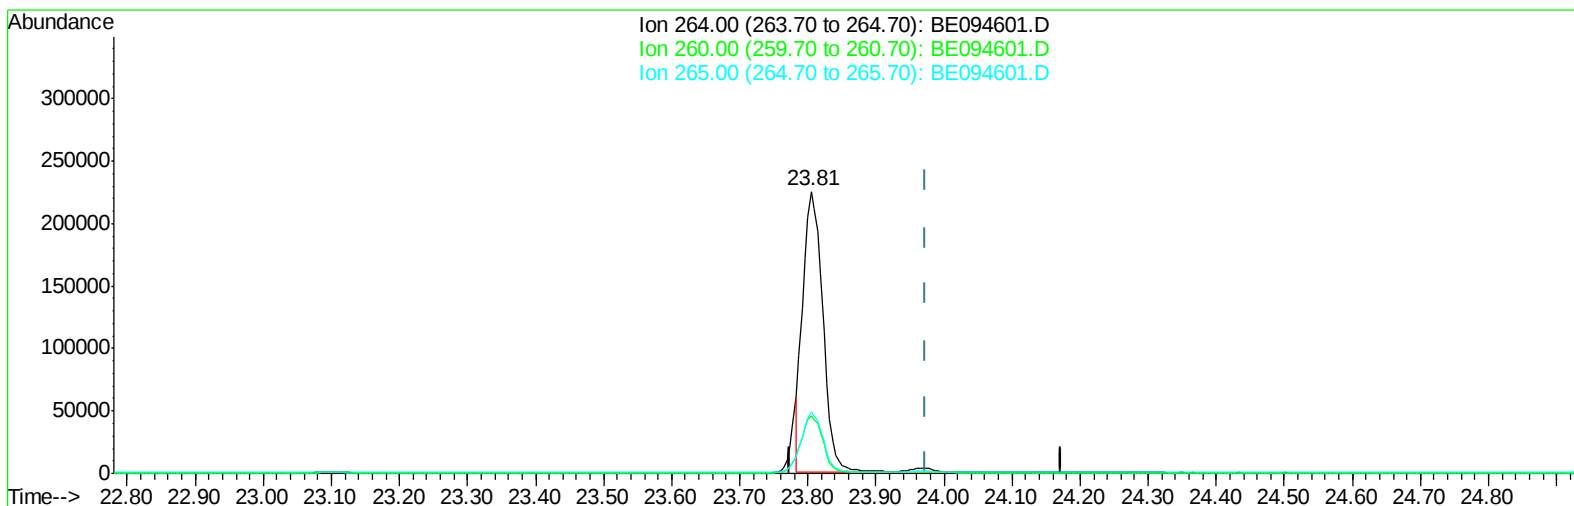

TIC: BE094601.D

(20) Perylene-d12 (I)

23.805min (-0.169) 0.40ng/ul

response 456845

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.67#
265.00	103.50	21.81#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103509BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Manual Integrations
APPROVED

Sohil
10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:32:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

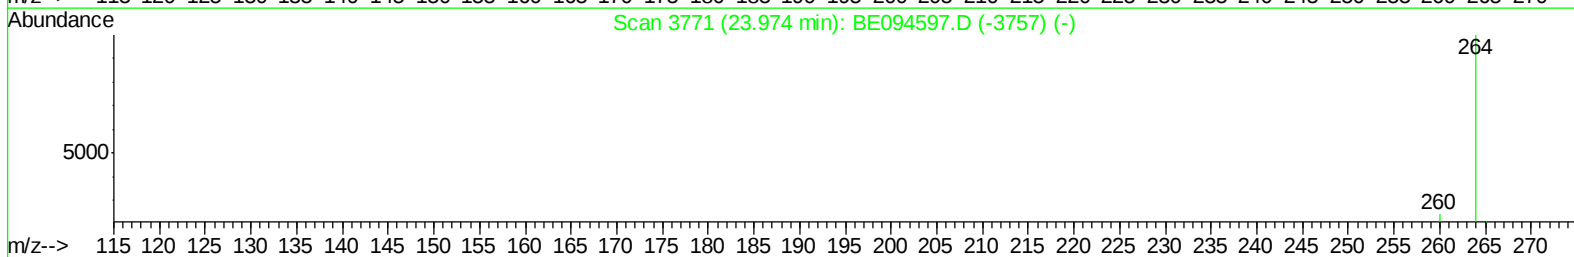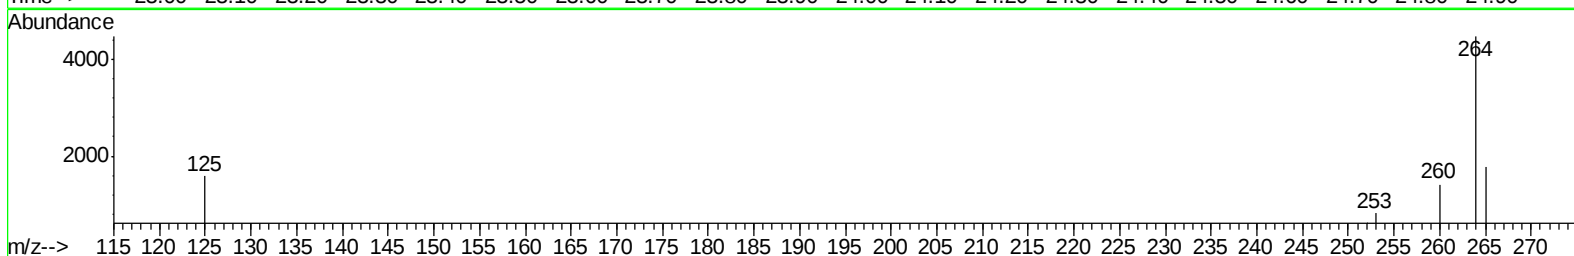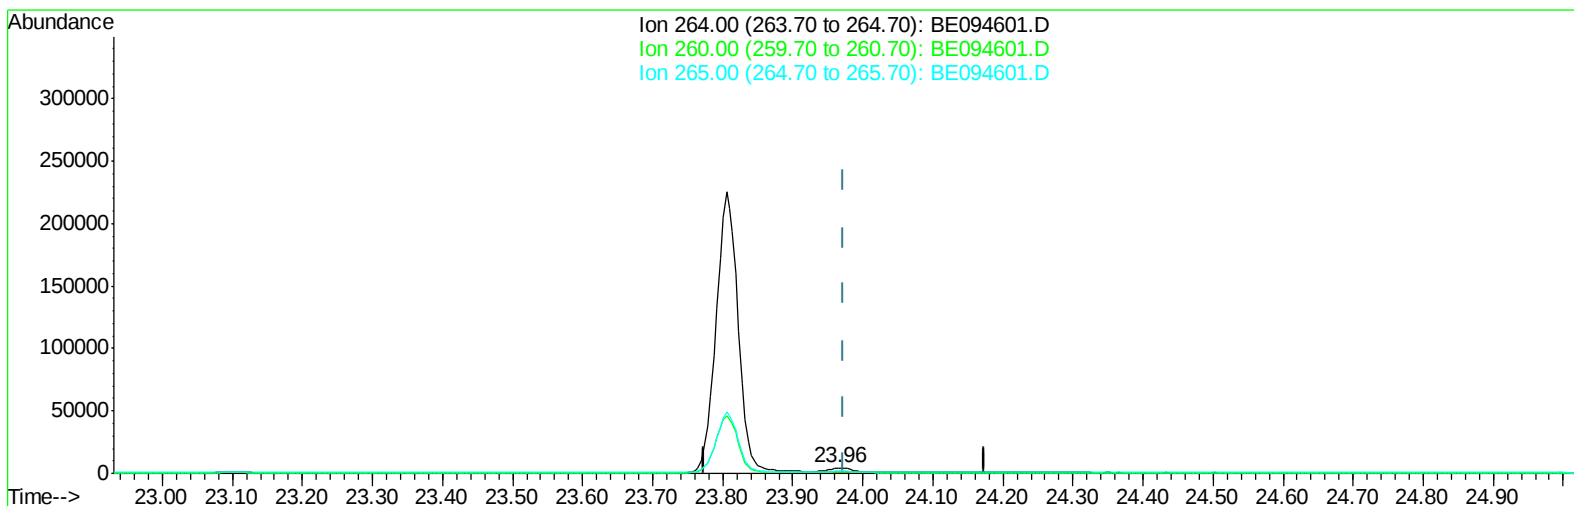

TIC: BE094601.D

(20) Perylene-d12 (I)

23.964min (-0.009) 0.40ng/ul m

response 8351

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	31.42
265.00	103.50	39.34#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094601.D
 Acq On : 27 Oct 2017 18:16
 Operator : SJ/JU
 Sample : PB103509BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK09

Manual Integrations
 APPROVED

Sohil
 10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:33:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1145	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6811	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4026	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8545m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	8038	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	8351m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3125	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	7172	0.28	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094601.D
Acq On : 27 Oct 2017 18:16
Operator : SJ/JU
Sample : PB103509BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK09

Manual Integrations
APPROVED

Sohil
10/30/2017 6:36:59 PM

Quant Time: Oct 30 01:33:24 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

