




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094602.D
Acq On : 27 Oct 2017 18:52
Operator : SJ/JU
Sample : I5842-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

Sohil
10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:11:49 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

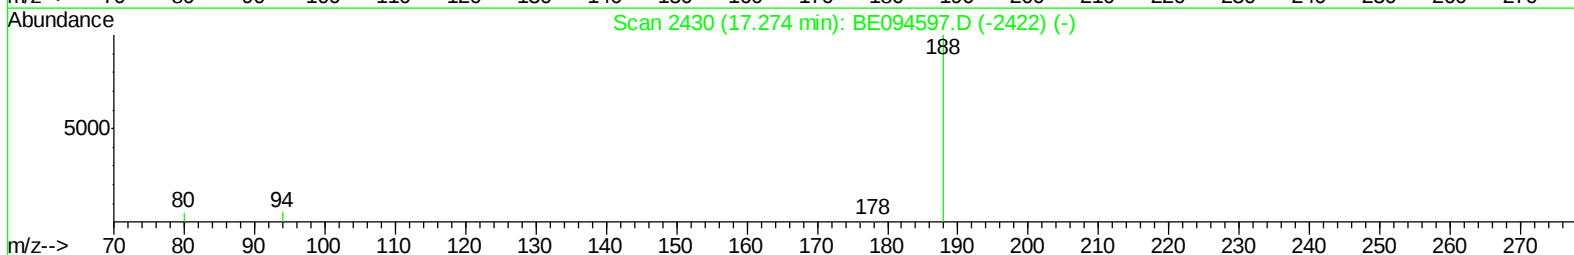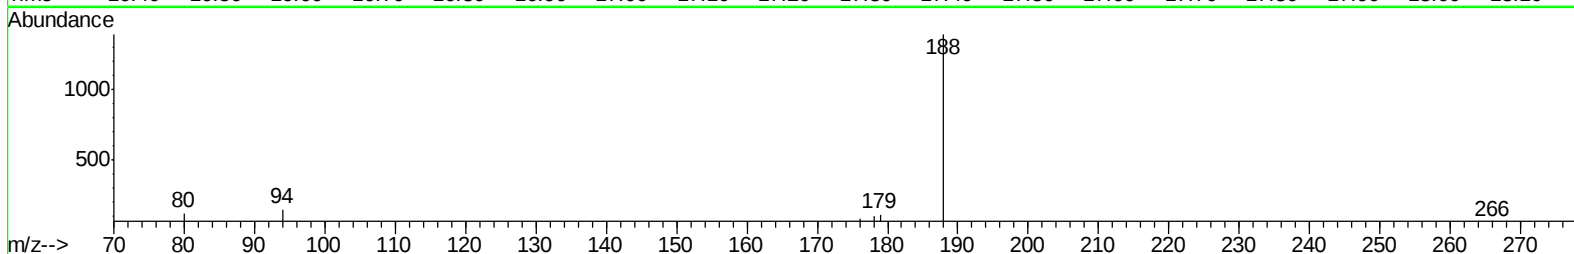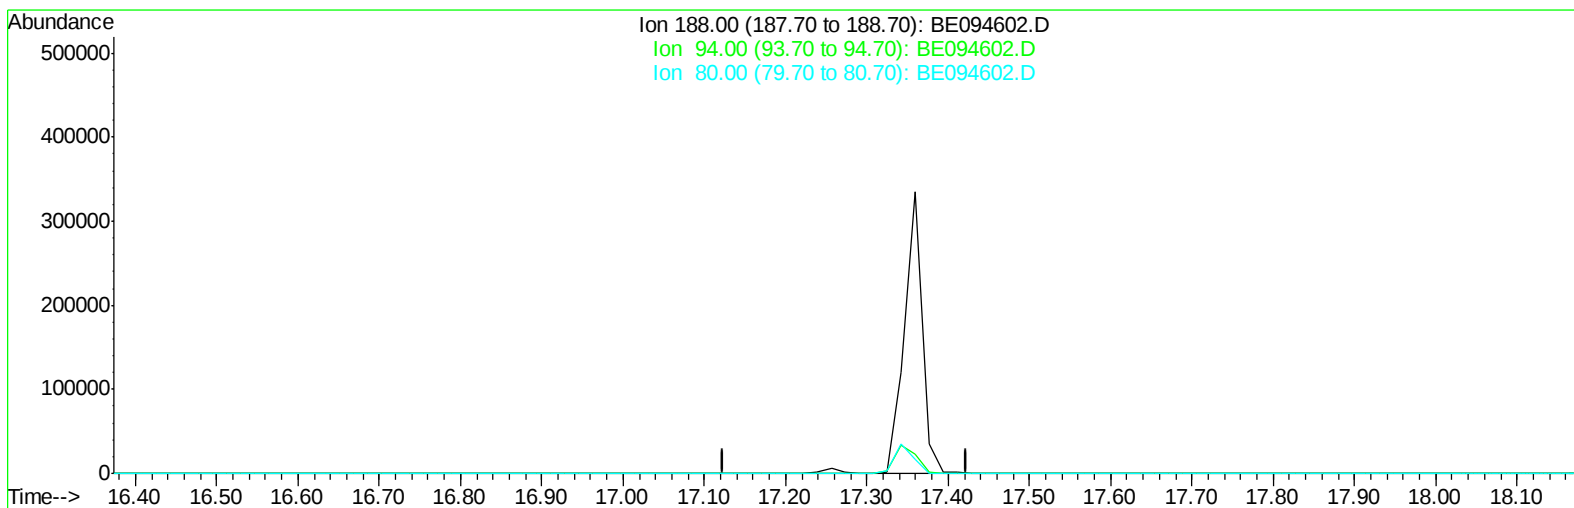

TIC: BE094602.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094602.D
 Acq On : 27 Oct 2017 18:52
 Operator : SJ/JU
 Sample : I5842-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

Sohil
 10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:11:49 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration

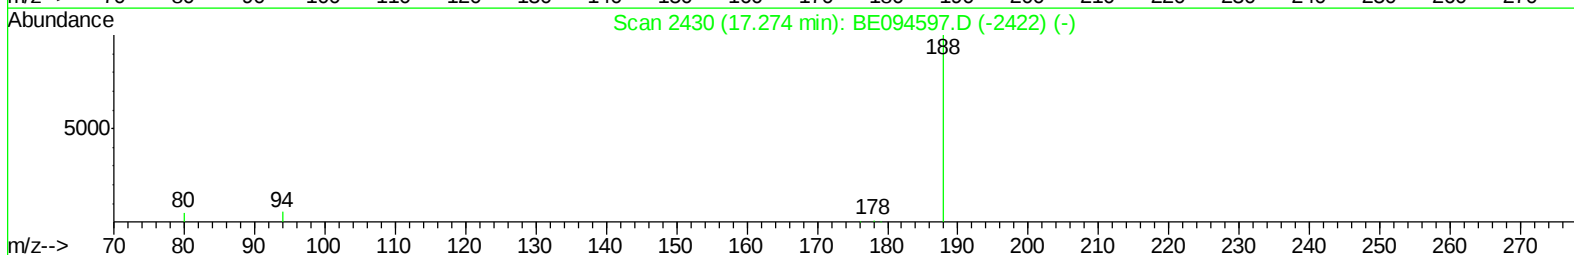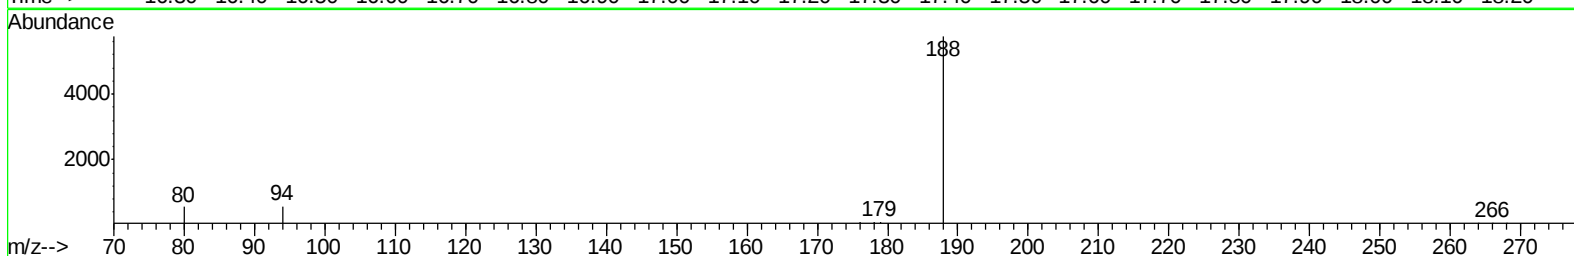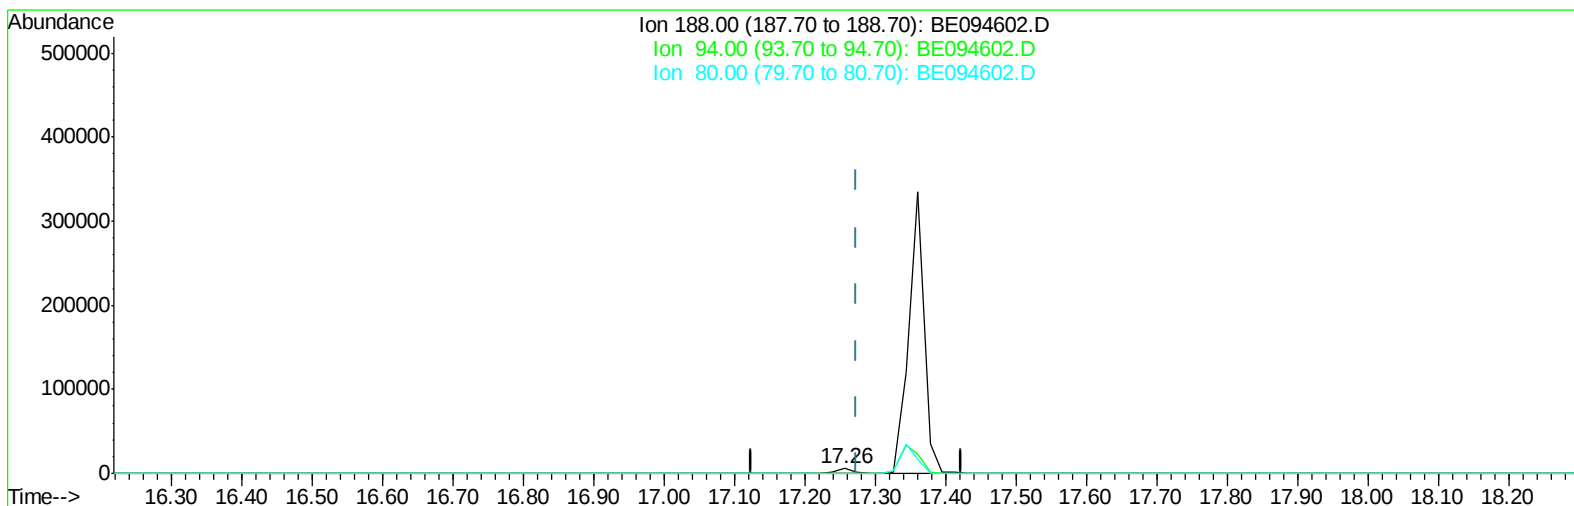

TIC: BE094602.D

(10) Phenanthrene-d10 (I)

17.256min (-0.017) 0.40ng/ul m

response 8554

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.84
80.00	11.80	9.82
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094602.D
Acq On : 27 Oct 2017 18:52
Operator : SJ/JU
Sample : I5842-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

Sohil
10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:38:11 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

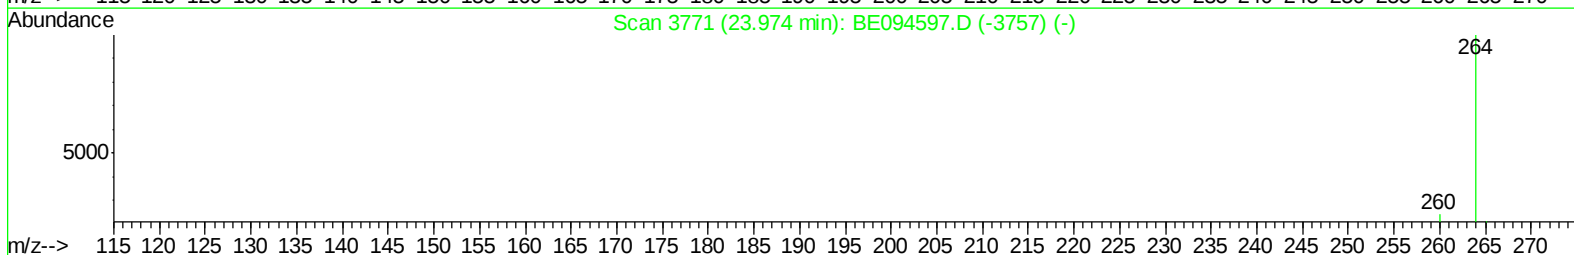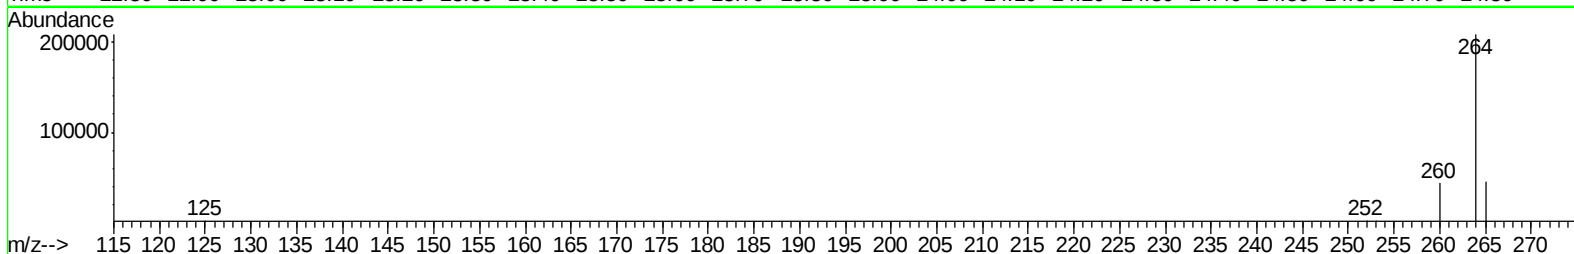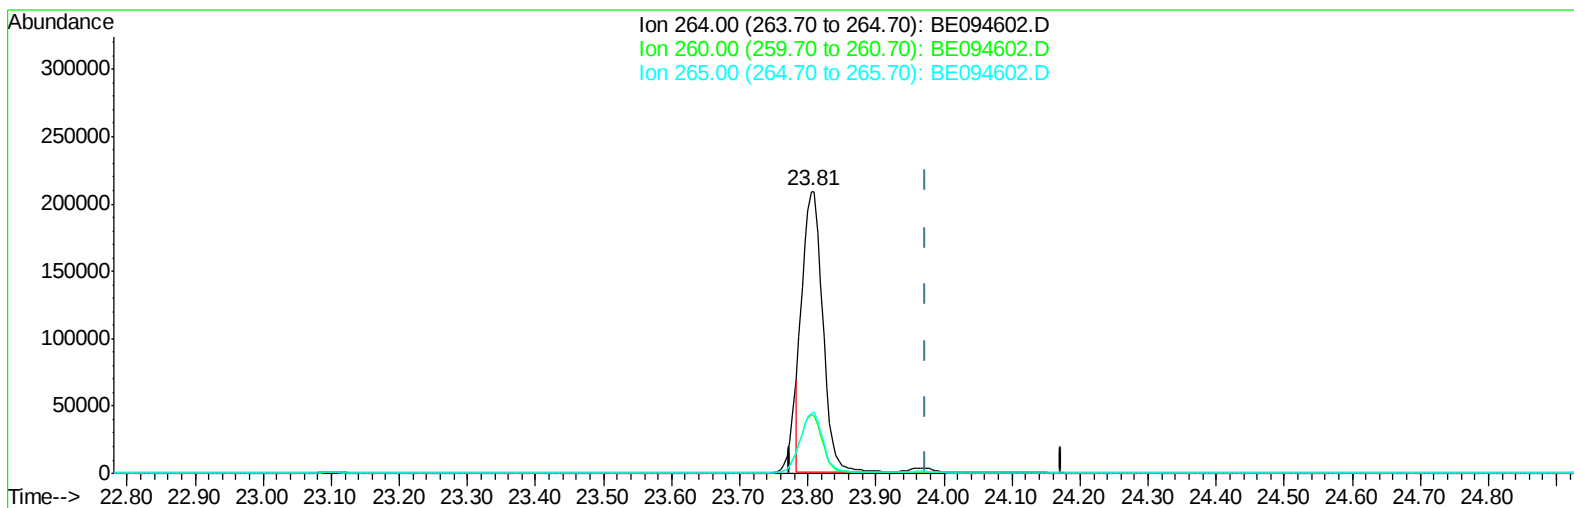

TIC: BE094602.D

(20) Perylene-d12 (I)

23.805min (-0.169) 0.40ng/ul

response 433877

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.76#
265.00	103.50	21.52#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094602.D
Acq On : 27 Oct 2017 18:52
Operator : SJ/JU
Sample : I5842-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

Sohil
10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:38:11 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

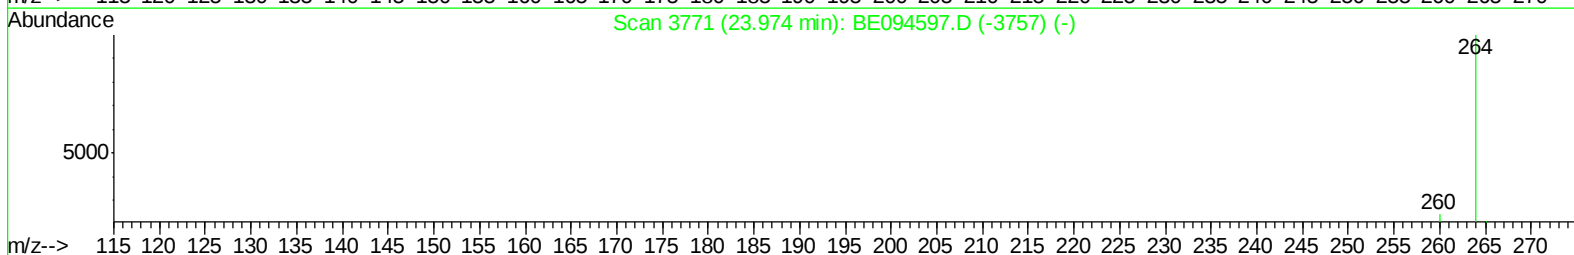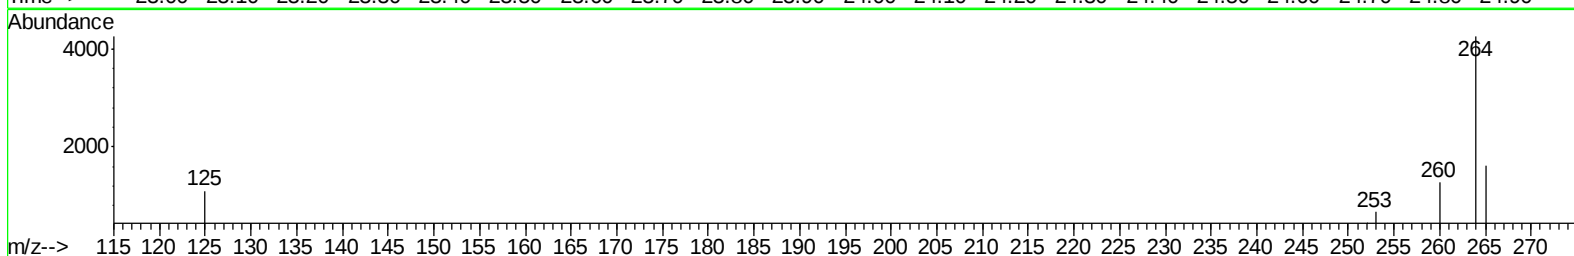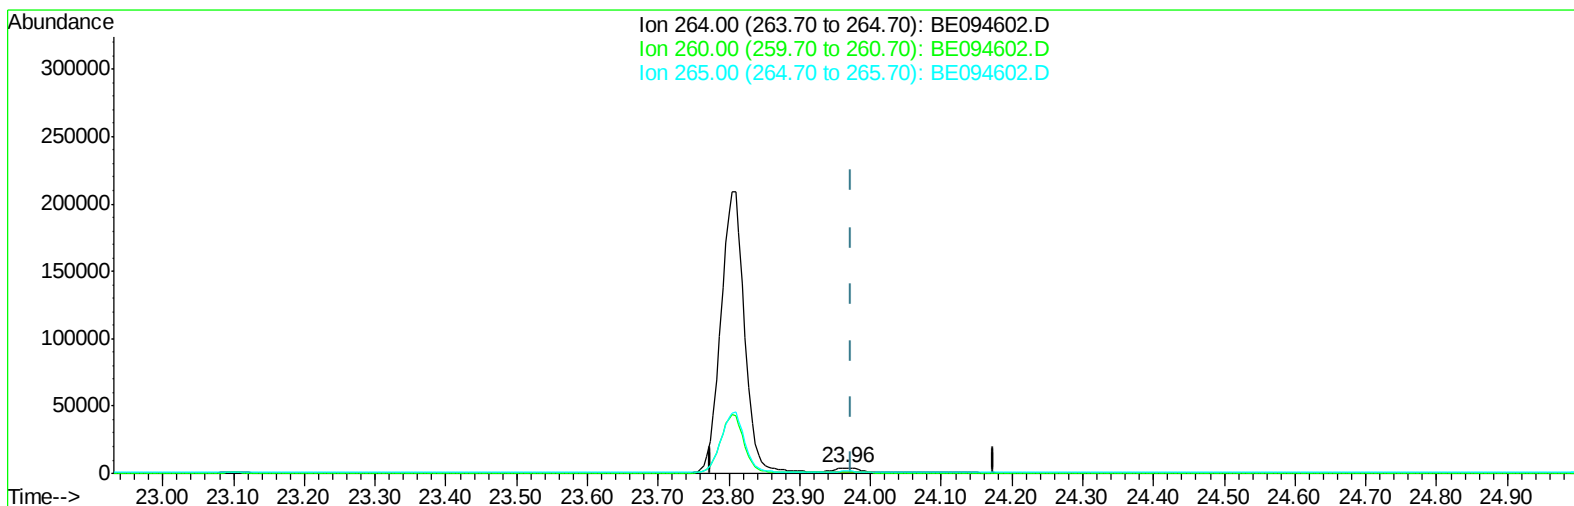

TIC: BE094602.D

(20) Perylene-d12 (I)

23.964min (-0.009) 0.40ng/ul m

response 8091

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	29.90
265.00	103.50	37.92#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
 Data File : BE094602.D
 Acq On : 27 Oct 2017 18:52
 Operator : SJ/JU
 Sample : I5842-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

Sohil
 10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:39:21 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 30 01:11:00 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1113	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6613	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	3837	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8554m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.43	240	7849	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	8091m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	2536	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	6845	0.27	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102717\
Data File : BE094602.D
Acq On : 27 Oct 2017 18:52
Operator : SJ/JU
Sample : I5842-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

Sohil
10/30/2017 6:37:01 PM

Quant Time: Oct 30 01:39:21 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 01:11:00 2017
Response via : Initial Calibration

