


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE102819\
 Data File : BE100674.D
 Acq On : 28 Oct 2019 15:25
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 23 16:49:33 2019

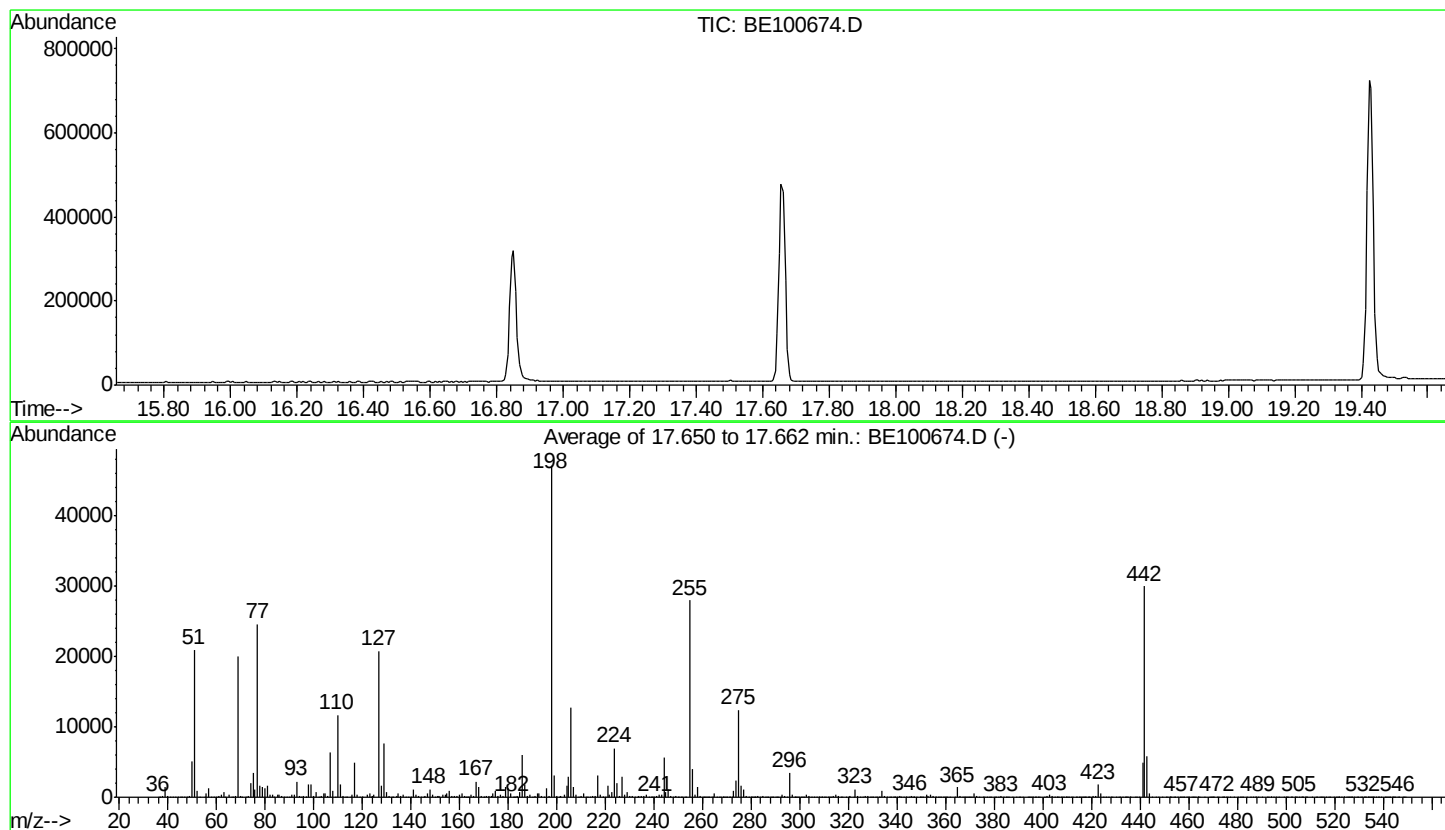

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	20934	PASS
68	69	0.00	2	1.0	209	PASS
69	198	0.00	100	42.4	19977	PASS
70	69	0.00	2	0.6	124	PASS
127	198	10	80	44.0	20759	PASS
197	198	0.00	2	0.3	125	PASS
198	198	100	100	100.0	47136	PASS
199	198	5	9	6.7	3163	PASS
275	198	10	60	26.4	12443	PASS
365	198	1	100	2.9	1386	PASS
441	198	0.01	100	10.4	4924	PASS
442	198	50	100	63.7	30013	PASS
443	442	15	24	19.3	5783	PASS