
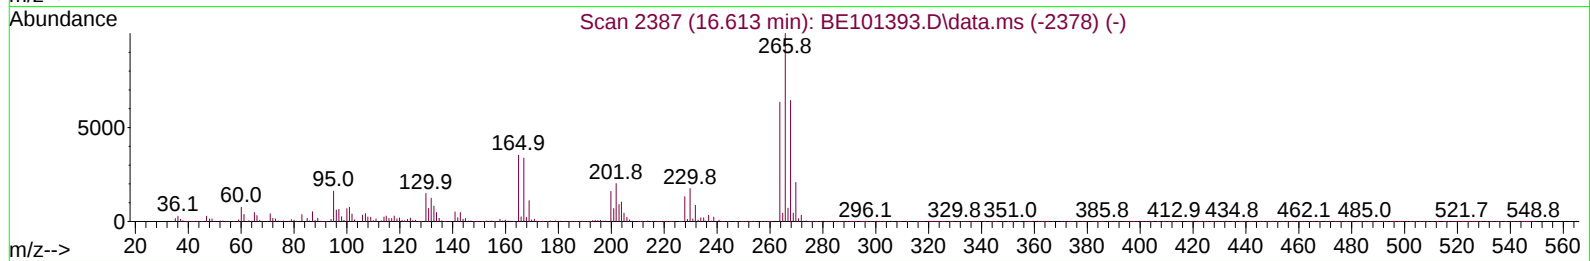
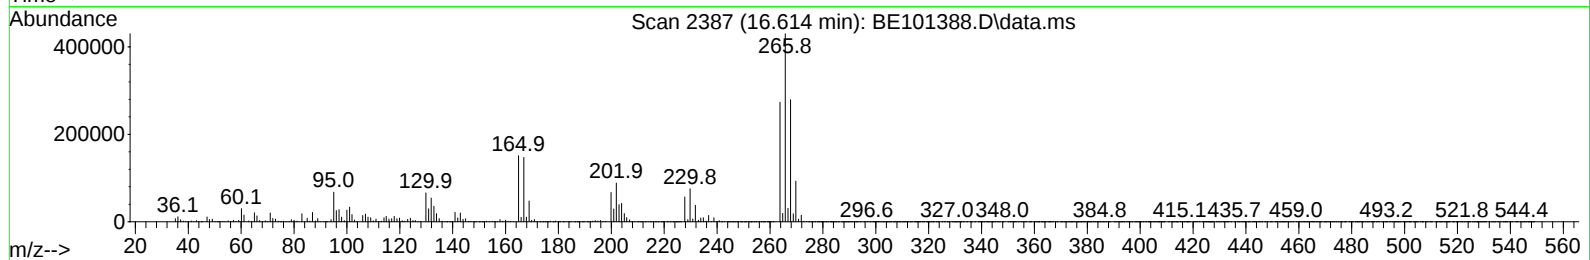


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101388.D
Acq On : 28 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

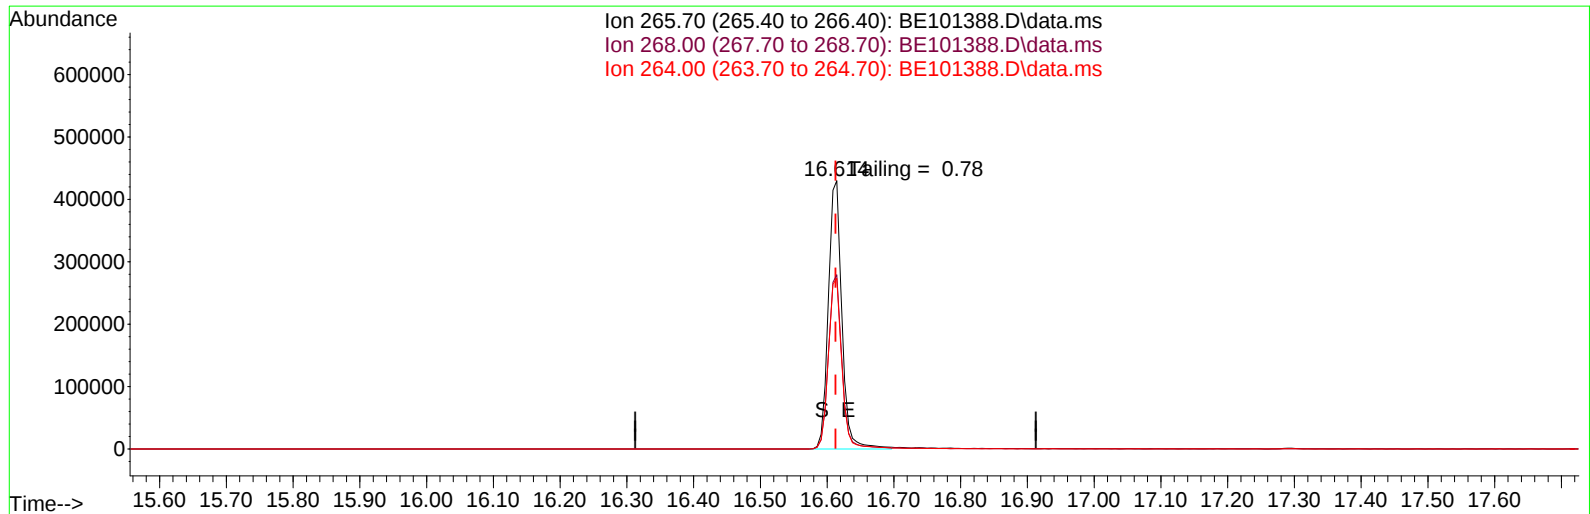

TIC: BE101388.D\data.ms

(70) Pentachlorophenol (C)




16.614min (+ 0.002) 1241130.64 ng

response 610726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.96
264.00	63.40	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE102824\
Data File : BE101388.D
Acq On : 28 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:32:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

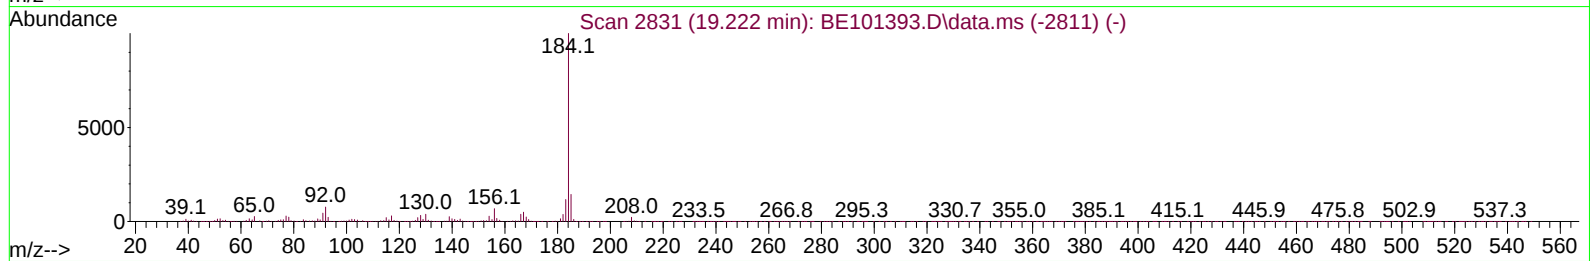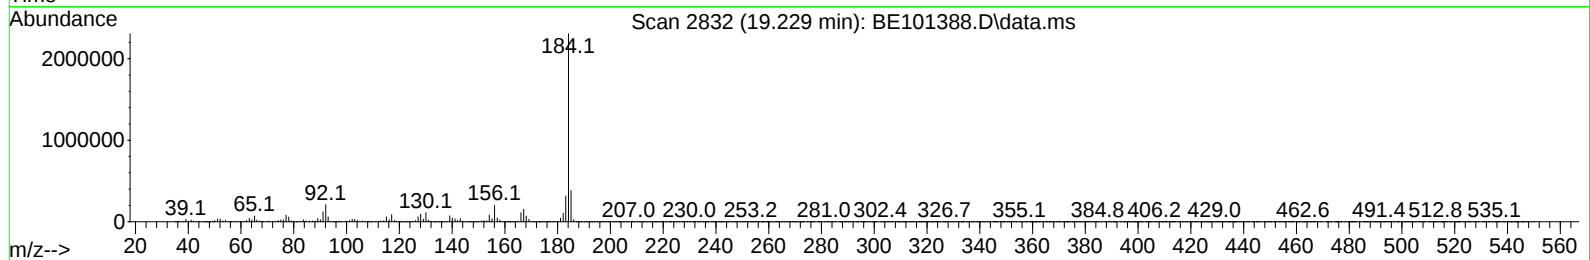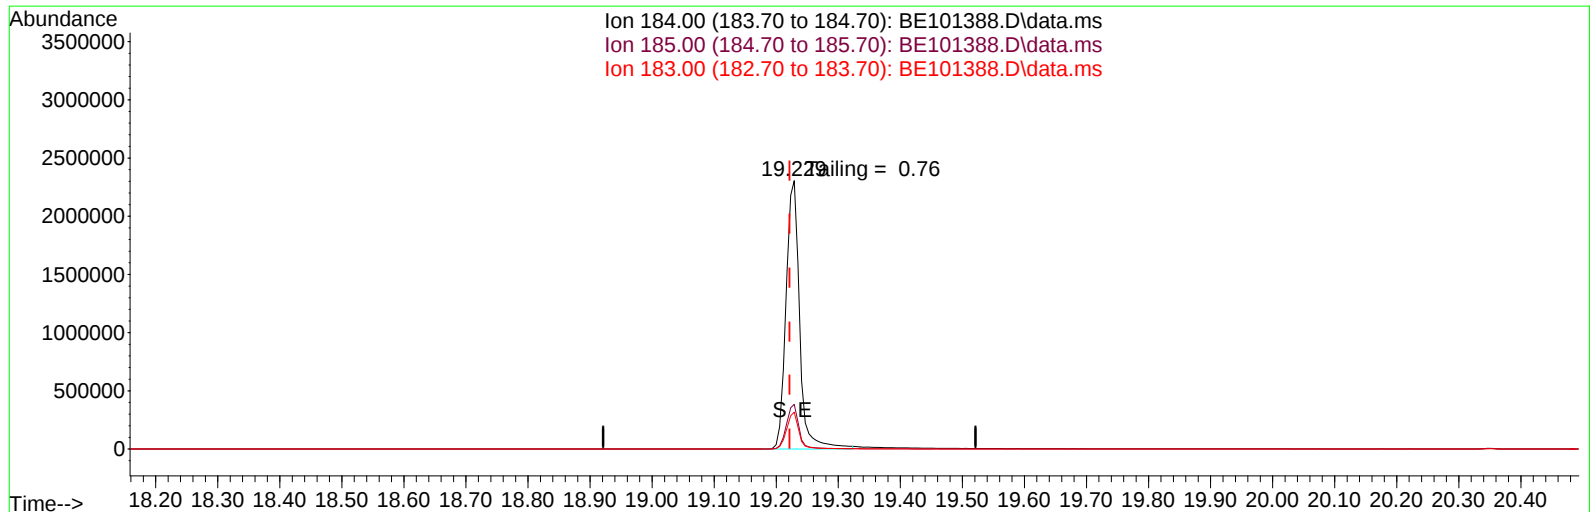

TIC: BE101388.D\data.ms

(77) Benzidine**19.229min (+ 0.008) 277076.80 ng****response 3629102**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	16.64
183.00	11.60	13.72
0.00	0.00	0.00