
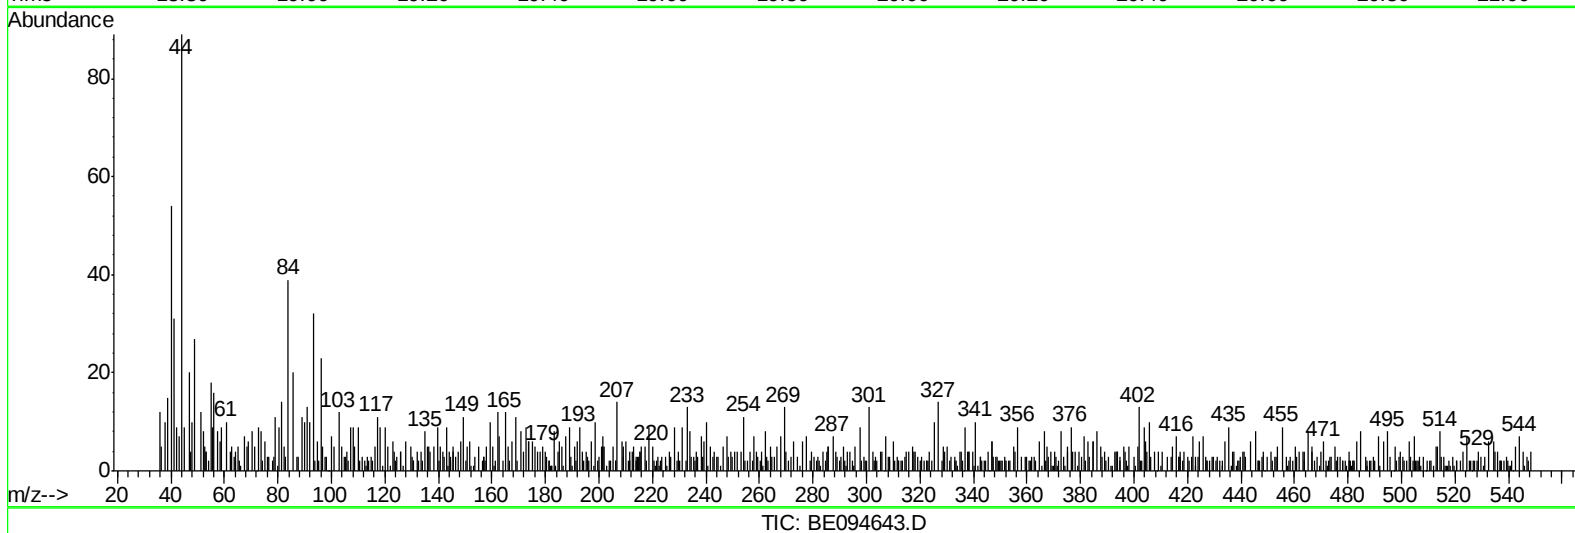


Data Path : Z:\HPCHEM1\BNA E\DATA\BE103017\  
Data File : BE094643.D  
Acq On : 30 Oct 2017 13:04  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 01:53:53 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 27 15:58:57 2017  
Response via : Initial Calibration

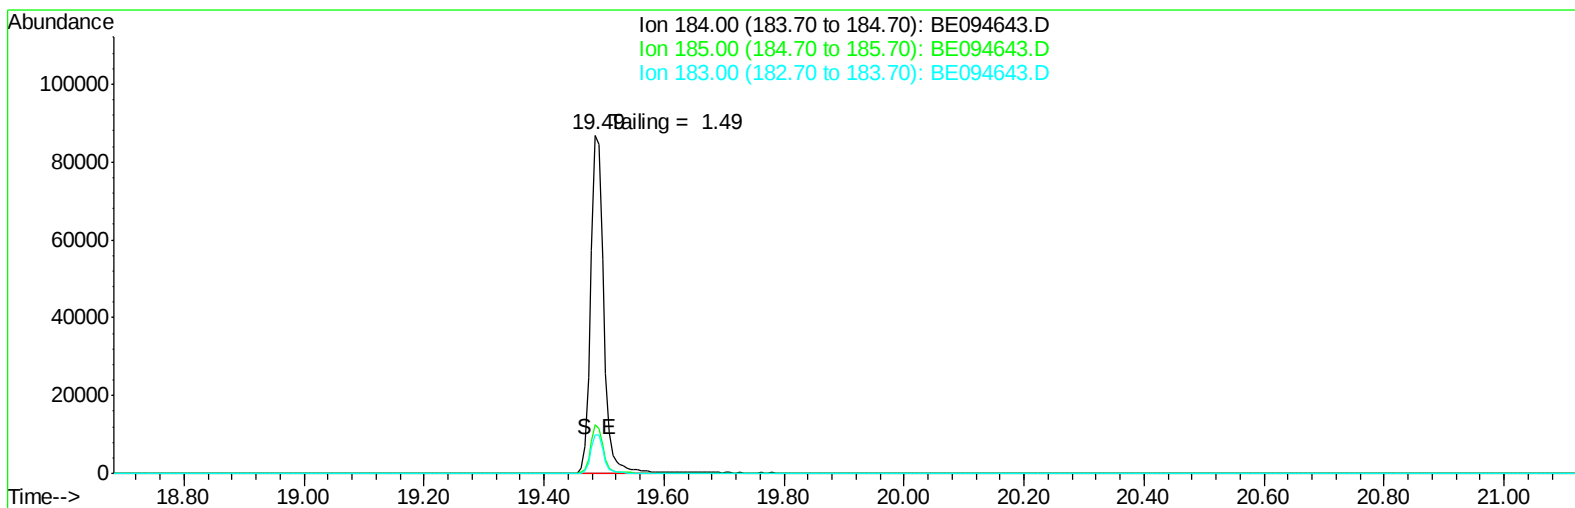

TIC: BE094643.D

(76) Benzidine



12.646min (-0.028) 22.85ng

response 4

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 184.00 | 100   | 100     |
| 185.00 | 15.70 | 120.00# |
| 183.00 | 11.60 | 160.00# |
| 0.00   | 0.00  | 0.00    |

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103017\  
Data File : BE094643.D  
Acq On : 30 Oct 2017 13:04  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 01:53:53 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 27 15:58:57 2017  
Response via : Initial Calibration

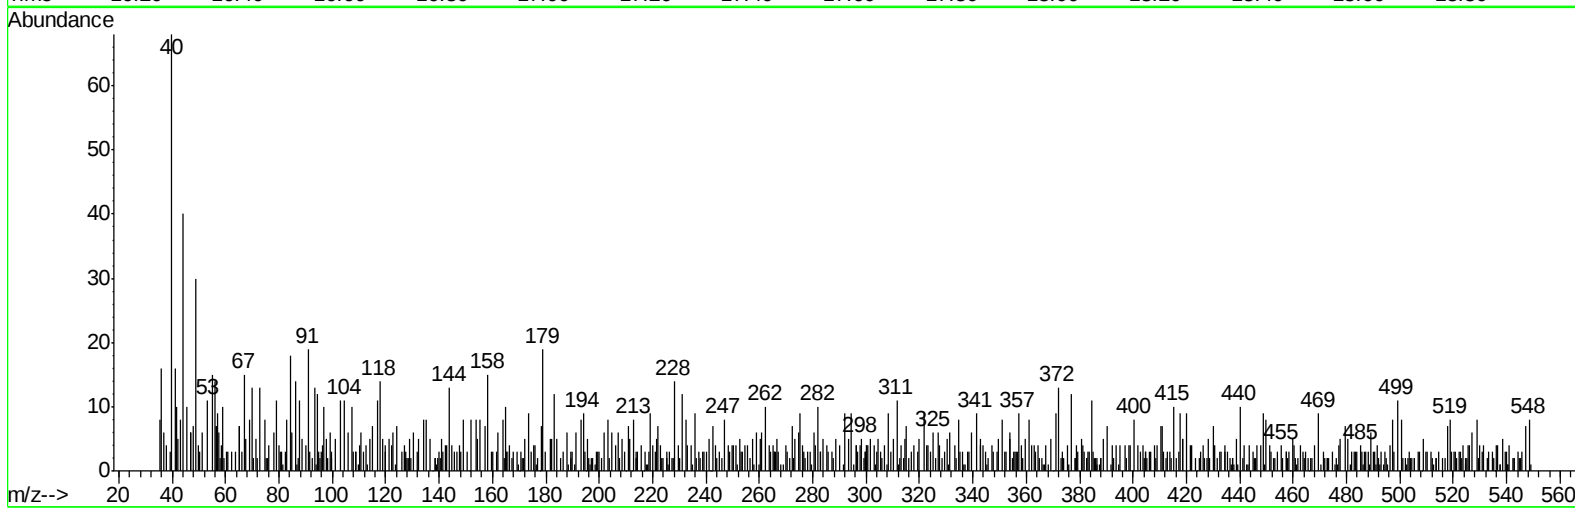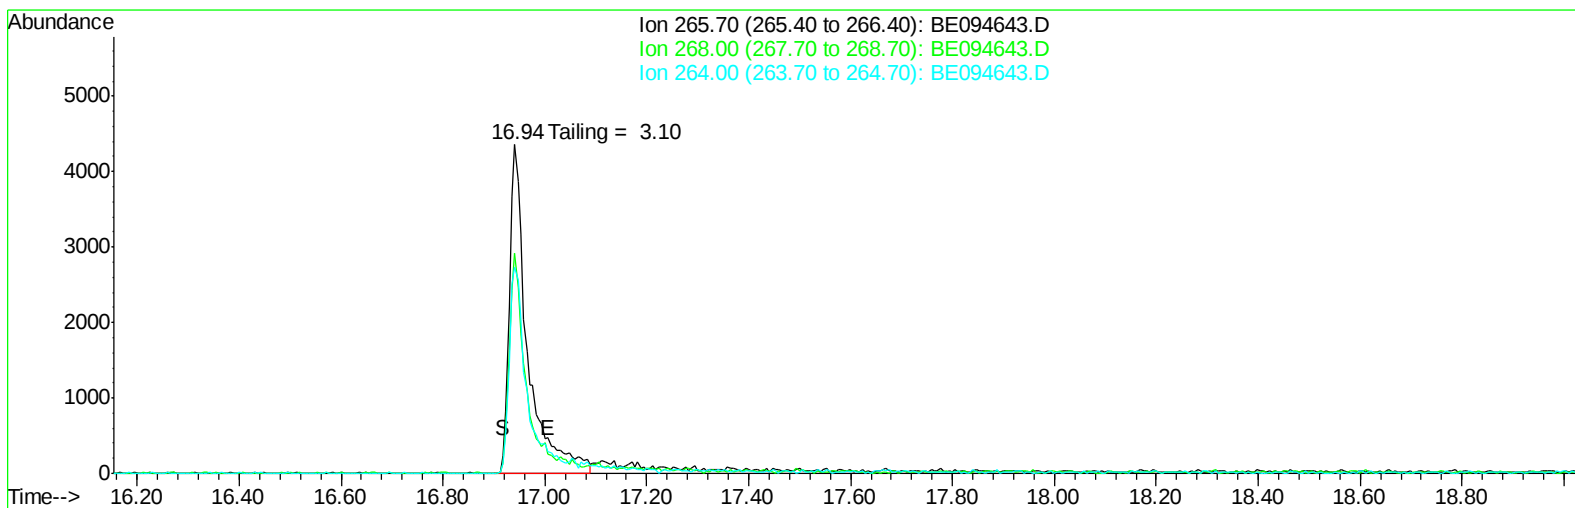

TIC: BE094643.D

(69) Pentachlorophenol (C)

11.130min (-0.021) 39.51ng

response 2

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 63.90 | 11.11# |
| 264.00 | 61.90 | 33.33# |
| 0.00   | 0.00  | 0.00   |