

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103017\
 Data File : BE094651.D
 Acq On : 30 Oct 2017 20:05
 Operator : SJ/JU
 Sample : I6036-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 MW-5

Quant Time: Oct 31 01:44:05 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 23 22:40:47 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1243	0.40	ng	0.00
7) Naphthalene-d8	10.69	136	7091	0.40	ng	-0.02
13) Acenaphthene-d10	14.51	164	4181	0.40	ng	0.00
19) Phenanthrene-d10	17.24	188	8315	0.40	ng	0.00
27) Chrysene-d12	21.43	240	9098	0.40	ng	0.00
34) Perylene-d12	23.97	264	8489	0.40	ng	0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.54	112	716	0.17	ng	0.01
5) Phenol-d6	7.14	99	678	0.11	ng	0.00
8) Nitrobenzene-d5	9.09	82	2272	0.40	ng	0.02
11) 2-Methylnaphthalene-d10	12.28	152	4832	0.42	ng	-0.01
14) 2,4,6-Tribromophenol	16.03	330	526	0.46	ng	0.00
15) 2-Fluorobiphenyl	13.13	172	6687	0.45	ng	-0.01
25) Fluoranthene-d10	19.28	212	48216	0.49	ng	0.00
29) Terphenyl-d14	19.86	244	8327	0.49	ng	0.00
Target Compounds						
17) Acenaphthene	14.57	154	1309	0.092	ng	# 67
23) Phenanthrene	17.30	178	3647	0.124	ng	# 61
32) Bis(2-ethylhexyl)phthalate	21.28	149	3841	0.053	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103017\
Data File : BE094651.D
Acq On : 30 Oct 2017 20:05
Operator : SJ/JU
Sample : I6036-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
MW-5

Quant Time: Oct 31 01:44:05 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 22:40:47 2017
Response via : Initial Calibration

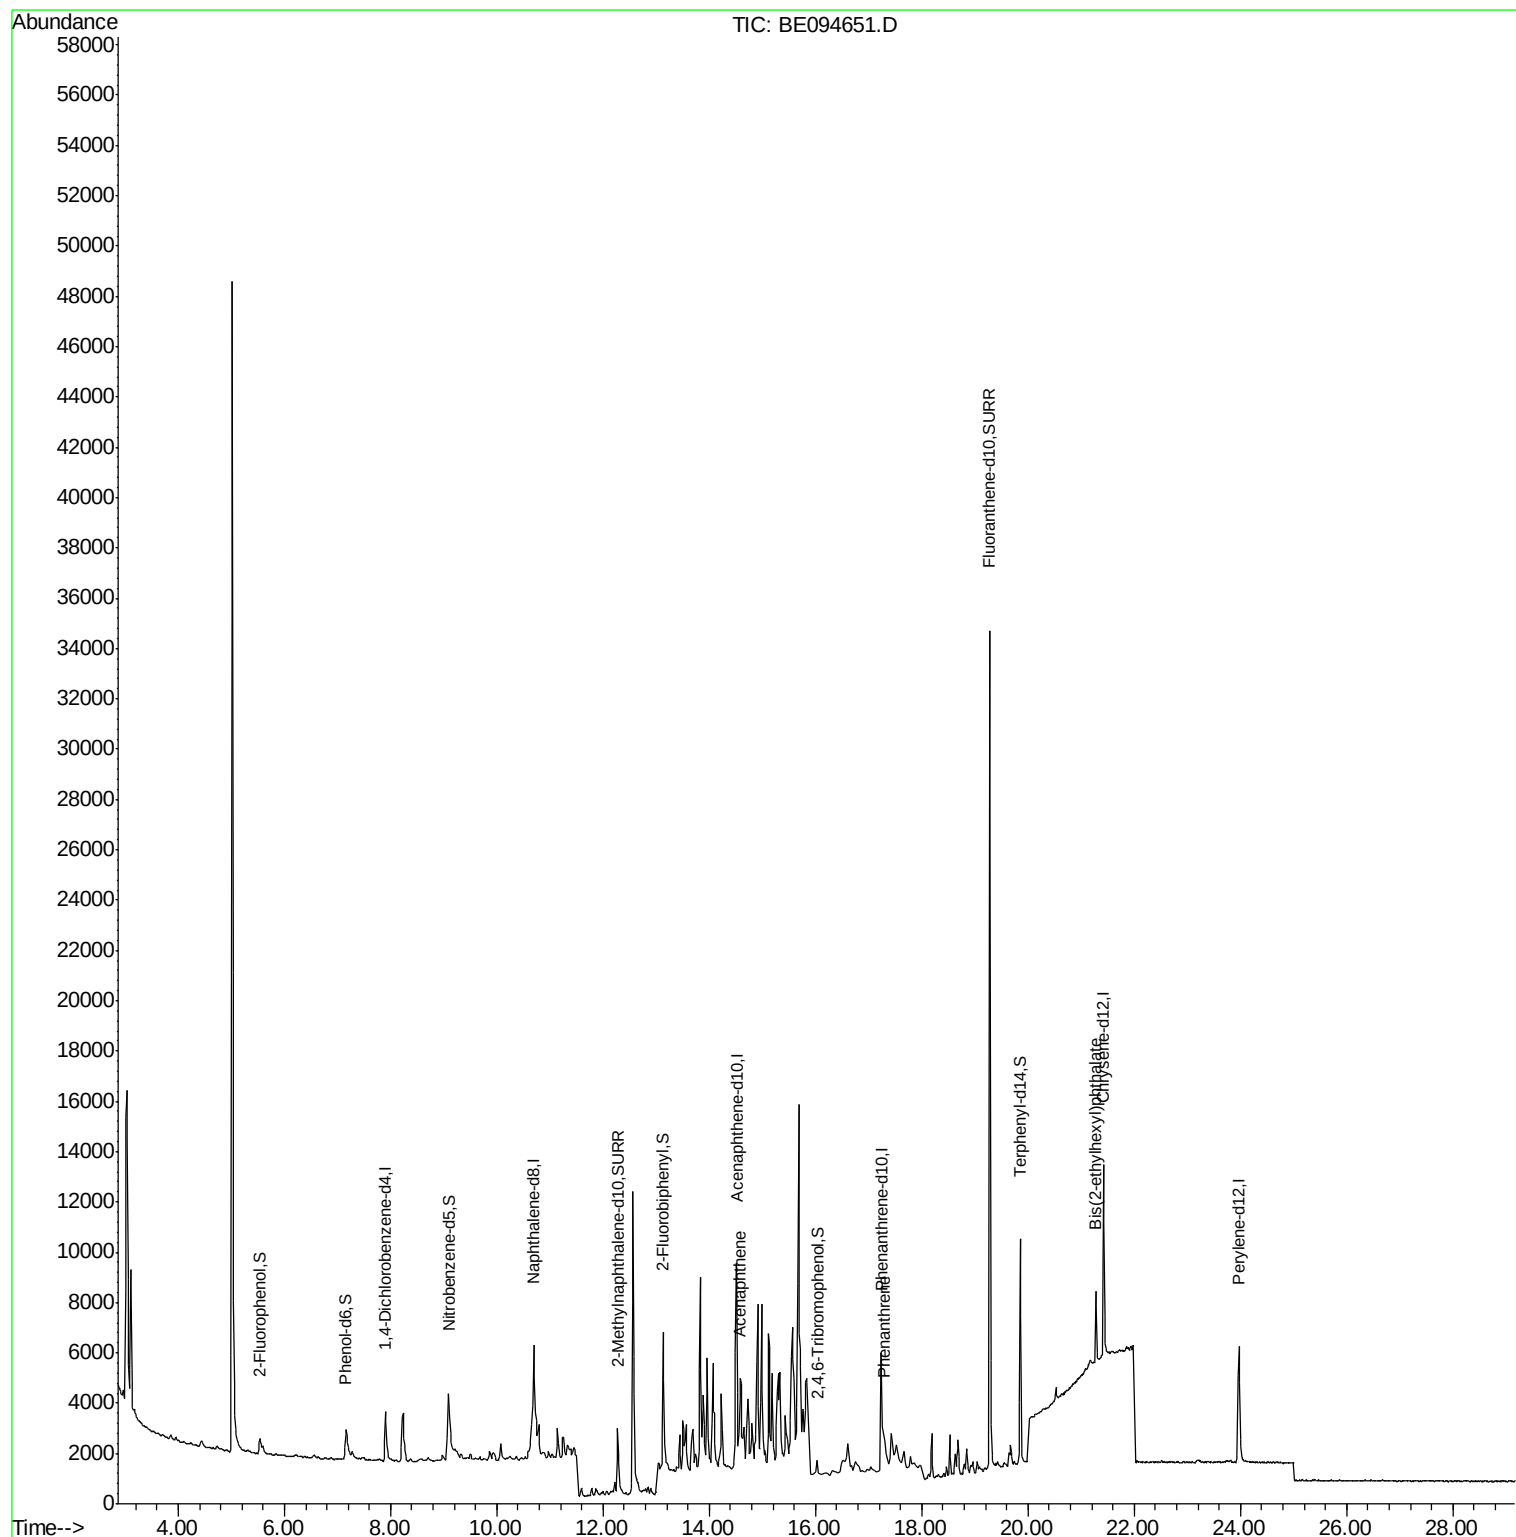

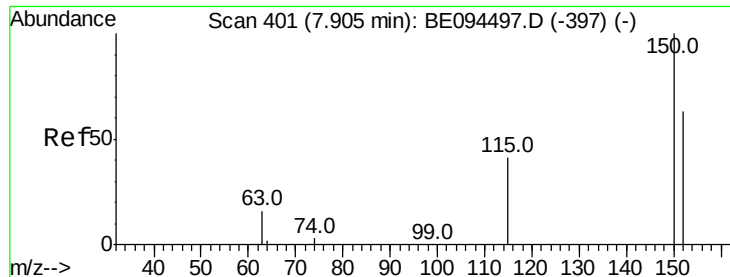

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.90 min Scan# 401

Delta R.T. -0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampleId :

MW-5


Tot Ion:152 Resp: 1243

Ion Ratio Lower Upper

152 100

150 157.6 117.2 175.8




115 79.3 57.0 85.6

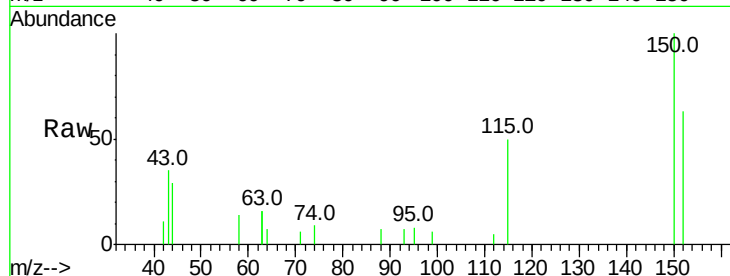

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

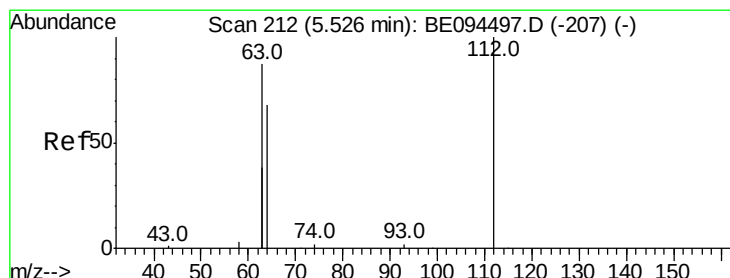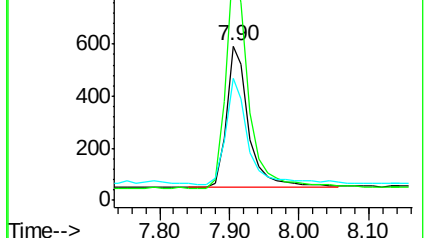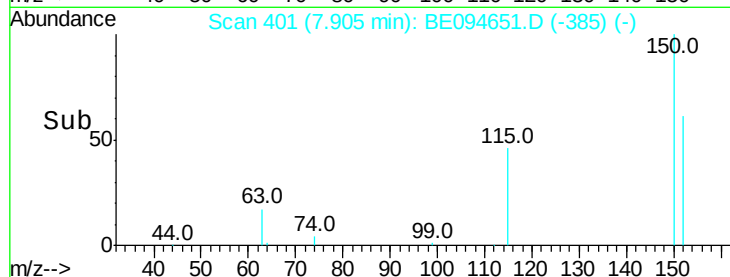

#4

2-Fluorophenol

Concen: 0.168 ng

RT: 5.54 min Scan# 213

Delta R.T. 0.01 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05


Tgt Ion:112 Resp: 716

Ion Ratio Lower Upper

112 100

64 72.2 60.1 90.1



63 147.2 116.8 175.2

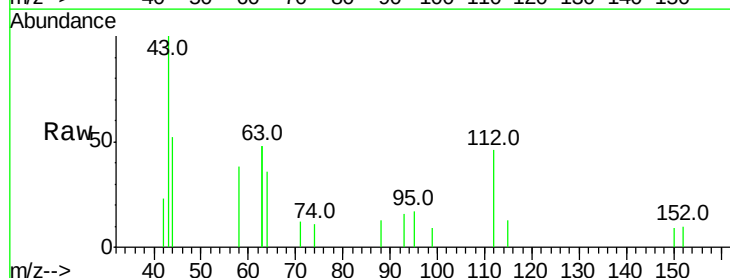


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

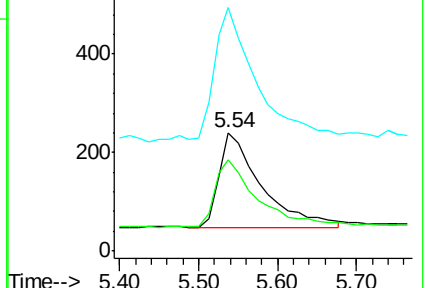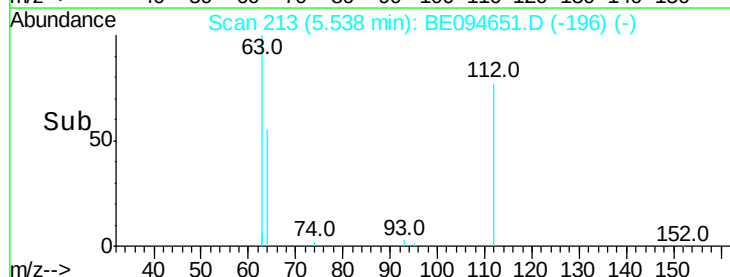

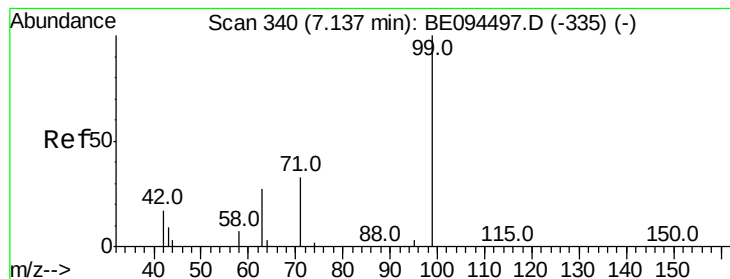

#5

Phenol-d6

Concen: 0.105 ng

RT: 7.14 min Scan# 340

Delta R.T. -0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampled :

MW-5


Tot Ion: 99 Resp: 678

Ion Ratio Lower Upper

99 100

42 0.0 20.2 30.2#




71 37.0 28.4 42.6

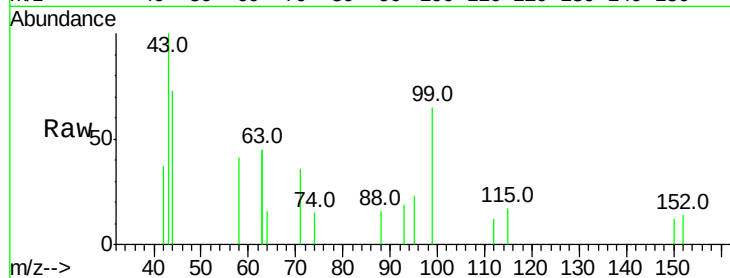

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

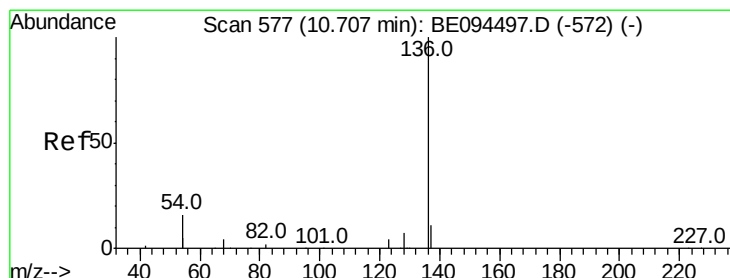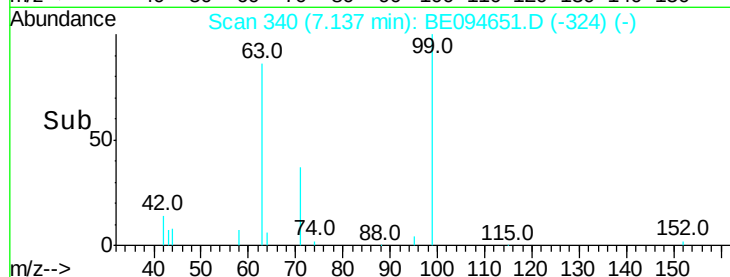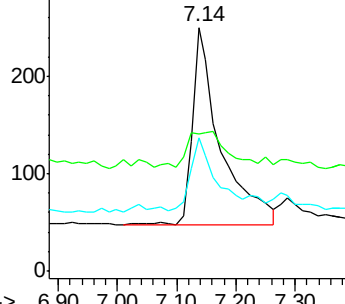

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.69 min Scan# 576

Delta R.T. -0.02 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Tgt Ion: 136 Resp: 7091


Ion Ratio Lower Upper

136 100

137 12.0 9.5 14.3

54 45.4 29.1 43.7#

68 9.6 6.2 9.2#


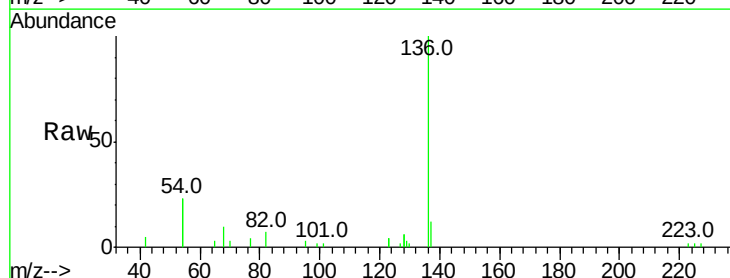



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

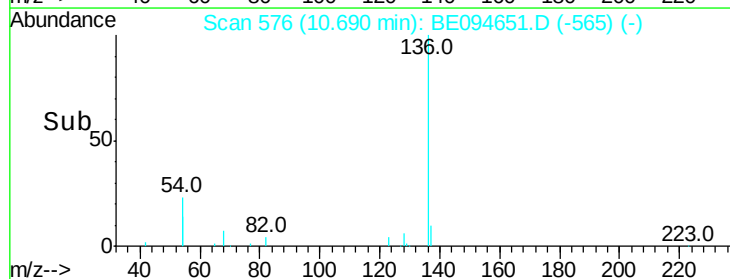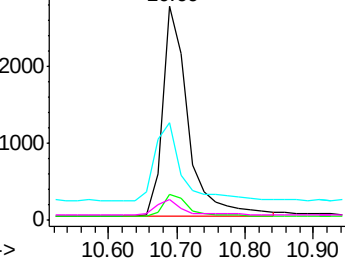



#8

Nitrobenzene-d5

Concen: 0.401 ng

RT: 9.09 min Scan# 481

Delta R.T. 0.02 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampleId :

MW-5


Tot Ion: 82 Resp: 2272

Ion Ratio Lower Upper

82 100

128 175.3 150.0 225.0




54 195.1 154.2 231.4

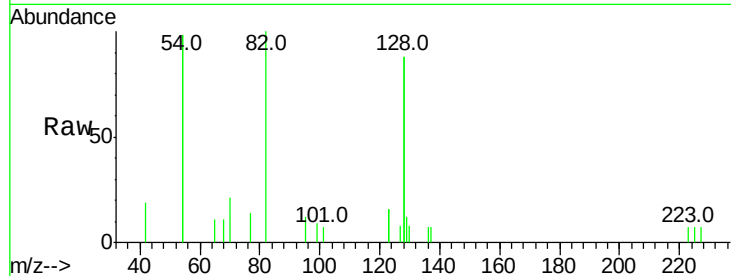

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

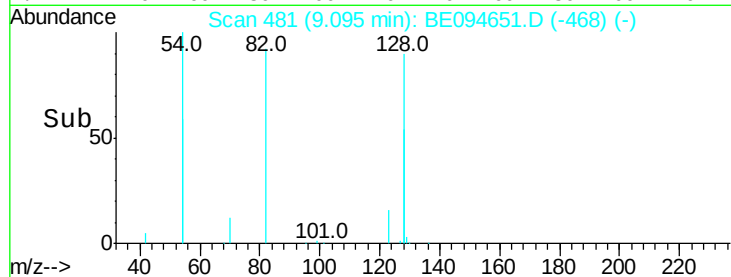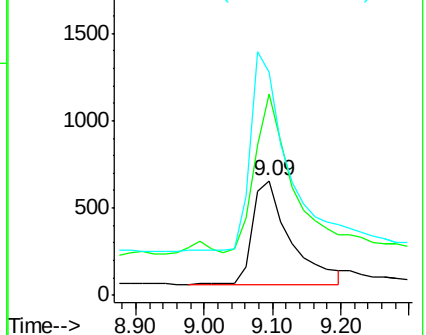

#11

2-Methylnaphthalene-d10

Concen: 0.425 ng

RT: 12.28 min Scan# 821

Delta R.T. -0.01 min

Lab File: BE094651.D


Acq: 30 Oct 2017 20:05

Tgt Ion: 152 Resp: 4832

Ion Ratio Lower Upper



152 100


151 19.3 15.4 23.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E



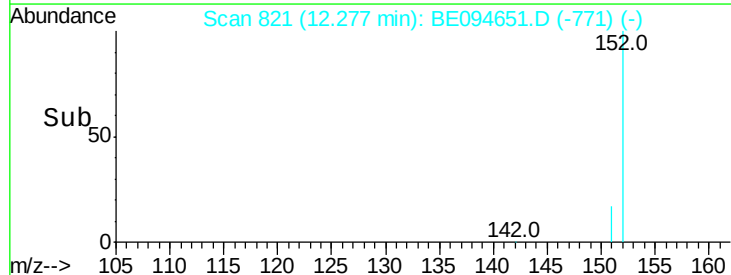
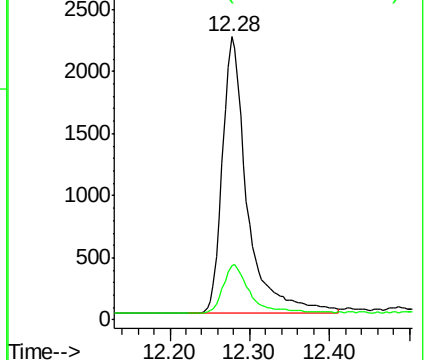




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.51 min Scan# 1111
 Delta R.T. 0.00 min
 Lab File: BE094651.D
 Acq: 30 Oct 2017 20:05




Instrument :
 BNA_E
 ClientSampleId :
 MW-5


Tot Ion:164 Resp: 4181
 Ion Ratio Lower Upper
 164 100
 162 103.0 83.1 124.7
 160 49.8 37.1 55.7

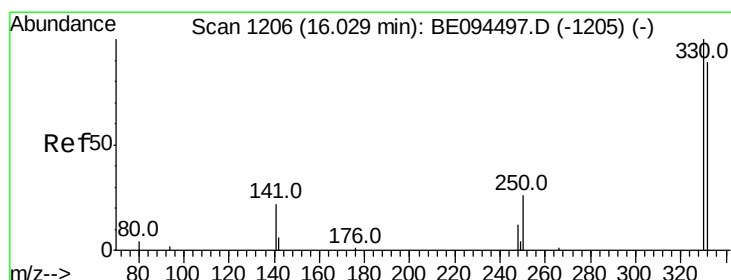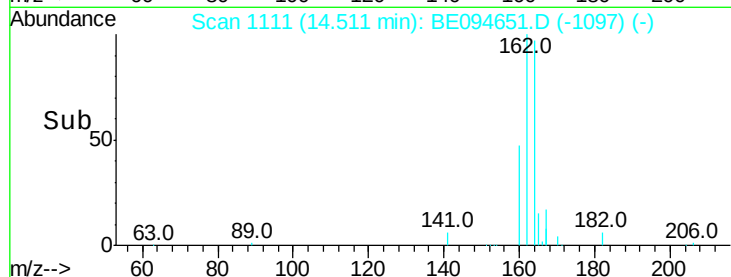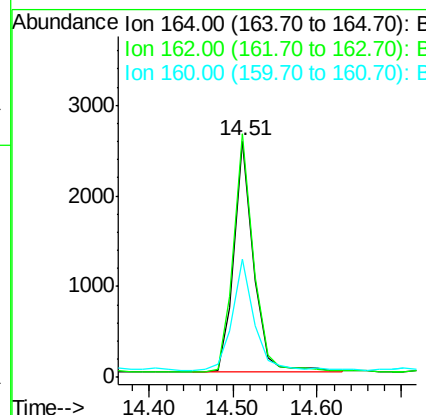

#14
 2,4,6-Tribromophenol
 Concen: 0.456 ng
 RT: 16.03 min Scan# 1206
 Delta R.T. 0.00 min
 Lab File: BE094651.D
 Acq: 30 Oct 2017 20:05

Tgt Ion:330 Resp: 526
 Ion Ratio Lower Upper
 330 100
 332 101.5 152.7 229.1#
 141 0.0 33.7 50.5#



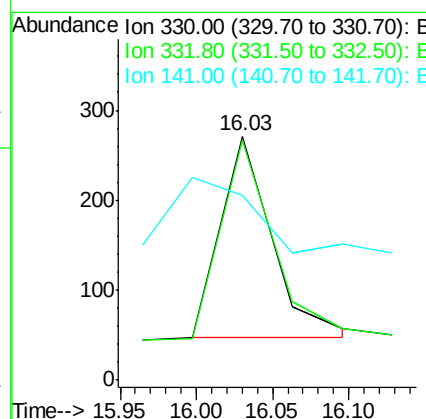
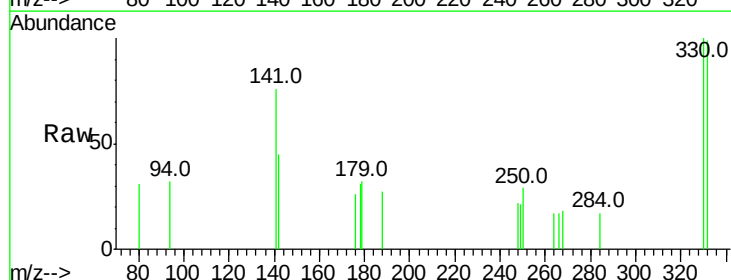


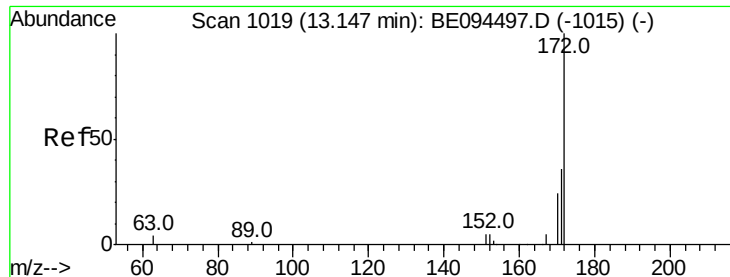

#15
2-Fluorobiphenyl
Concen: 0.454 ng
RT: 13.13 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BE094651.D
Acq: 30 Oct 2017 20:05




Instrument :
BNA_E
ClientSampleId :
MW-5


Tot Ion:172 Resp: 6687
Ion Ratio Lower Upper
172 100
171 36.2 29.9 44.9
170 24.7 21.8 32.8

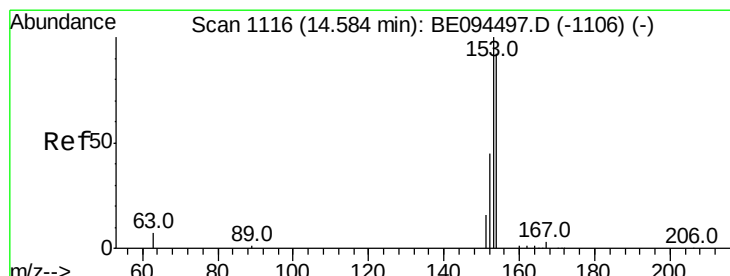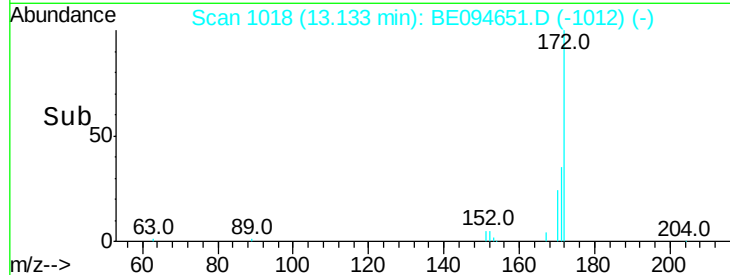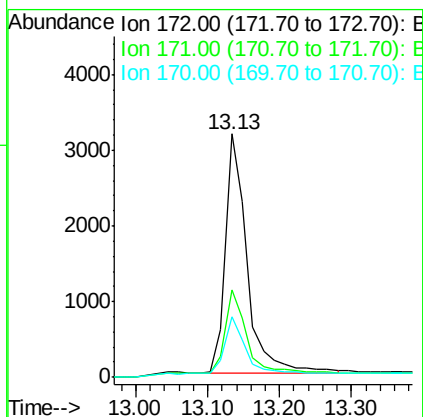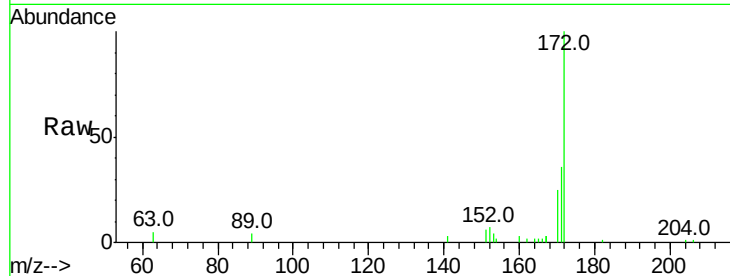

#17
Acenaphthene
Concen: 0.092 ng
RT: 14.57 min Scan# 1115
Delta R.T. -0.01 min
Lab File: BE094651.D
Acq: 30 Oct 2017 20:05

Tgt Ion:154 Resp: 1309
Ion Ratio Lower Upper
154 100
153 136.6 89.2 133.8#
152 90.5 42.0 63.0#

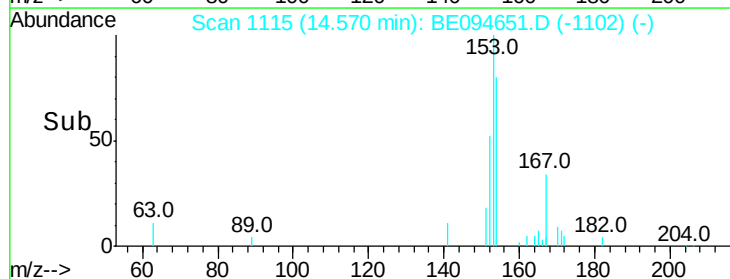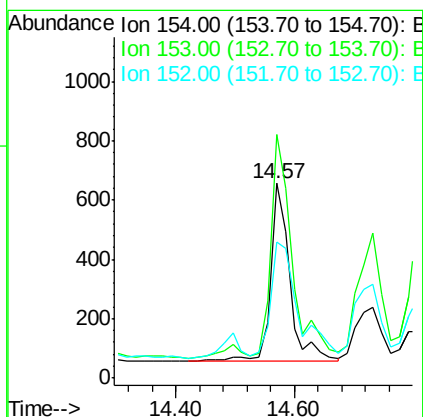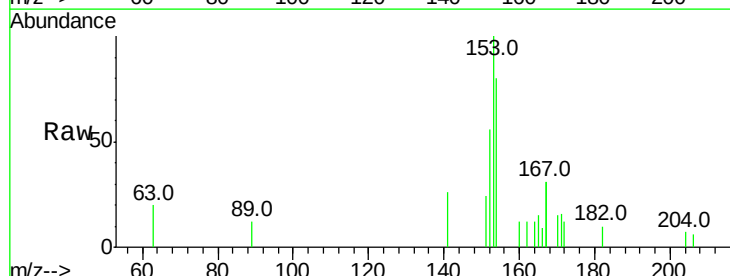



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.24 min Scan# 1243

Delta R.T. 0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampleId :

MW-5


Tot Ion:188 Resp: 8315

Ion Ratio Lower Upper

188 100

94 20.2 3.9 5.9#




80 21.7 3.6 5.4#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

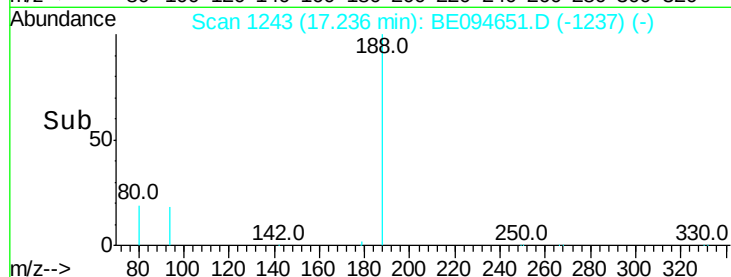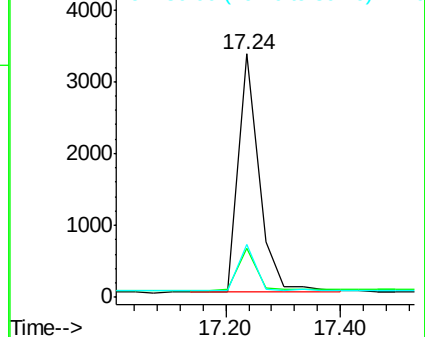

#23

Phenanthrene

Concen: 0.124 ng

RT: 17.30 min Scan# 1245

Delta R.T. 0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05


Tgt Ion:178 Resp: 3647

Ion Ratio Lower Upper

178 100

176 0.0 15.1 22.7#



179 0.0 11.8 17.6#




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

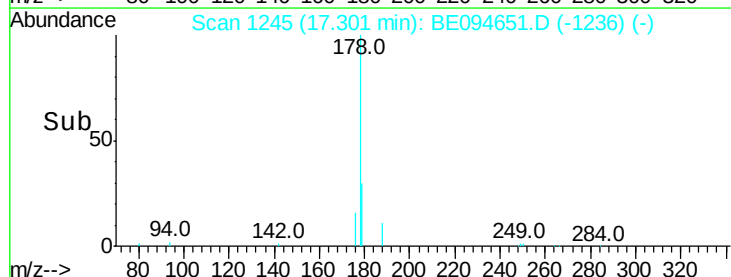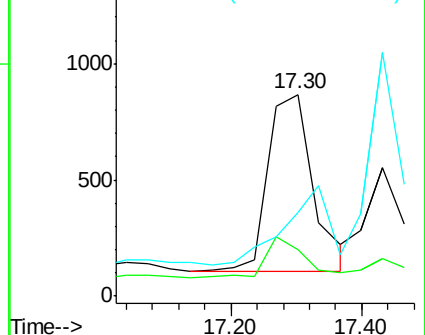



#25

Fluoranthene-d10

Concen: 0.489 ng

RT: 19.28 min Scan# 1433

Delta R.T. -0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampleId :

MW-5


Tot Ion:212 Resp: 48216

Ion Ratio Lower Upper

212 100

106 3.5 2.8 4.2




104 2.0 1.6 2.4

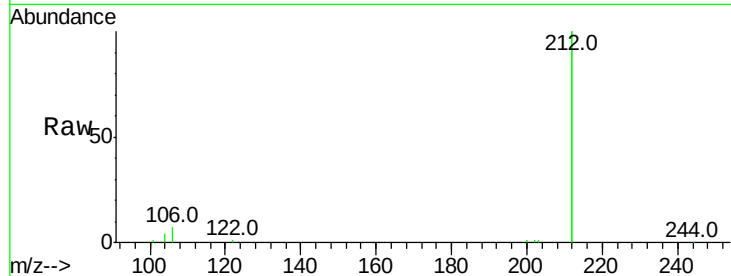

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

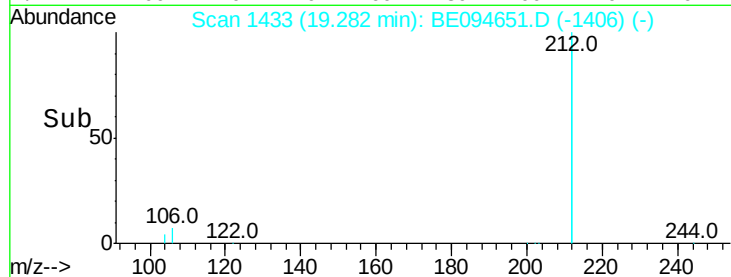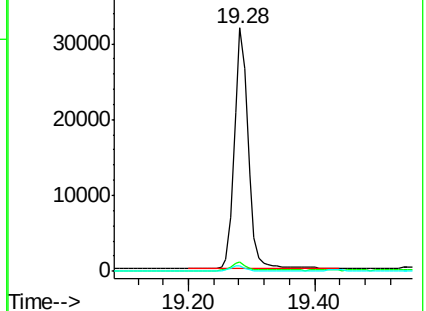

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.43 min Scan# 1656

Delta R.T. 0.00 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05


Tgt Ion:240 Resp: 9098

Ion Ratio Lower Upper

240 100

120 16.1 5.5 8.3#



236 28.0 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




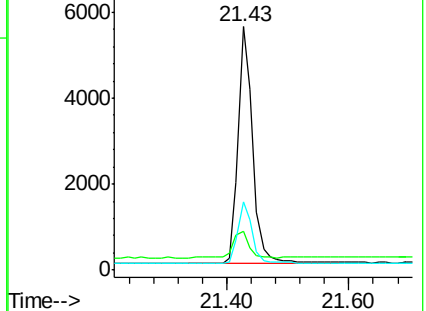




#29
 Terphenyl-d14
 Concen: 0.485 ng
 RT: 19.86 min Scan# 1511
 Delta R.T. -0.01 min
 Lab File: BE094651.D
 Acq: 30 Oct 2017 20:05




Instrument :
 BNA_E
 ClientSampleId :
 MW-5




Tot Ion:244 Resp: 8327
 Ion Ratio Lower Upper
 244 100
 212 38.9 25.4 38.0#
 122 13.8 8.1 12.1#

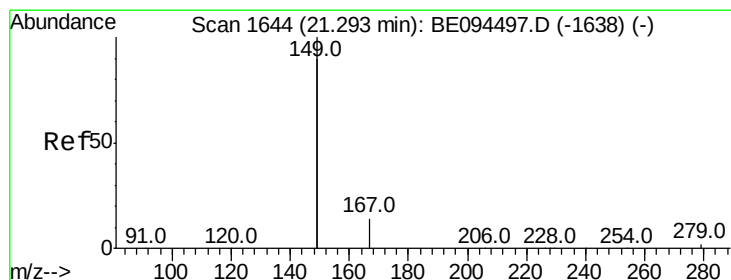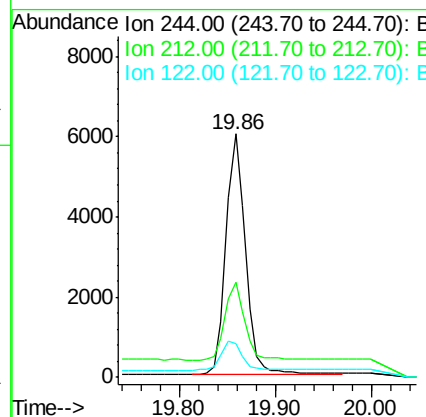

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.053 ng
 RT: 21.28 min Scan# 1643
 Delta R.T. -0.01 min
 Lab File: BE094651.D
 Acq: 30 Oct 2017 20:05

Tgt Ion:149 Resp: 3841
 Ion Ratio Lower Upper
 149 100
 167 6.6 5.4 8.0
 279 2.4 0.7 1.1#

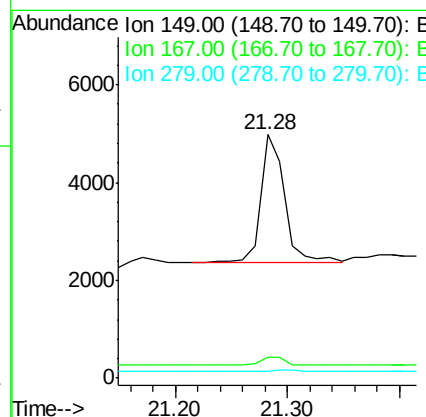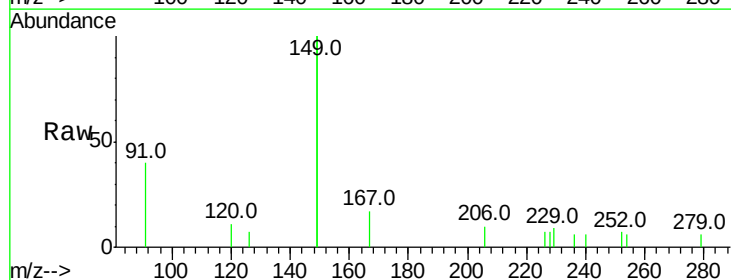



#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.97 min Scan# 2135

Delta R.T. 0.02 min

Lab File: BE094651.D

Acq: 30 Oct 2017 20:05

Instrument :

BNA_E

ClientSampleId :

MW-5

Tot Ion: 264 Resp: 8489

Ion Ratio Lower Upper

264 100

260 27.1 20.5 30.7

265 35.6 22.8 34.2#

