


Data Path : Z:\HPCHEM1\BNA E\Data\BE103017\
 Data File : BE094643.D
 Acq On : 30 Oct 2017 13:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 22:40:47 2017

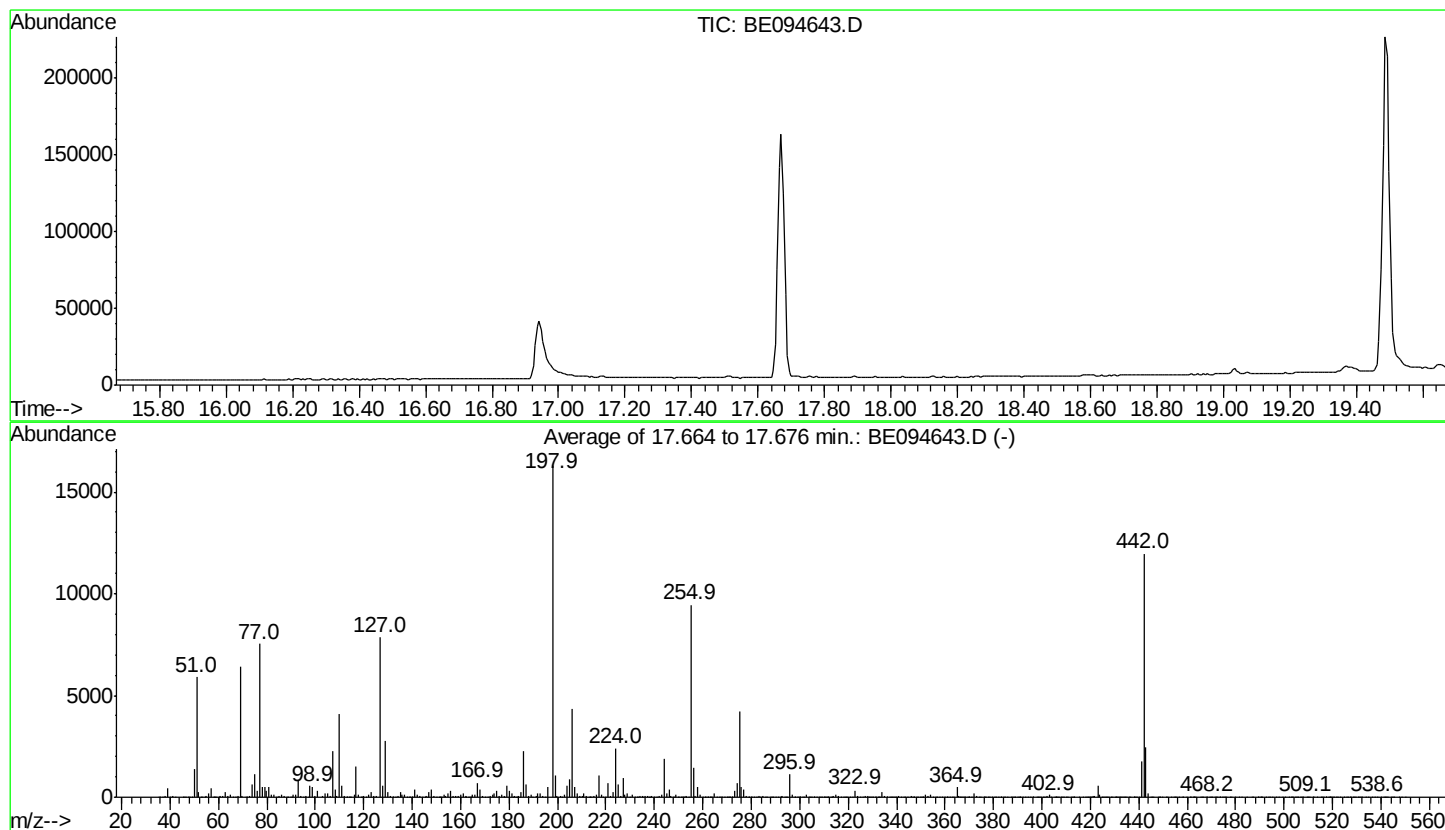

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	5892	PASS
68	69	0.00	2	1.2	75	PASS
69	198	0.00	100	39.5	6437	PASS
70	69	0.00	2	0.7	42	PASS
127	198	10	80	48.1	7842	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16291	PASS
199	198	5	9	6.6	1075	PASS
275	198	10	60	25.7	4192	PASS
365	198	1	100	3.0	490	PASS
441	442	0.01	24	14.9	1784	PASS
442	198	50	100	73.5	11970	PASS
443	442	15	24	20.4	2443	PASS