
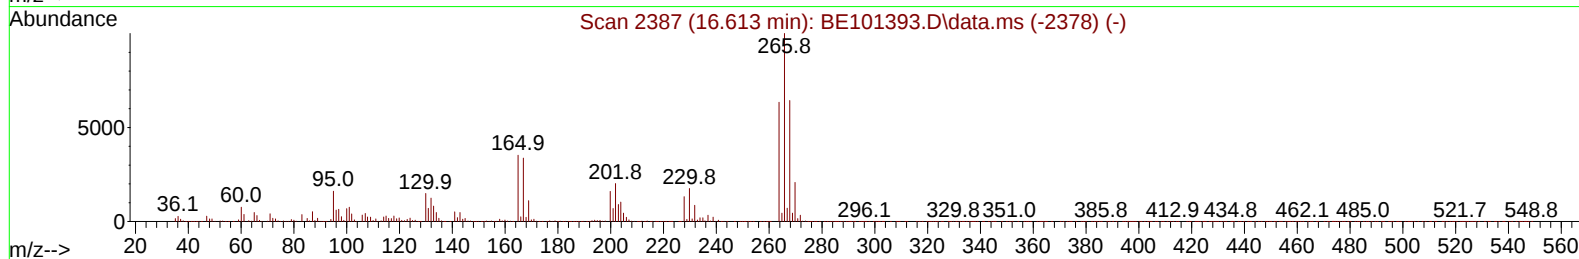
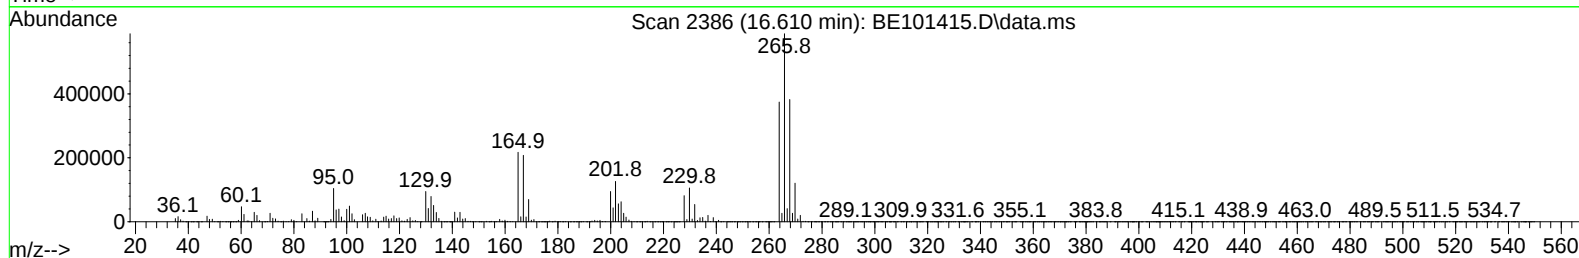


Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE103024\  
Data File : BE101415.D  
Acq On : 30 Oct 2024 8:33  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:32:57 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

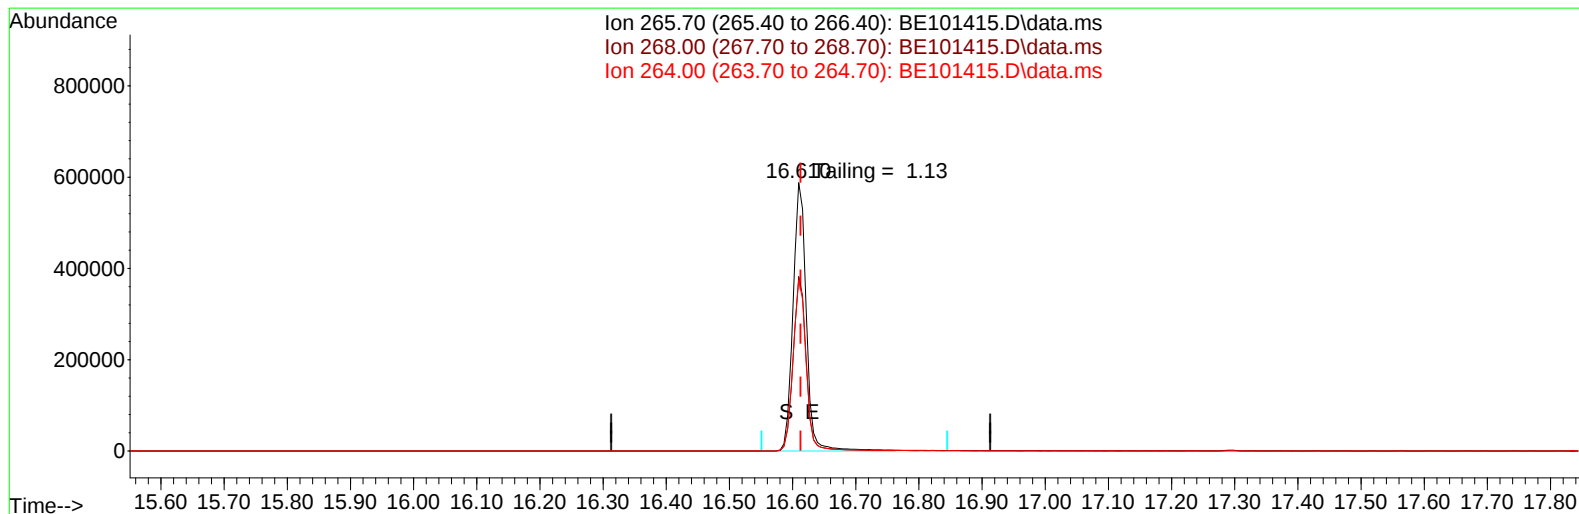

TIC: BE101415.D\data.ms

**(70) Pentachlorophenol (C)**




16.610min (-0.003) 1457840.97 ng

response 867778

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.40  | 65.02  |
| 264.00 | 63.40  | 63.69  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE103024\  
Data File : BE101415.D  
Acq On : 30 Oct 2024 8:33  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 11:32:57 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

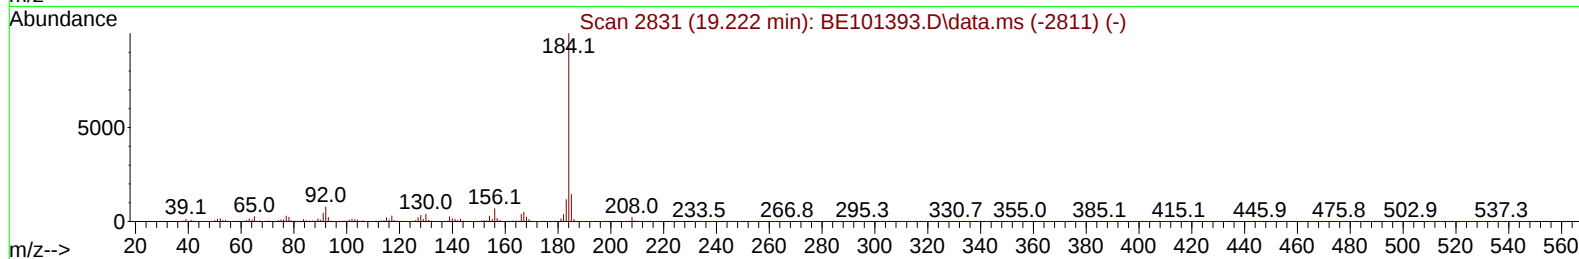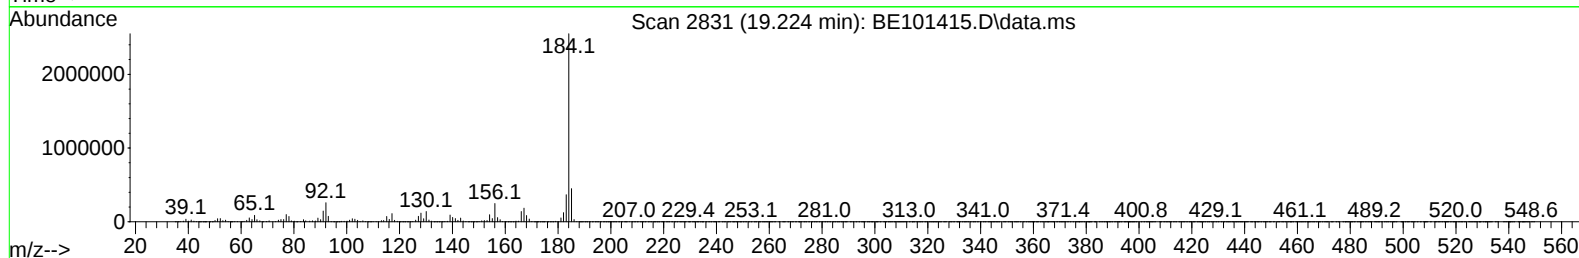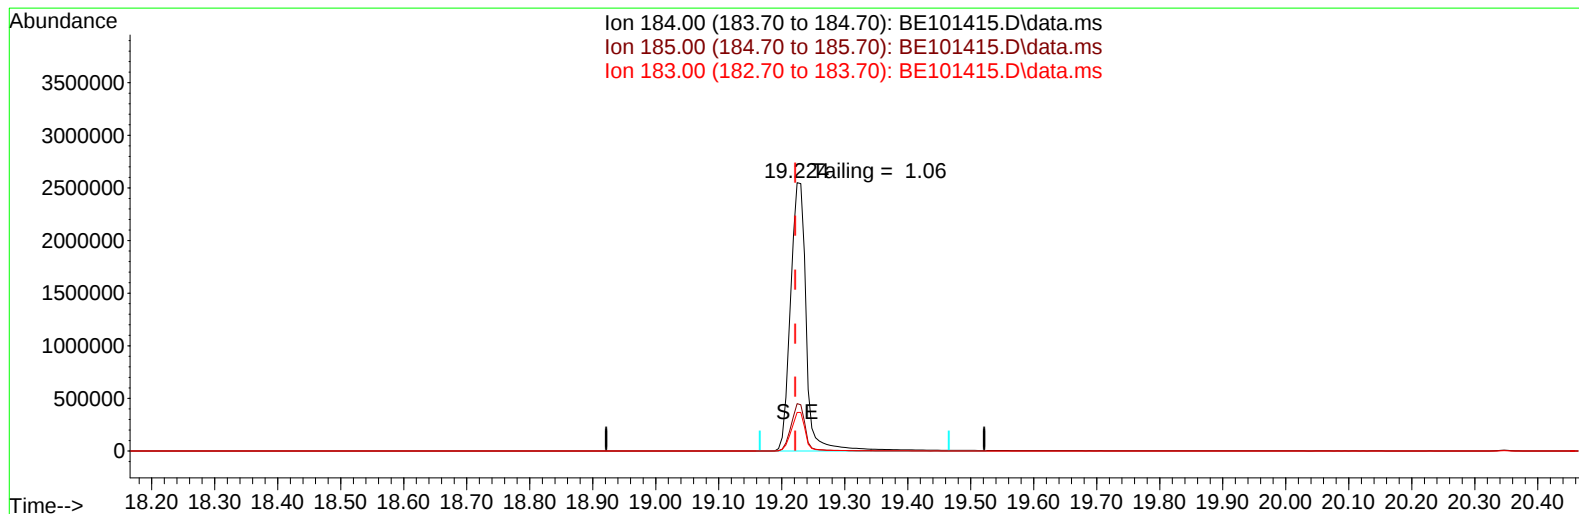

TIC: BE101415.D\data.ms

**(77) Benzidine****19.224min (+ 0.003) 119973.08 ng****response 4469009**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 17.64# |
| 183.00 | 11.60  | 14.37# |
| 0.00   | 0.00   | 0.00   |