

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
 Data File : BE101422.D
 Acq On : 30 Oct 2024 13:34
 Operator : RC/JU
 Sample : PB164382BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164382BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.319	459	465	496	rBV	2370278	3677839	34.28%	8.475%
2	6.946	735	742	776	rBV	2255975	3798603	35.41%	8.754%
3	7.569	841	848	857	rBV	437754	692479	6.46%	1.596%
4	8.779	1047	1054	1075	rBV	1350825	2320700	21.63%	5.348%
5	10.336	1311	1319	1339	rBV	591980	1051053	9.80%	2.422%
6	12.804	1731	1739	1760	rBV	3996124	6037260	56.28%	13.912%
7	14.179	1966	1973	1987	rBV	1039710	1516079	14.13%	3.494%
8	15.683	2221	2229	2250	rBV	3743007	5368204	50.04%	12.371%
9	16.911	2432	2438	2451	rBV	1312192	1964843	18.32%	4.528%
10	19.508	2874	2880	2899	rBV	7811338	10727413	100.00%	24.721%
11	21.071	3140	3146	3159	rBV	2105528	2770305	25.82%	6.384%
12	23.356	3527	3535	3546	rBV	1754728	3470017	32.35%	7.996%




Sum of corrected areas: 43394795

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101422.D
Acq On : 30 Oct 2024 13:34
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

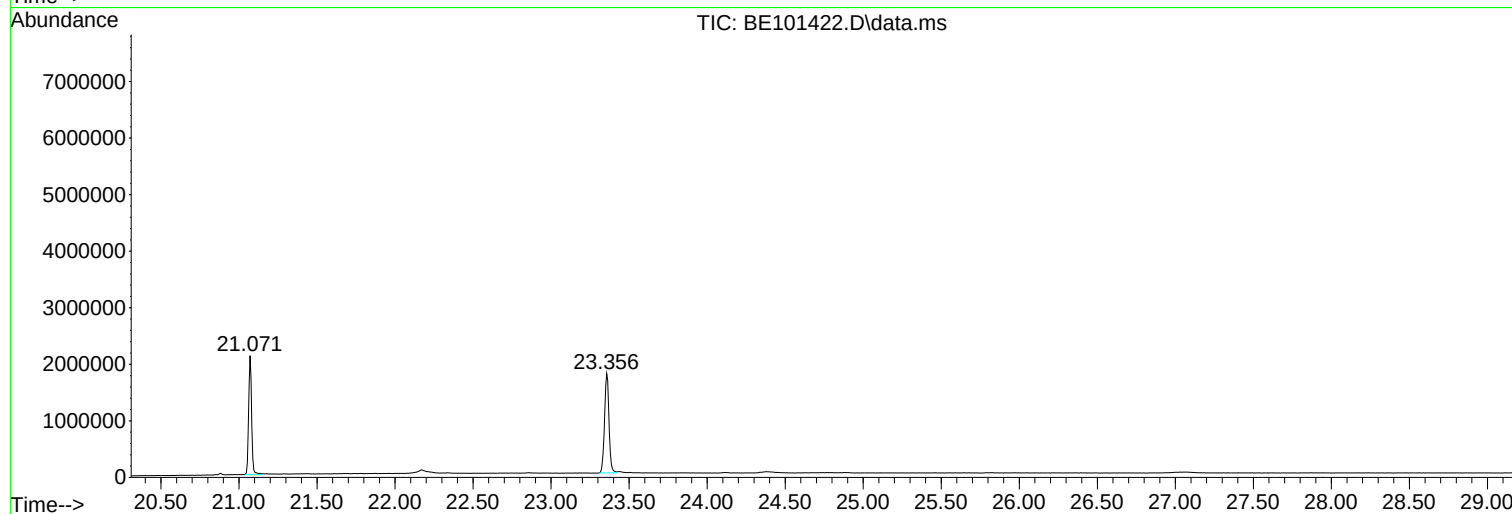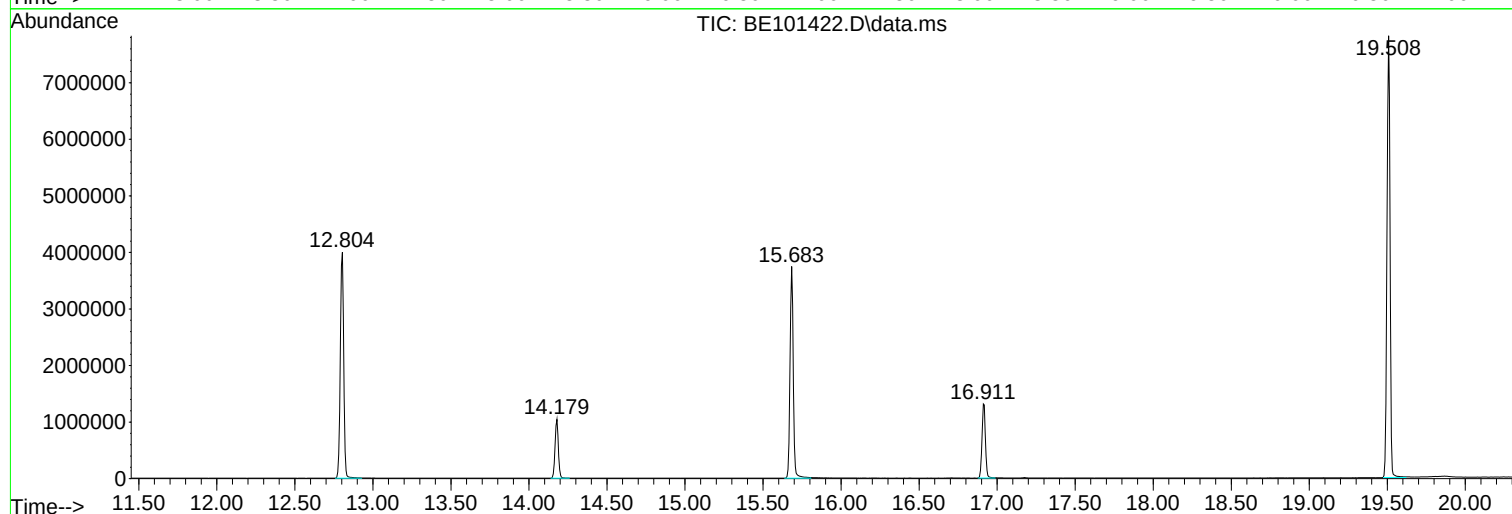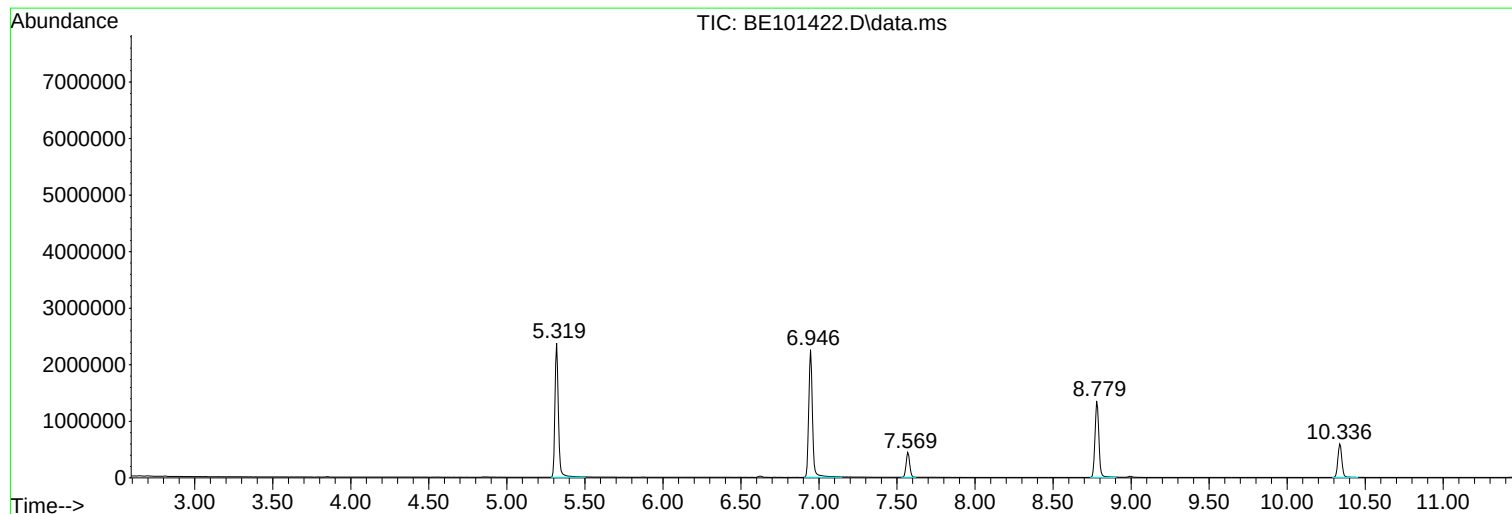

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101422.D
Acq On : 30 Oct 2024 13:34
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101422.D
Acq On : 30 Oct 2024 13:34
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------