
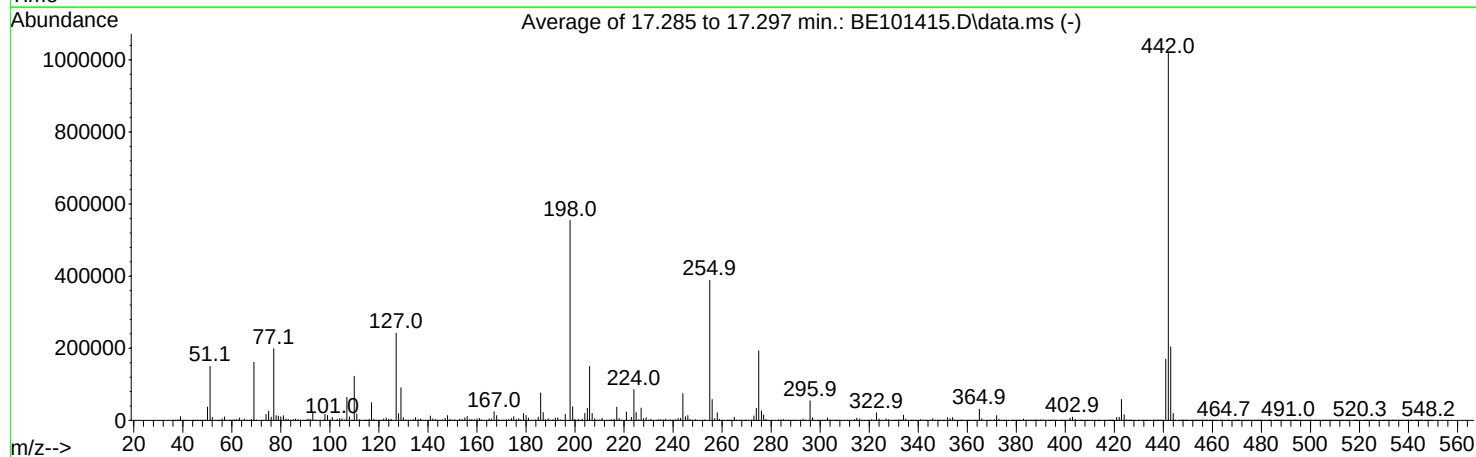


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101415.D
Acq On : 30 Oct 2024 8:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 29 01:26:30 2024

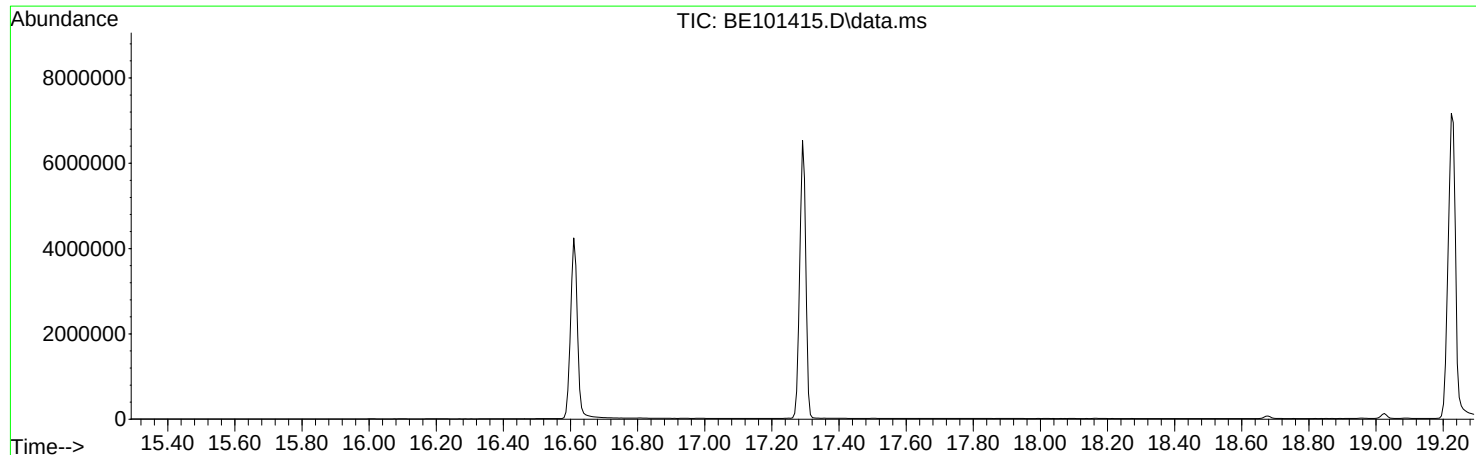




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	149650	PASS
68	69	0.00	2	1.5	2442	PASS
69	198	0.00	100	29.1	161402	PASS
70	69	0.00	2	0.5	775	PASS
127	198	10	80	43.6	242042	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	554688	PASS
199	198	5	9	6.8	37811	PASS
275	198	10	60	34.8	192789	PASS
365	198	1	100	5.6	31245	PASS
441	198	0.01	100	30.6	169798	PASS
442	442	50	100	100.0	1020544	PASS
443	442	15	24	20.0	203661	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101415.D
Acq On : 30 Oct 2024 8:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

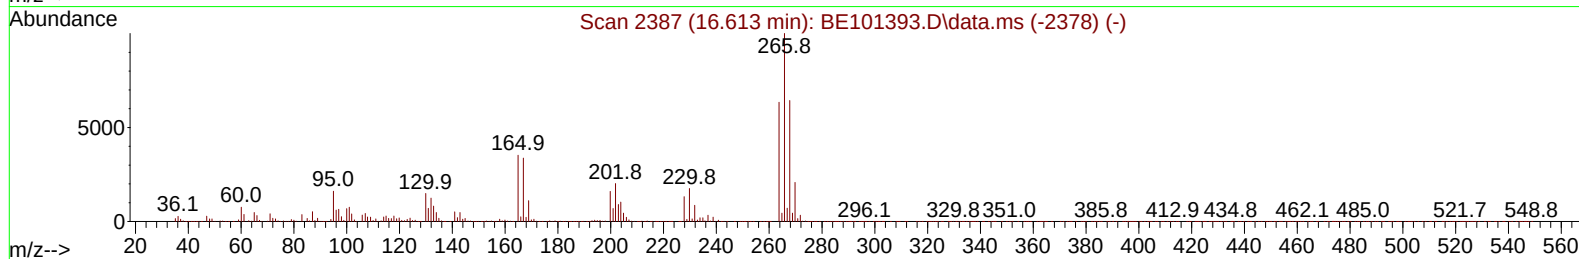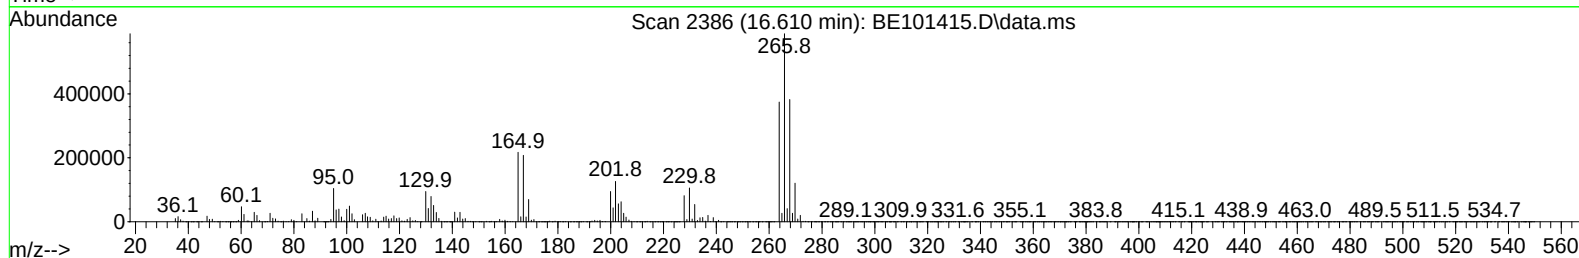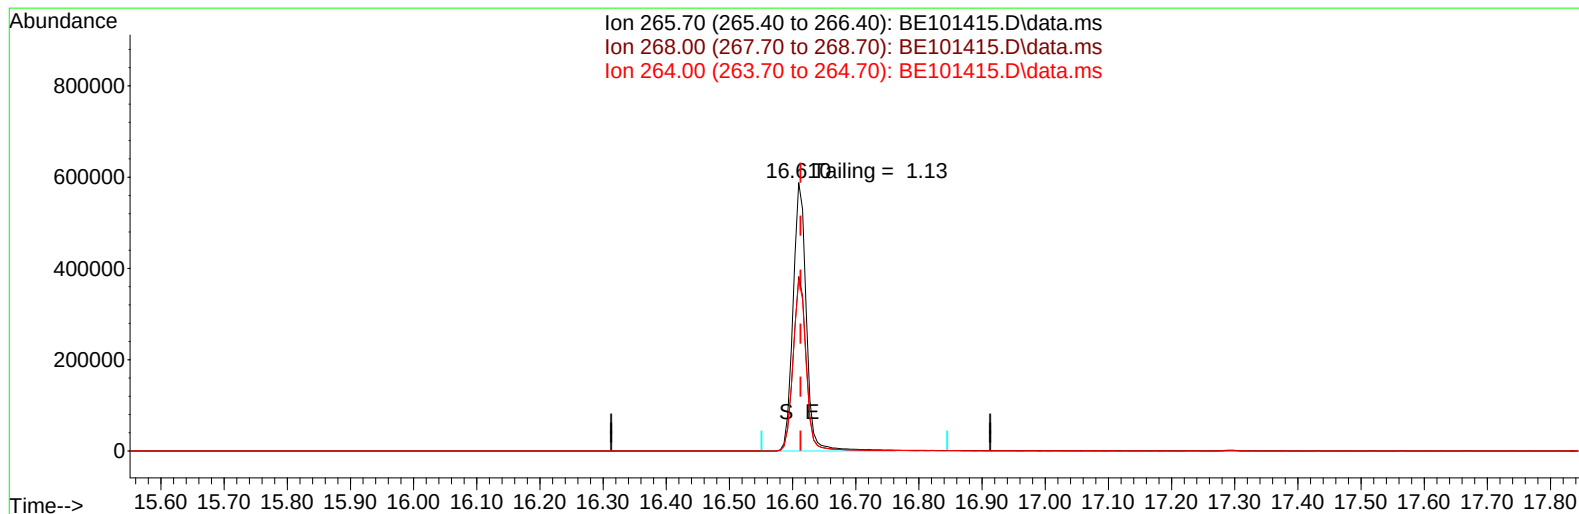

TIC: BE101415.D\data.ms

(70) Pentachlorophenol (C)

16.610min (-0.003) 1457840.97 ng




response 867778

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.02
264.00	63.40	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103024\
Data File : BE101415.D
Acq On : 30 Oct 2024 8:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Oct 30 11:32:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

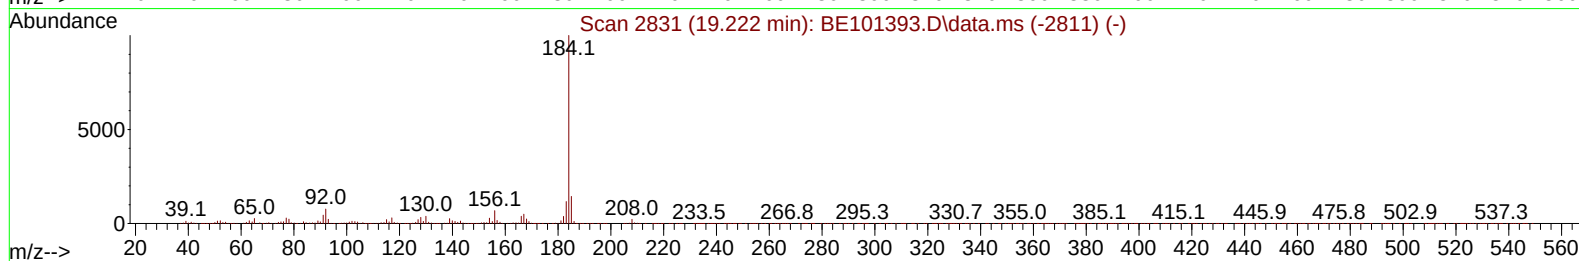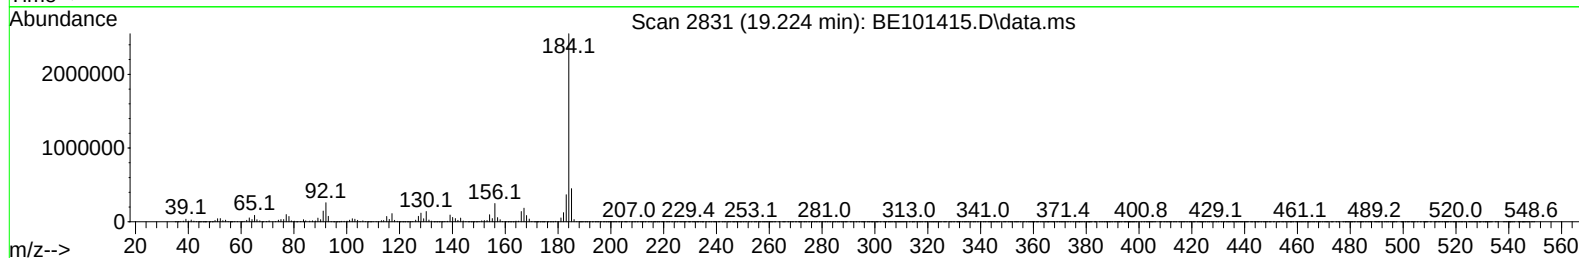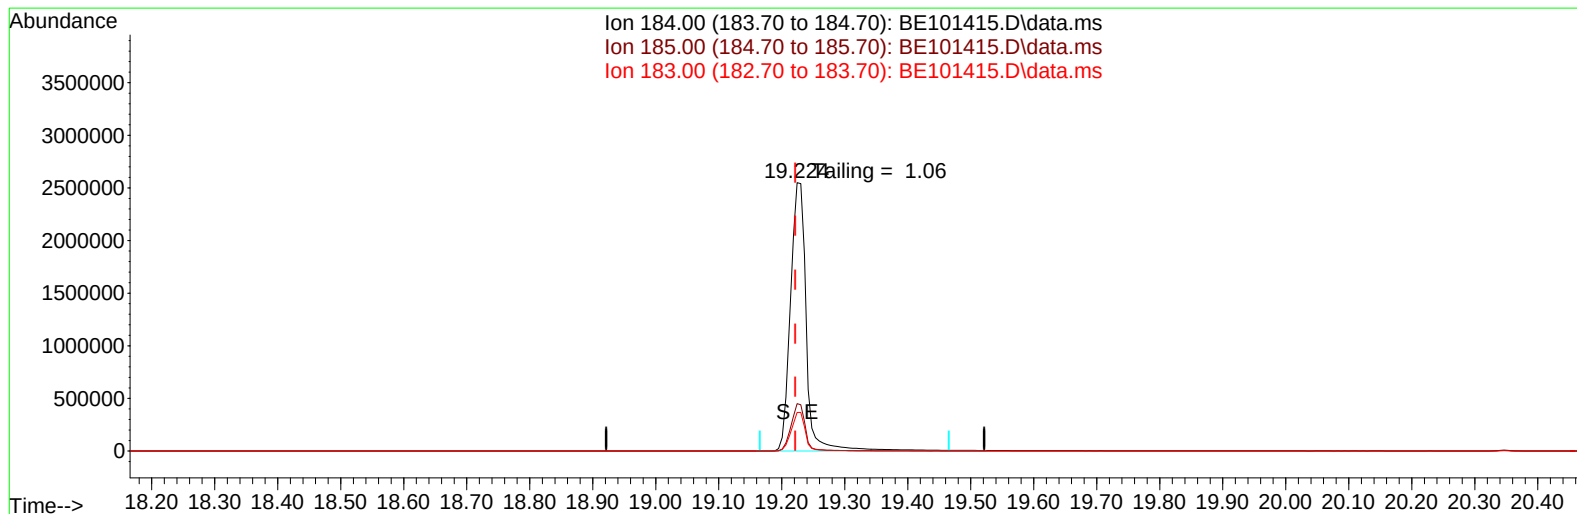

TIC: BE101415.D\data.ms

(77) Benzidine

19.224min (+ 0.003) 119973.08 ng

response 4469009

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	17.64#
183.00	11.60	14.37#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2024	BNA_E	<u>BE101415.D</u>
Compound Name	Response	Retention Time
DDT	2196903	20.347
DDD	83566	19.912
DDE	196	19.5
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83762	2280665	3.67

Instrument :
BNA_E
ClientSampleId :
DFTPP