


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE103114\
 Data File : BE088421.D
 Acq On : 31 Oct 2014 14:02
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE103114.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 01 00:42:07 2014

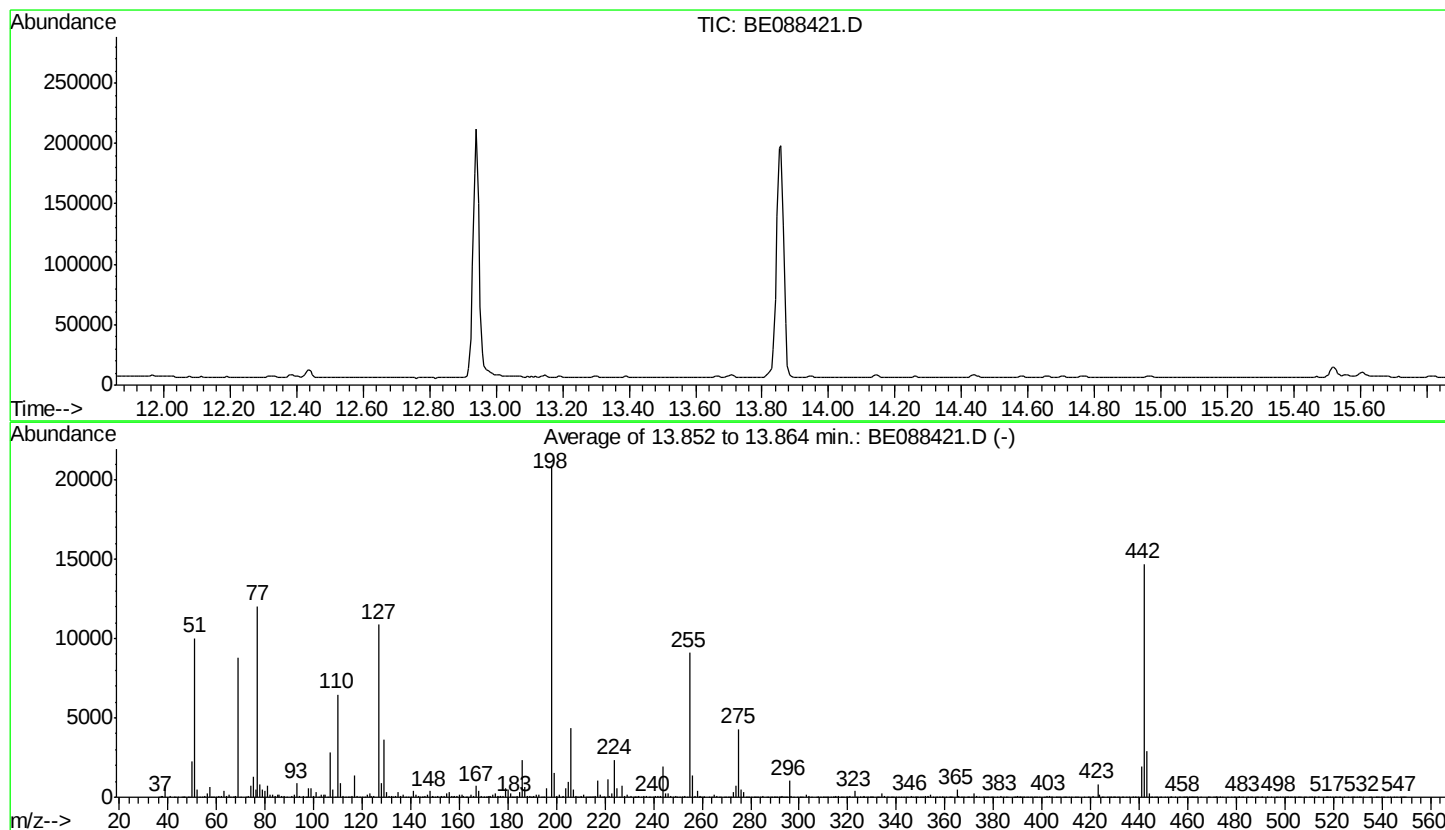

AutoFind: Scans 1815, 1816, 1817; Background Corrected with Scan 1799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	10029	PASS
68	69	0.00	2	1.3	110	PASS
69	198	0.00	100	41.9	8754	PASS
70	69	0.00	2	0.4	38	PASS
127	198	10	80	52.0	10865	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20893	PASS
199	198	5	9	7.3	1522	PASS
275	198	10	60	20.5	4278	PASS
365	198	1	100	2.1	447	PASS
441	442	0.01	24	13.4	1968	PASS
442	198	50	100	70.4	14707	PASS
443	442	15	24	19.6	2876	PASS