


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE103114\
 Data File : BE088432.D
 Acq On : 31 Oct 2014 20:23
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE103114.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 01 00:42:07 2014

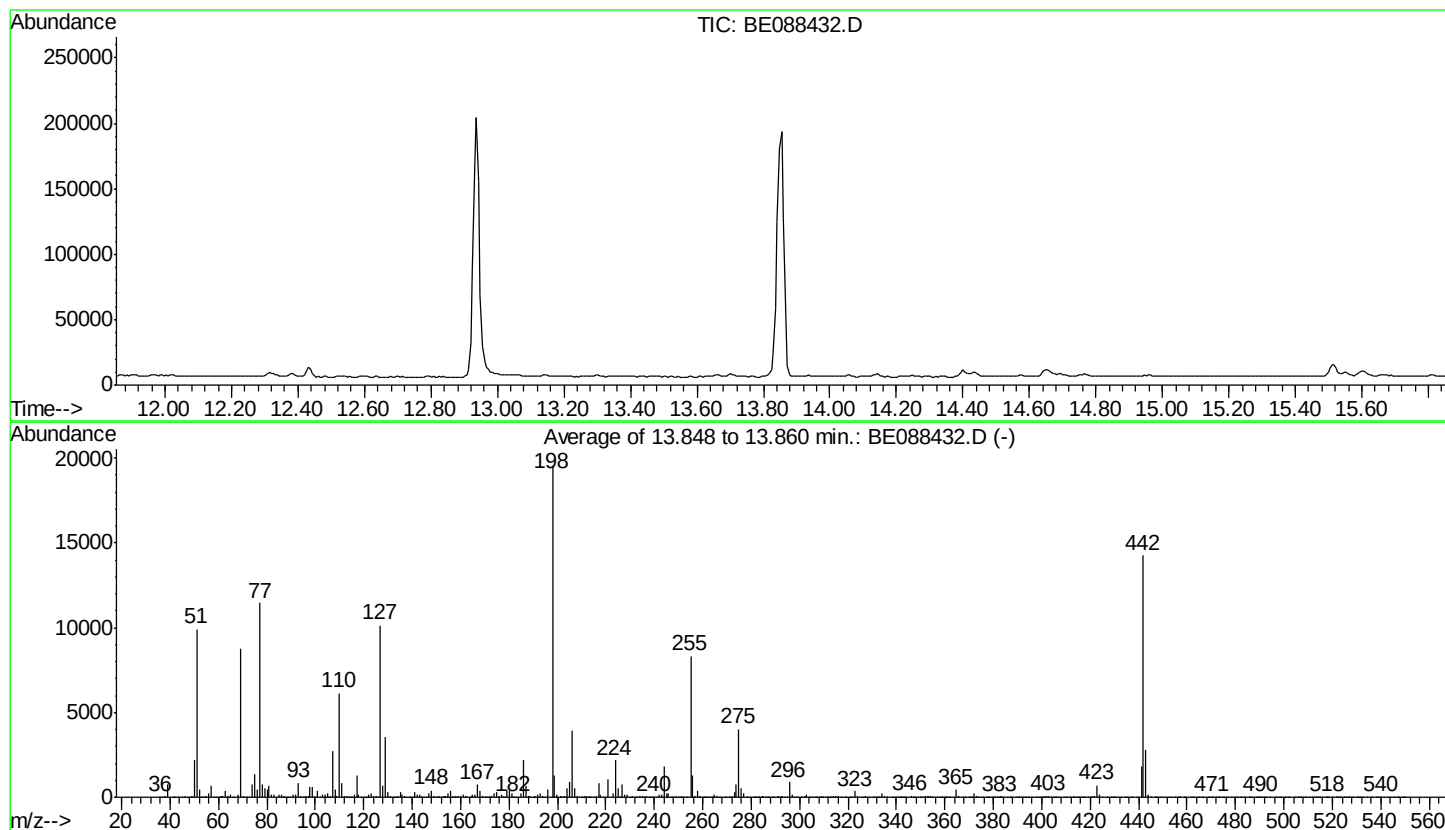

AutoFind: Scans 1814, 1815, 1816; Background Corrected with Scan 1803

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	9930	PASS
68	69	0.00	2	1.3	117	PASS
69	198	0.00	100	44.7	8744	PASS
70	69	0.00	2	0.7	57	PASS
127	198	10	80	51.9	10150	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19562	PASS
199	198	5	9	6.7	1308	PASS
275	198	10	60	20.6	4029	PASS
365	198	1	100	2.2	427	PASS
441	442	0.01	24	12.5	1786	PASS
442	198	50	100	72.9	14268	PASS
443	442	15	24	19.7	2813	PASS