


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE103114\  
 Data File : BE088453.D  
 Acq On : 1 Nov 2014 14:59  
 Operator : TP/JJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-PAH-BE103114.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Nov 01 00:42:07 2014

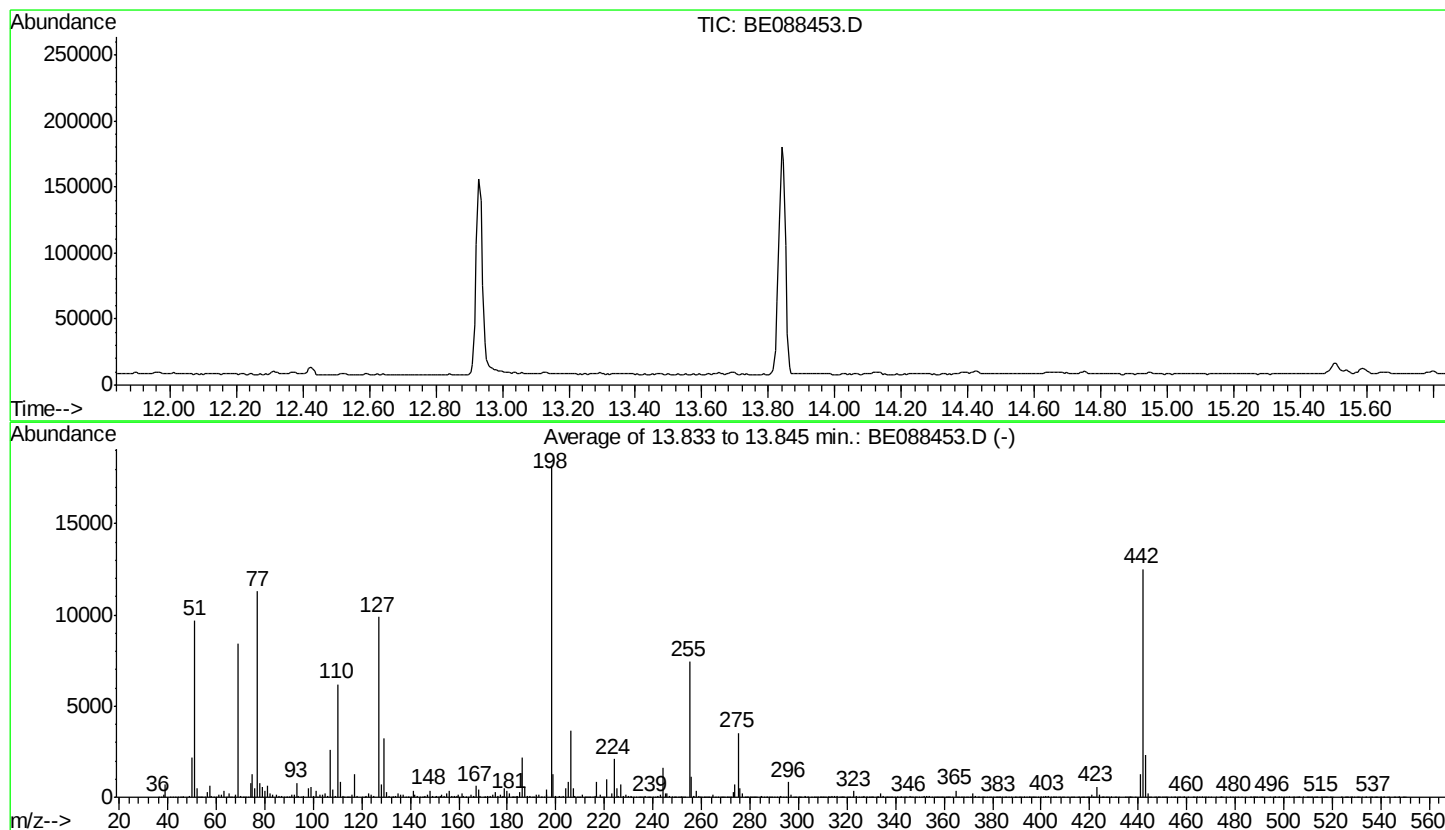

AutoFind: Scans 1812, 1813, 1814; Background Corrected with Scan 1799

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 53.2      | 9665    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 117     | PASS             |
| 69          | 198          | 0.00         | 100          | 46.3      | 8428    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 43      | PASS             |
| 127         | 198          | 10           | 80           | 54.4      | 9895    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 18184   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 1243    | PASS             |
| 275         | 198          | 10           | 60           | 19.4      | 3532    | PASS             |
| 365         | 198          | 1            | 100          | 2.0       | 356     | PASS             |
| 441         | 442          | 0.01         | 24           | 10.0      | 1254    | PASS             |
| 442         | 198          | 50           | 100          | 68.8      | 12508   | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 2290    | PASS             |