

Data Path : Z:\HPCHEM1\BNA_E\Data\BE103116\
 Data File : BE092484.D
 Acq On : 31 Oct 2016 17:51
 Operator : UM/SJ
 Sample : H5473-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 WOOLSTON-TS-003

Quant Time: Nov 01 11:08:45 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 25 15:25:33 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	11315	5.00	ng	0.00
7) Naphthalene-d8	10.95	136	52395	5.00	ng	0.00
12) Acenaphthene-d10	14.82	164	32779	5.00	ng	0.00
18) Phenanthrene-d10	17.56	188	64634	5.00	ng	-0.02
24) Chrysene-d12	21.75	240	93032	5.00	ng	0.00
31) Perylene-d12	24.11	264	79388	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.66	112	25072	11.87	ng	-0.02
5) Phenol-d6	7.34	99	34140	10.75	ng	-0.02
8) Nitrobenzene-d5	9.34	82	16029	4.32	ng	-0.02
13) 2,4,6-Tribromophenol	16.31	330	9180	10.30	ng	-0.01
14) 2-Fluorobiphenyl	13.43	172	35168	4.40	ng	-0.01
26) Terphenyl-d14	20.17	244	45695	3.97	ng	-0.02
Target Compounds						
2) 1,4-Dioxane	3.64	88	7	Below Cal	#	19
3) n-Nitrosodimethylamine	3.70	42	195	0.30 ng	#	2
20) Pentachlorophenol	17.23	266	163	0.45 ng		94
29) Bis(2-ethylhexyl)phthalate	21.63	149	5610	0.75 ng	#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE103116\
Data File : BE092484.D
Acq On : 31 Oct 2016 17:51
Operator : UM/SJ
Sample : H5473-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
WOOLSTON-TS-003

Quant Time: Nov 01 11:08:45 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 15:25:33 2016
Response via : Initial Calibration

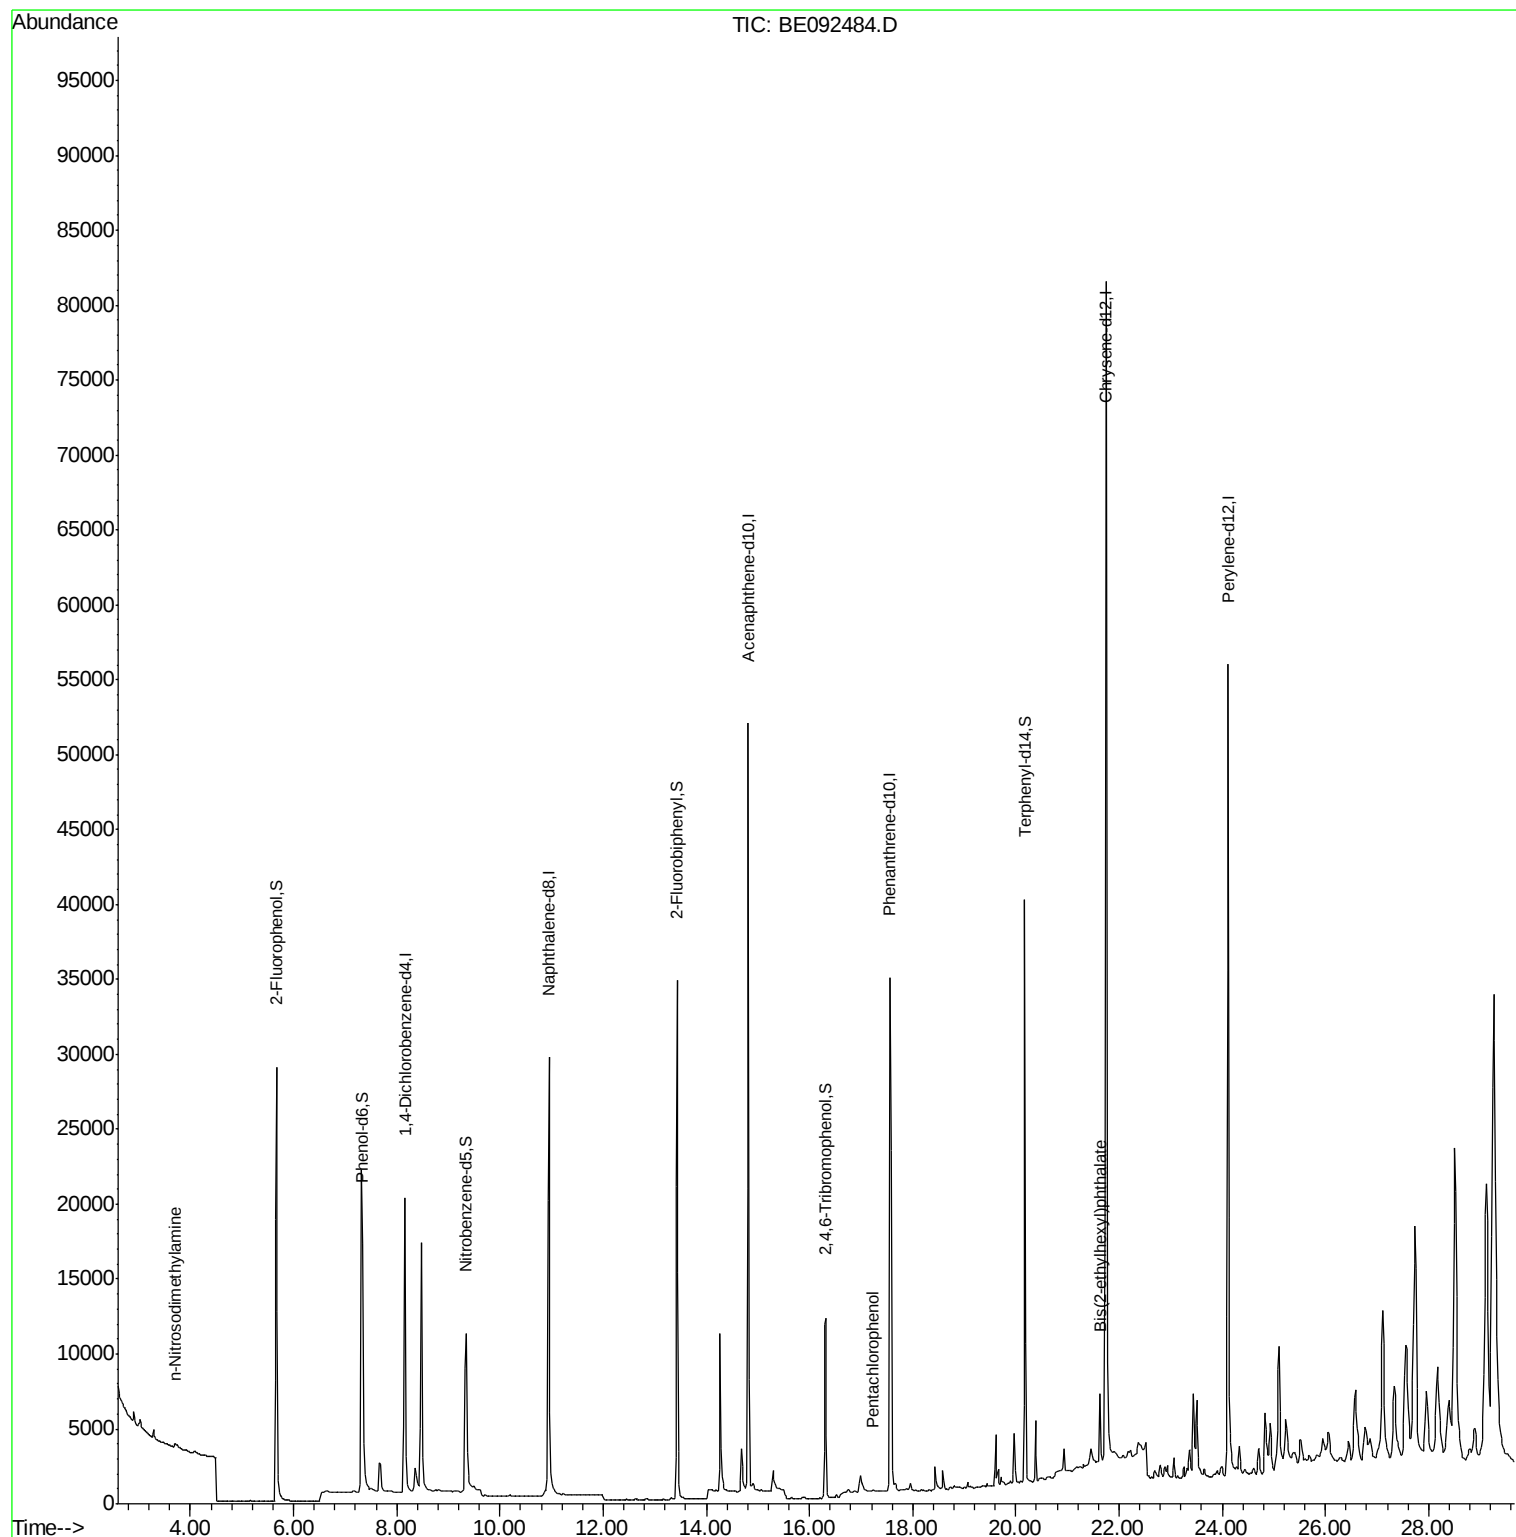




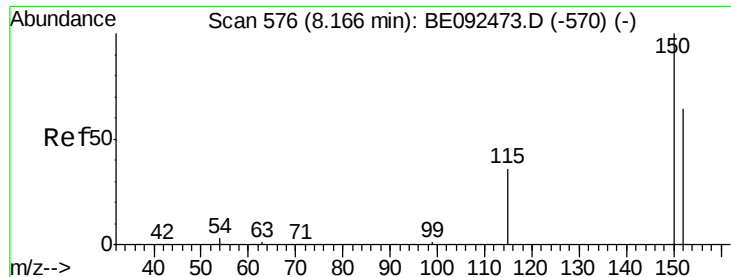


#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 8.17 min Scan# 576
Delta R.T. -0.00 min
Lab File: BE092484.D
Acq: 31 Oct 2016 17:51

Instrument :
BNA_E
ClientSampleId :
WOOLSTON-TS-003




Tgt Ion:152 Resp: 11315
Ion Ratio Lower Upper
152 100
150 149.6 106.0 159.0
115 51.5 31.2 46.8#

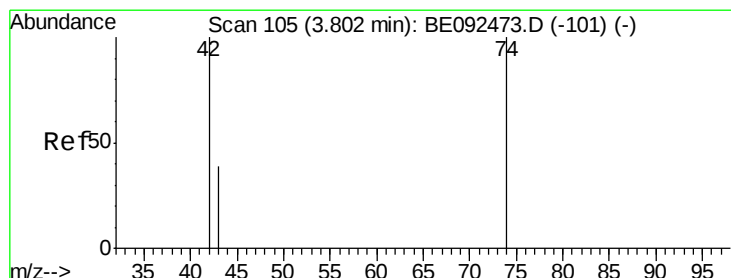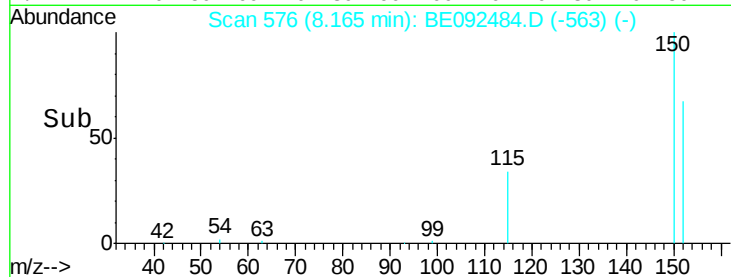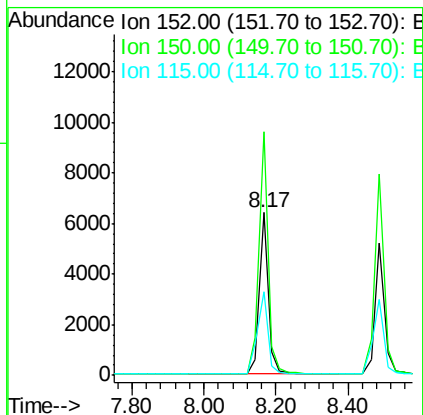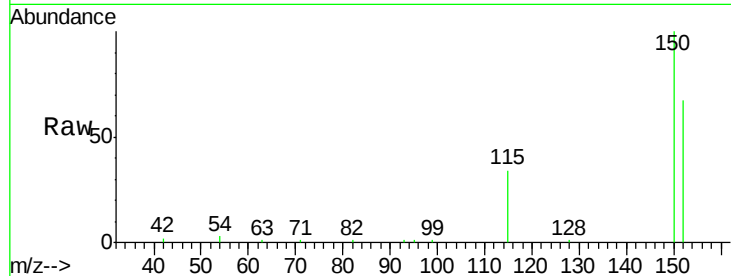


#3

n-Nitrosodimethylamine
Concen: 0.30 ng
RT: 3.70 min Scan# 96
Delta R.T. -0.10 min
Lab File: BE092484.D
Acq: 31 Oct 2016 17:51

Tgt Ion: 42 Resp: 195
Ion Ratio Lower Upper
42 100
74 0.0 86.0 129.0#
44 0.0 5.1 7.7#

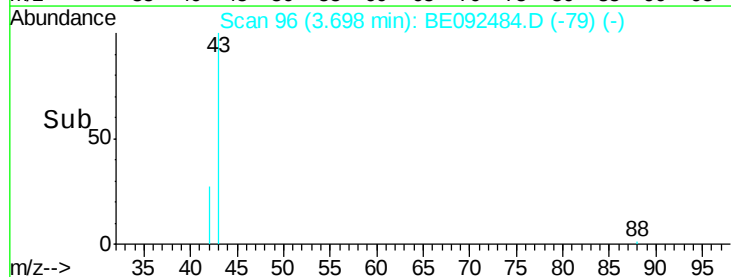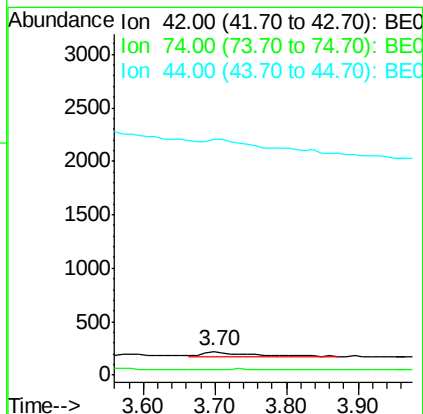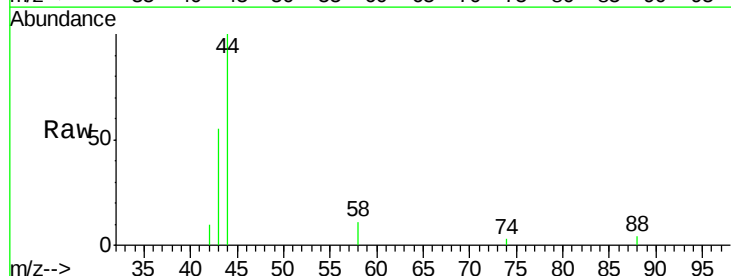

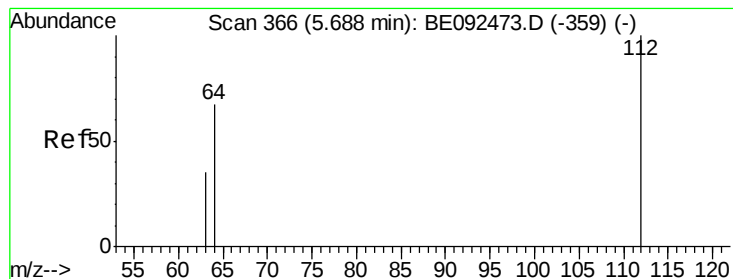

#4

2-Fluorophenol

Concen: 11.87 ng

RT: 5.66 min Scan# 362

Delta R.T. -0.02 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51

Instrument :

BNA_E

ClientSampleId :

WOOLSTON-TS-003


Tgt Ion: 112 Resp: 25072

Ion Ratio Lower Upper

112 100

64 68.4 53.5 80.3

63 36.9 27.9 41.9

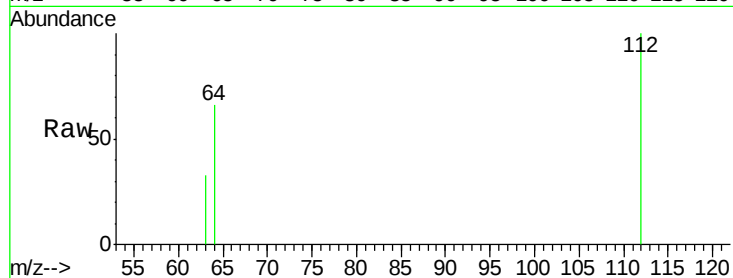




Abundance Ion 112.00 (111.70 to 112.70): BE092484.D (-314) (-)

20000

Ion 64.00 (63.70 to 64.70): BE092484.D (-314) (-)

15000

Ion 63.00 (62.70 to 63.70): BE092484.D (-314) (-)

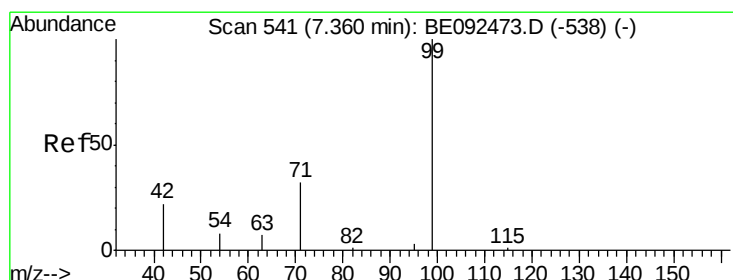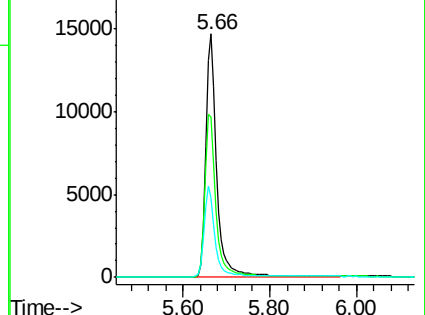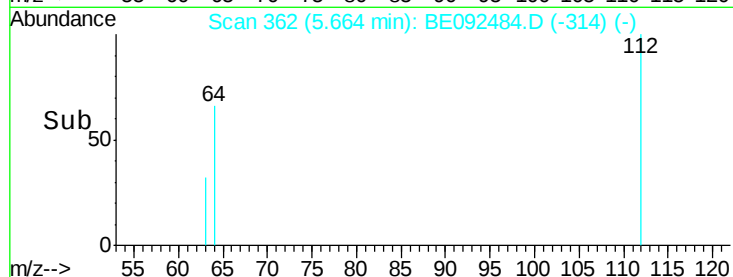

#5

Phenol-d6

Concen: 10.75 ng

RT: 7.34 min Scan# 540

Delta R.T. -0.02 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51


Tgt Ion: 99 Resp: 34140

Ion Ratio Lower Upper

99 100

42 0.0 16.0 24.0#

71 0.0 30.6 45.8#

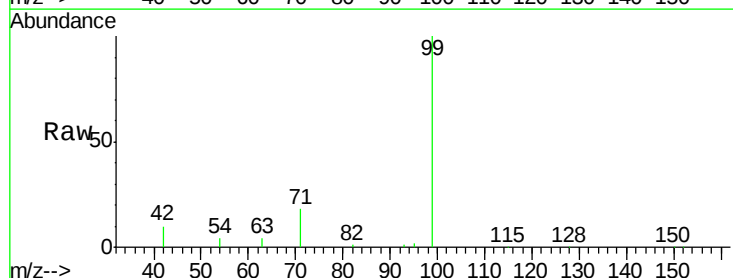



Abundance Ion 99.00 (98.70 to 99.70): BE092484.D (-528) (-)


15000

Ion 42.00 (41.70 to 42.70): BE092484.D (-528) (-)

10000

Ion 71.00 (70.70 to 71.70): BE092484.D (-528) (-)

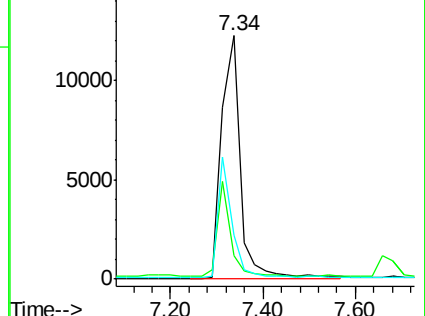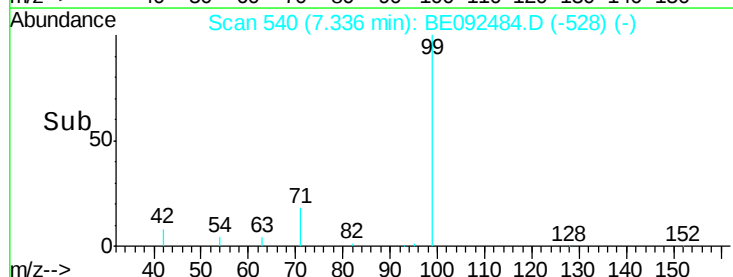

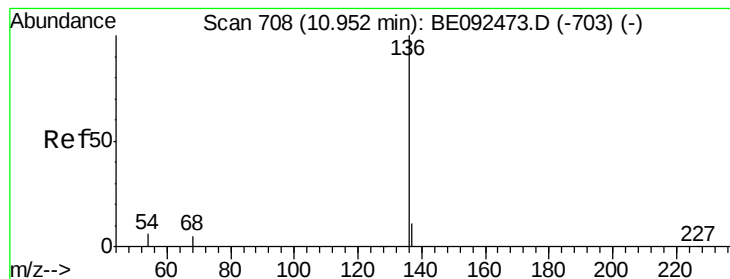

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. -0.00 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51

Instrument :

BNA_E

ClientSampleId :

WOOLSTON-TS-003

Tgt Ion:136 Resp: 52395


Ion Ratio Lower Upper

136 100

137 11.9 8.2 12.4

54 5.7 9.6 14.4#

68 4.8 6.7 10.1#



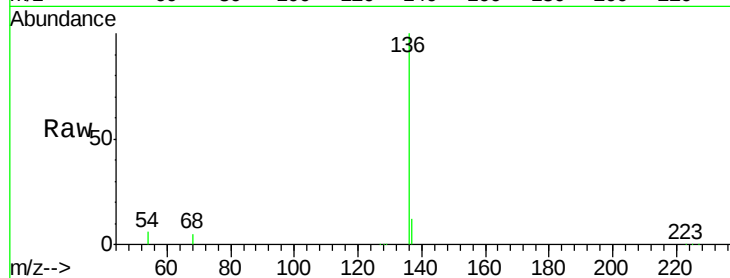


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

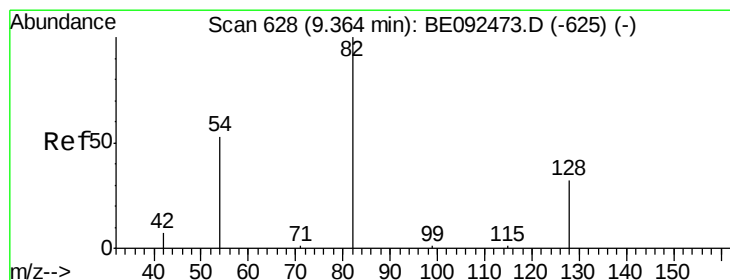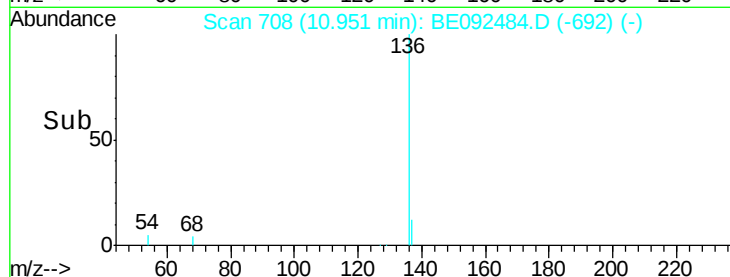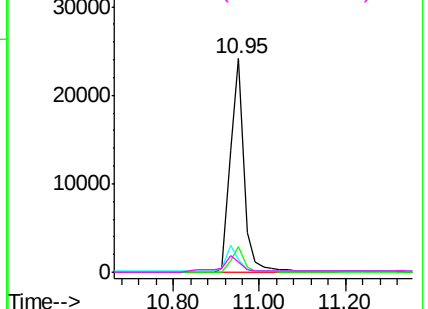

#8

Nitrobenzene-d5

Concen: 4.32 ng

RT: 9.34 min Scan# 627

Delta R.T. -0.02 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51


Tgt Ion: 82 Resp: 16029

Ion Ratio Lower Upper

82 100

128 48.9 39.0 58.4



54 44.0 44.8 67.2#

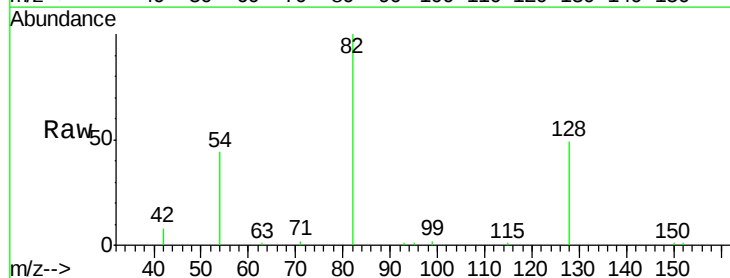


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

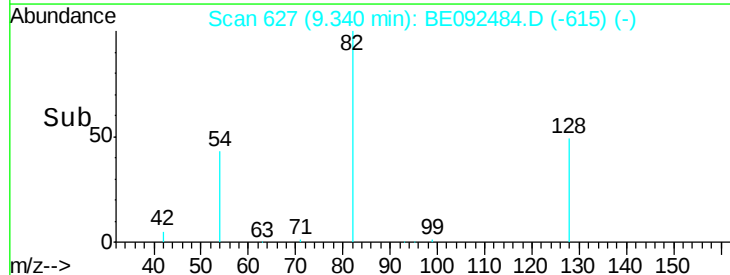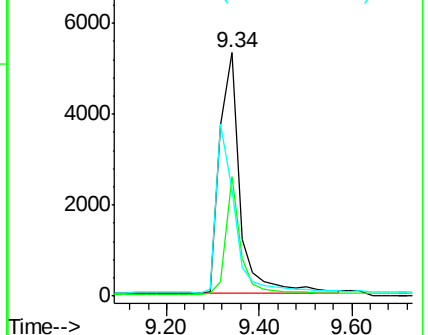

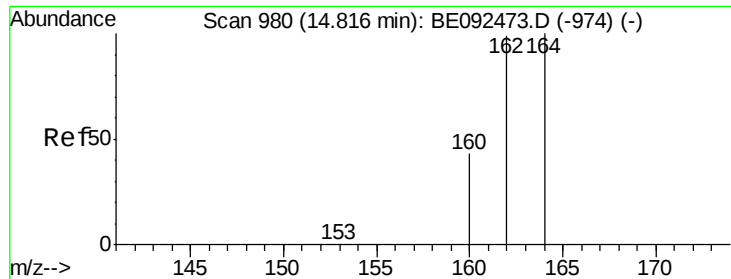

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.82 min Scan# 980

Delta R.T. -0.00 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51

Instrument :

BNA_E

ClientSampleId :

WOOLSTON-TS-003





Tgt Ion:164 Resp: 32779

Ion Ratio Lower Upper

164 100

162 97.2 71.4 107.0

160 39.9 27.4 41.2

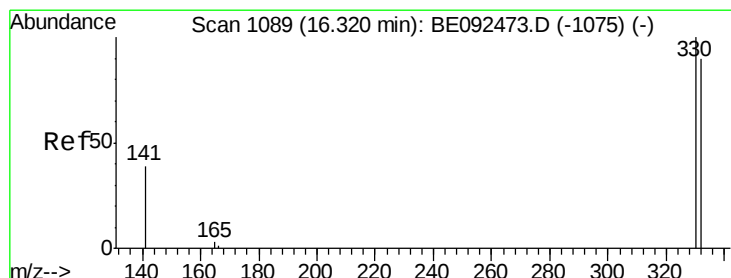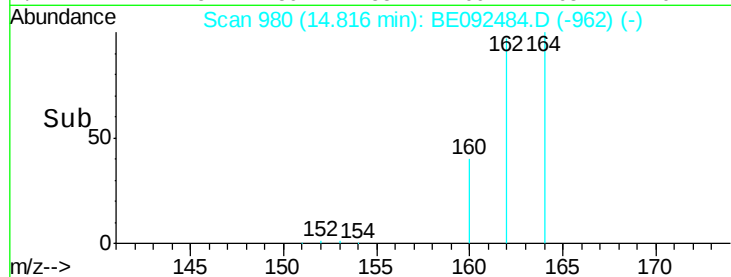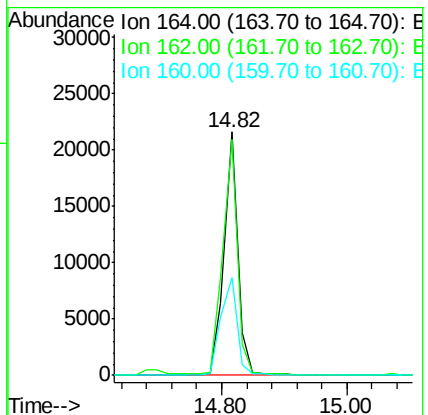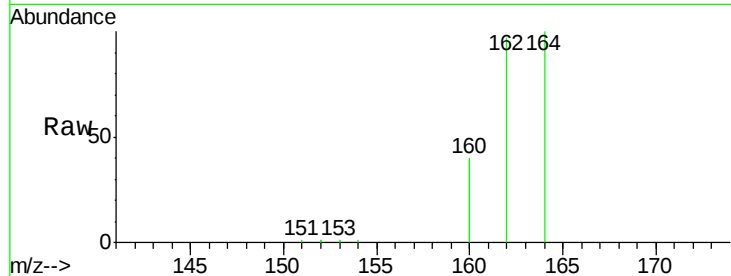

#13

2,4,6-Tribromophenol

Concen: 10.30 ng

RT: 16.31 min Scan# 1088

Delta R.T. -0.01 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51




Tgt Ion:330 Resp: 9180


Ion Ratio Lower Upper

330 100

332 96.3 75.4 113.0

141 44.4 31.0 46.6


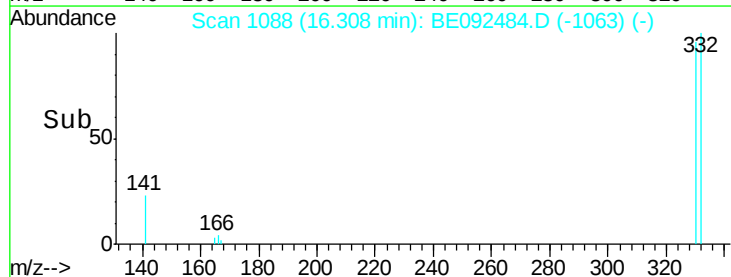
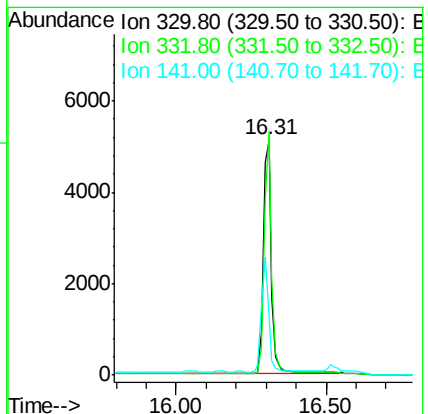
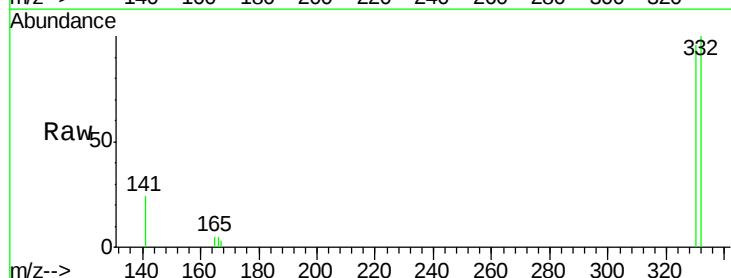


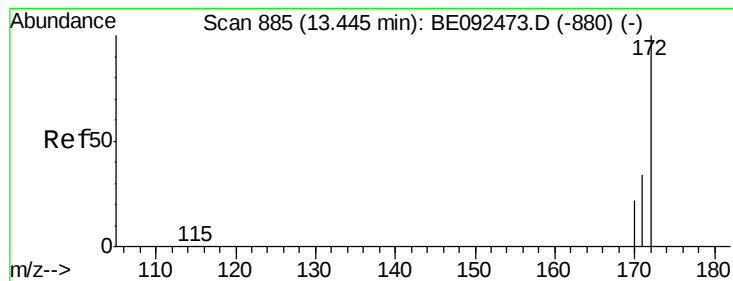

#14
 2-Fluorobiphenyl
 Concen: 4.40 ng
 RT: 13.43 min Scan# 884
 Delta R.T. -0.01 min
 Lab File: BE092484.D
 Acq: 31 Oct 2016 17:51




Instrument :
 BNA_E
 ClientSampleId :
 WOOLSTON-TS-003


Tgt Ion:172 Resp: 35168
 Ion Ratio Lower Upper
 172 100
 171 33.0 30.1 45.1
 170 21.4 21.8 32.6#

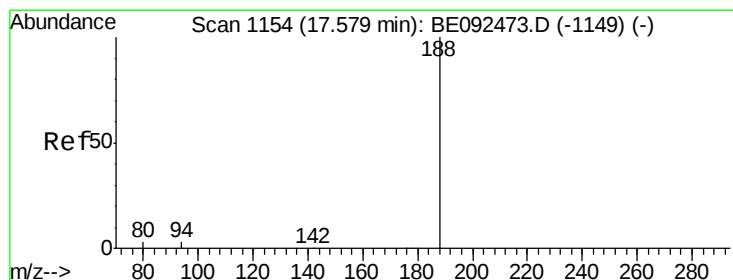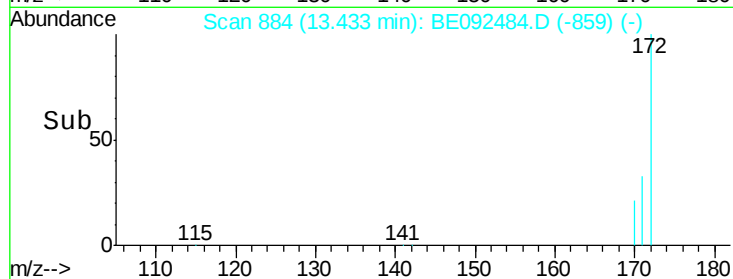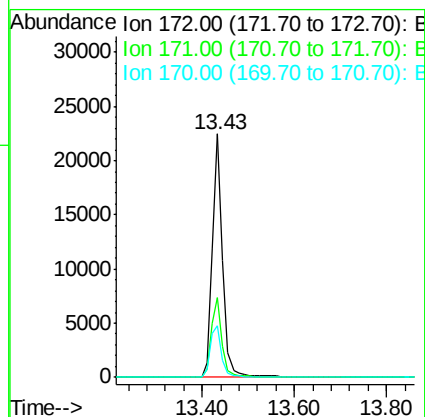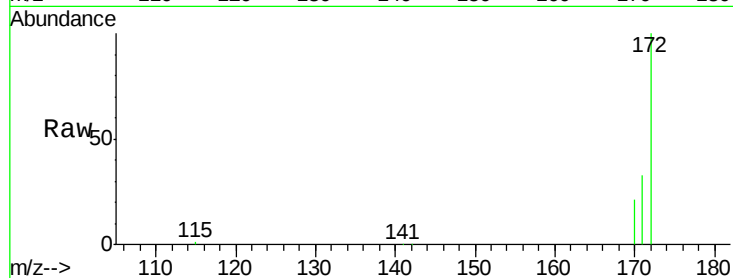

#18
 Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.56 min Scan# 1153
 Delta R.T. -0.02 min
 Lab File: BE092484.D
 Acq: 31 Oct 2016 17:51

Tgt Ion:188 Resp: 64634
 Ion Ratio Lower Upper
 188 100
 94 21.9 3.2 4.8#
 80 24.4 2.6 3.8#

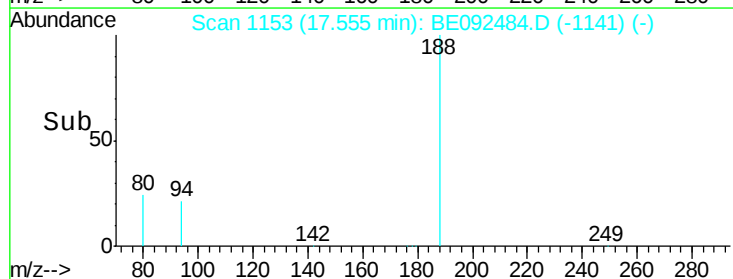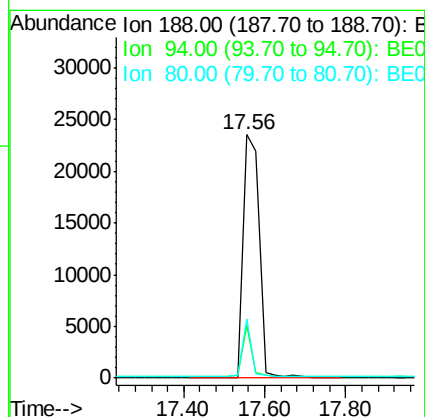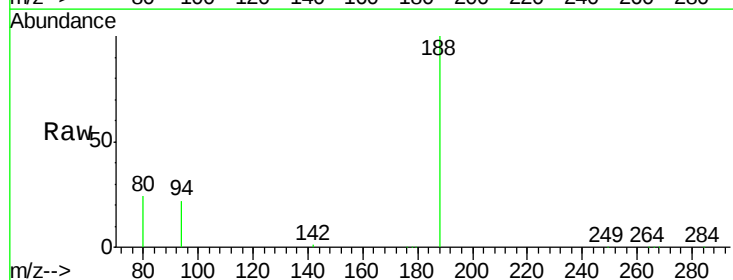

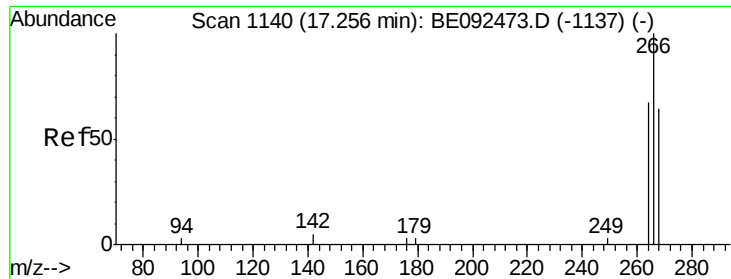

#20

Pentachlorophenol

Concen: 0.45 ng

RT: 17.23 min Scan# 1139

Delta R.T. -0.02 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51

Instrument :

BNA_E

ClientSampleId :

WOOLSTON-TS-003


Tgt Ion: 266 Resp: 163

Ion Ratio Lower Upper




266 100

268 77.1 62.5 93.7

264 81.0 57.2 85.8

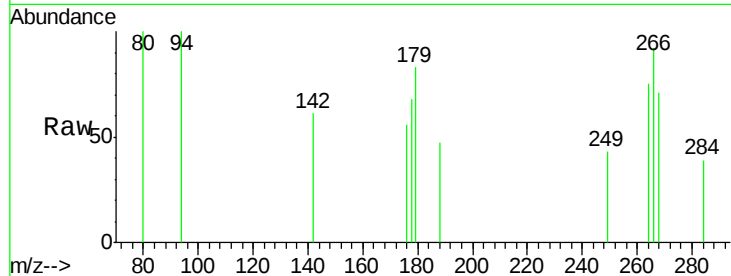

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

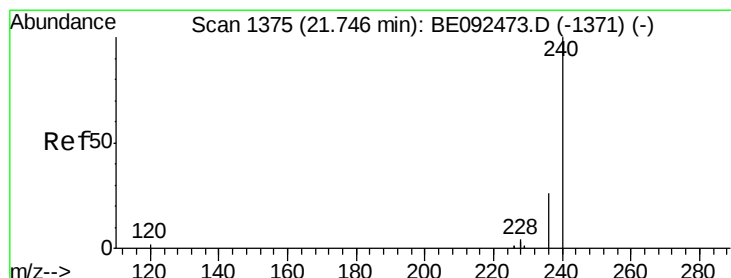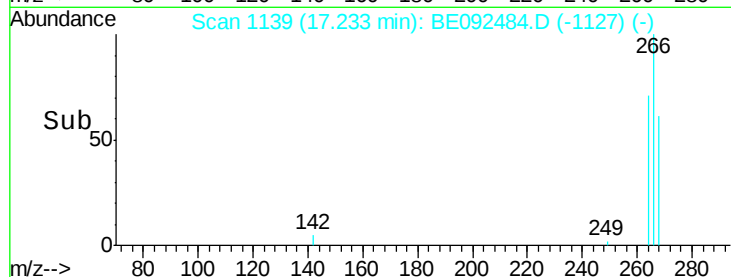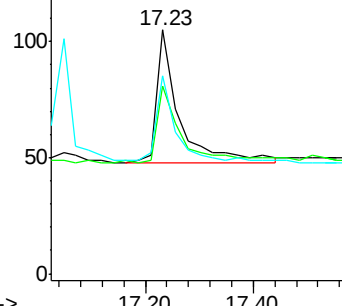

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1375

Delta R.T. 0.00 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51


Tgt Ion: 240 Resp: 93032

Ion Ratio Lower Upper



240 100


120 1.3 2.6 4.0#

236 24.5 24.6 37.0#

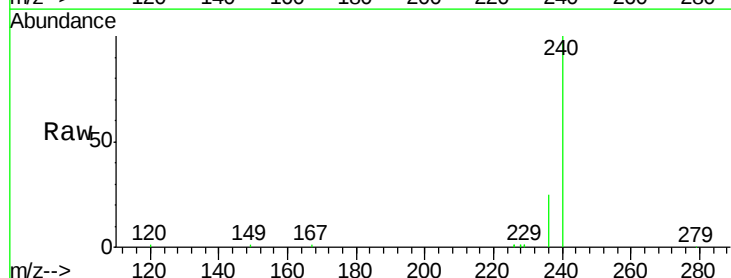

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



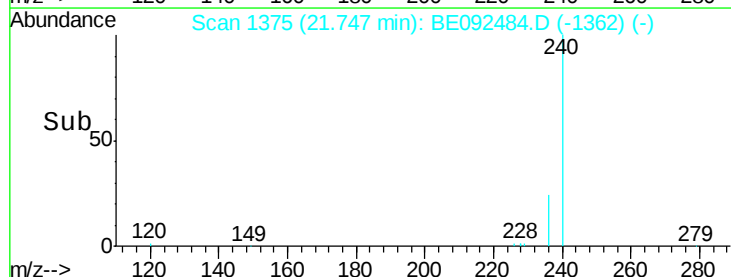
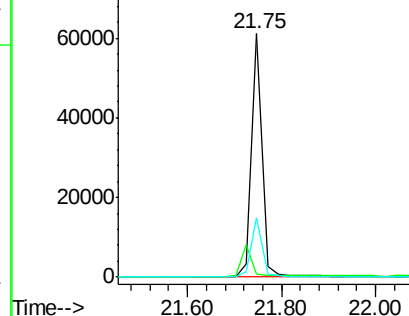


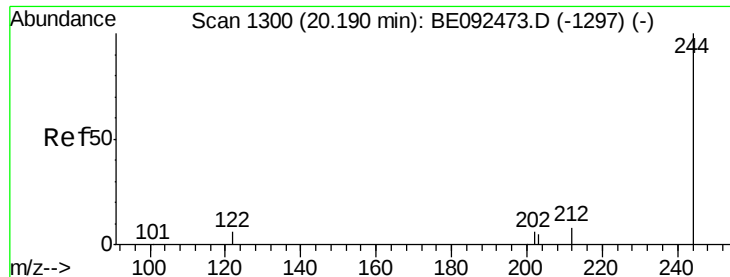

#26
 Terphenyl-d14
 Concen: 3.97 ng
 RT: 20.17 min Scan# 1299
 Delta R.T. -0.02 min
 Lab File: BE092484.D
 Acq: 31 Oct 2016 17:51




Instrument :
 BNA_E
 ClientSampleId :
 WOOLSTON-TS-003




Tgt Ion: 244 Resp: 45695
 Ion Ratio Lower Upper
 244 100
 212 9.1 6.7 10.1
 122 7.4 3.6 5.4#

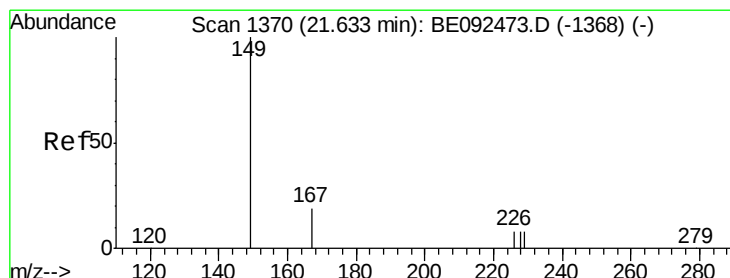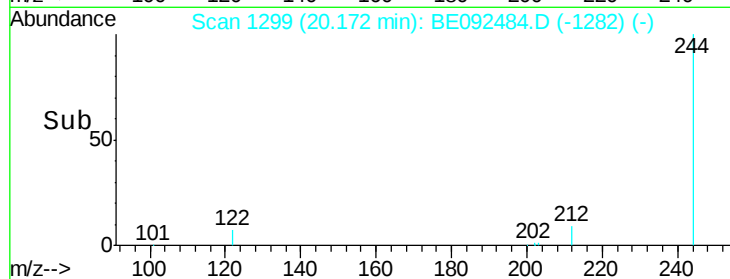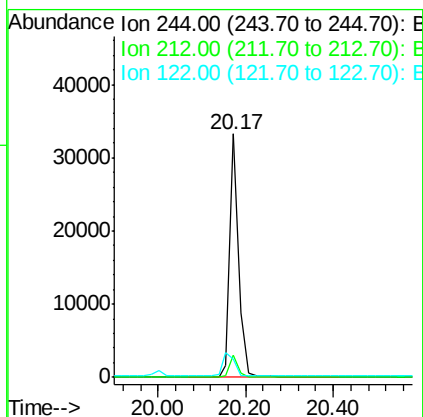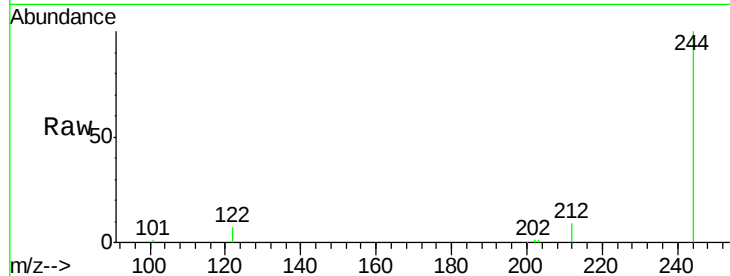

#29
 Bis(2-ethylhexyl)phthalate
 Concen: 0.75 ng
 RT: 21.63 min Scan# 1370
 Delta R.T. 0.00 min
 Lab File: BE092484.D
 Acq: 31 Oct 2016 17:51

Tgt Ion: 149 Resp: 5610
 Ion Ratio Lower Upper
 149 100
 167 24.5 16.0 24.0#
 279 0.0 16.0 24.0#

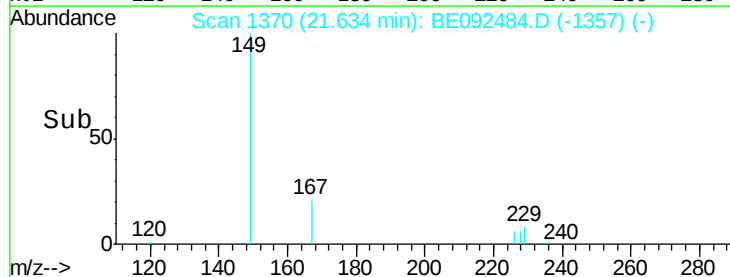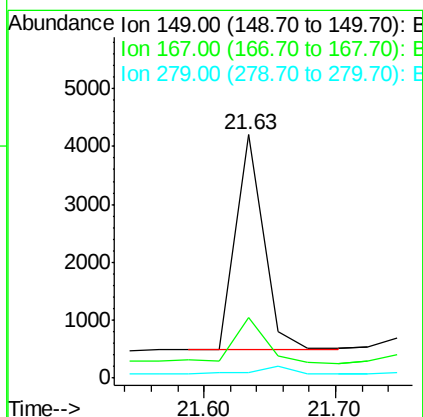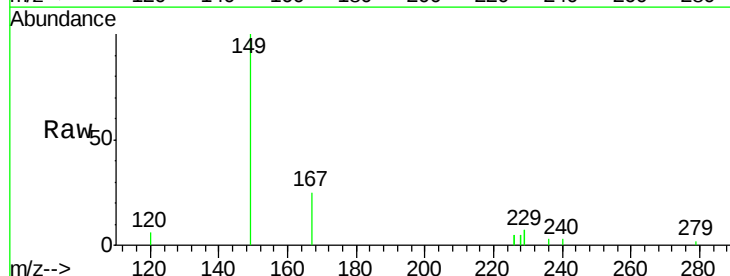

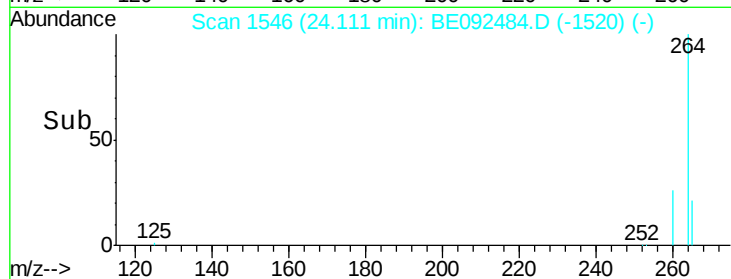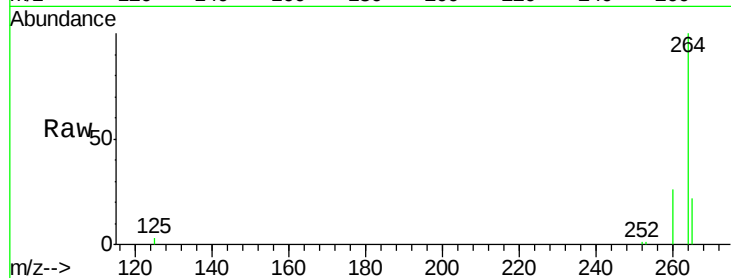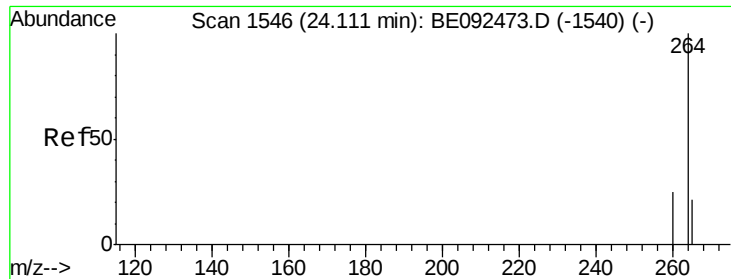

#31

Perylene-d12

Concen: 5.00 ng

RT: 24.11 min Scan# 1546

Delta R.T. -0.00 min

Lab File: BE092484.D

Acq: 31 Oct 2016 17:51

Instrument :

BNA_E

ClientSampleId :

WOOLSTON-TS-003

Tgt Ion: 264 Resp: 79388

Ion Ratio Lower Upper

264 100

260 25.8 20.1 30.1

265 21.8 17.9 26.9

