


Data Path : Z:\HPCHEM1\BNA_E\Data\BE103116\
 Data File : BE092480.D
 Acq On : 31 Oct 2016 13:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 25 15:25:33 2016

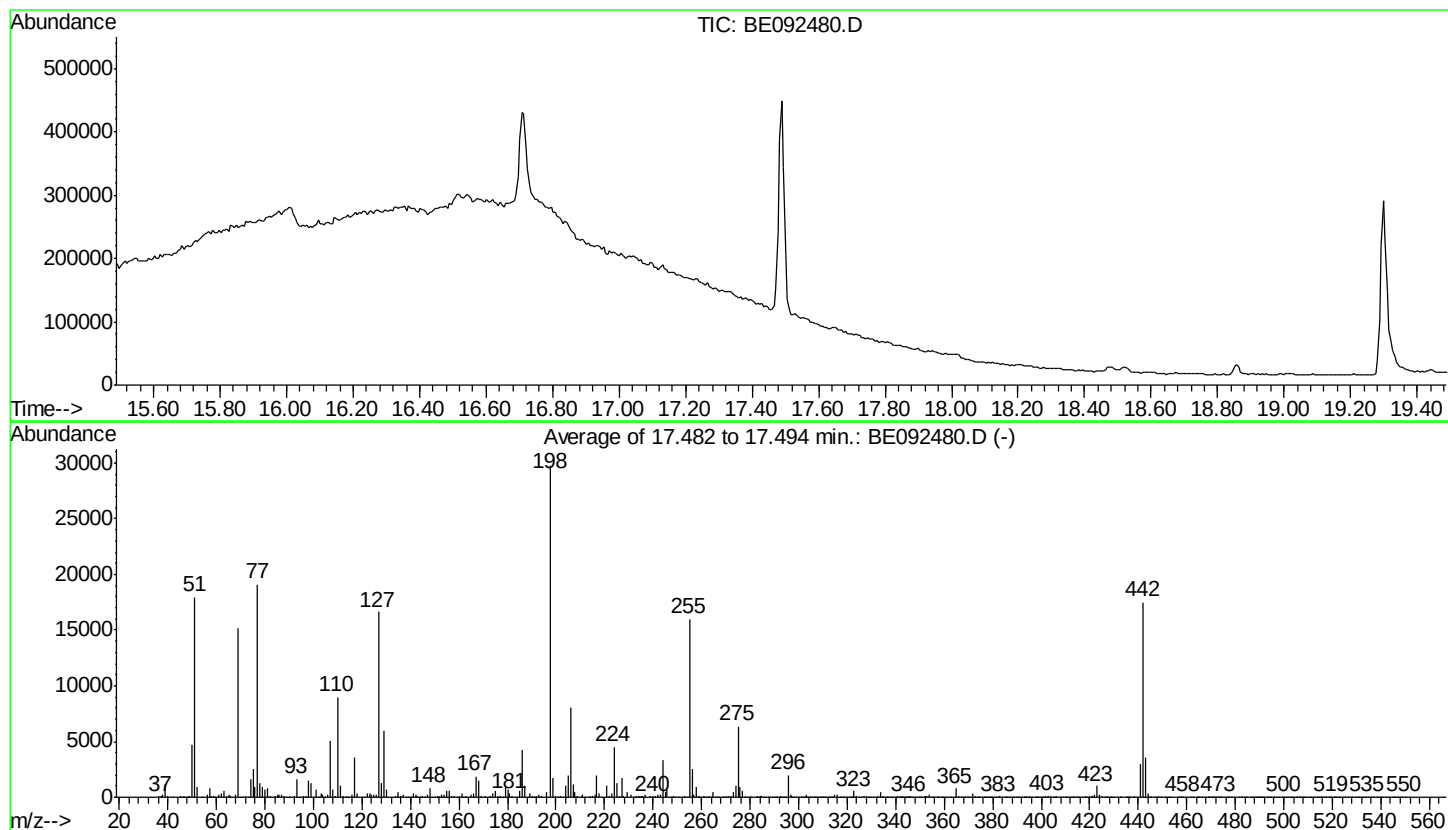

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.3	17957	PASS
68	69	0.00	2	1.5	221	PASS
69	198	0.00	100	51.0	15188	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	55.9	16635	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29756	PASS
199	198	5	9	5.9	1768	PASS
275	198	10	60	21.2	6319	PASS
365	198	1	100	2.6	764	PASS
441	442	0.01	24	16.9	2955	PASS
442	198	50	100	58.8	17501	PASS
443	442	15	24	20.6	3602	PASS