
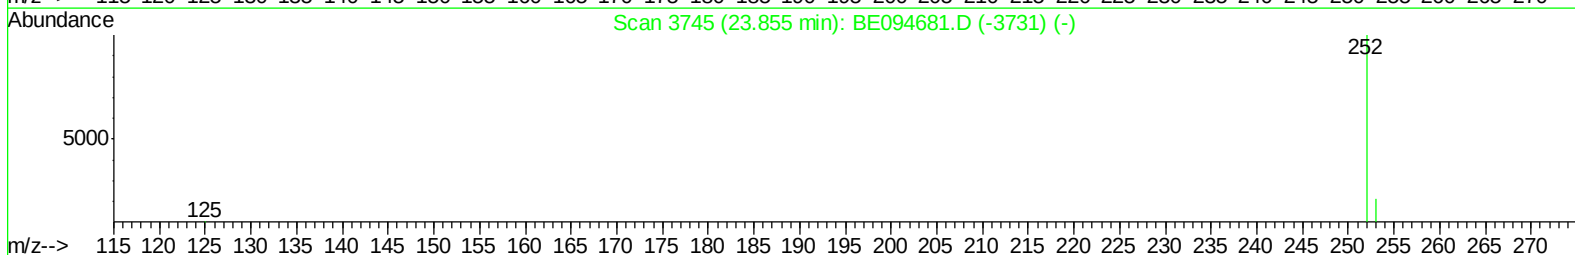
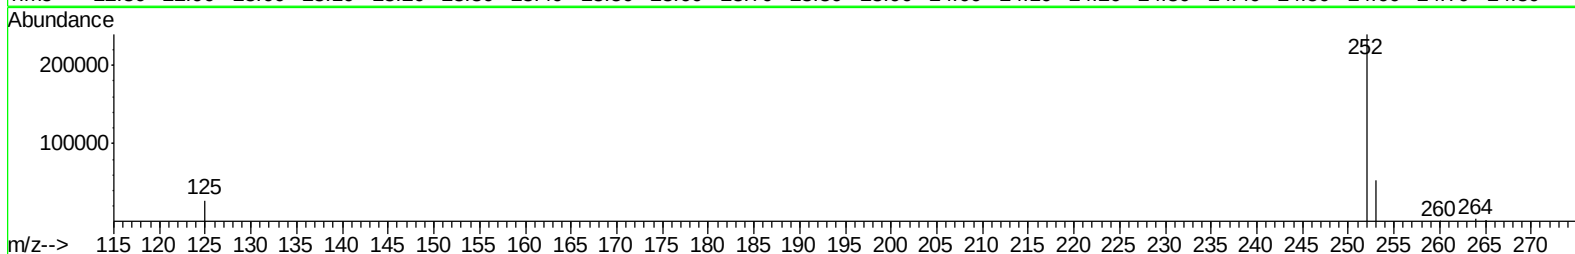


Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094682.D
Acq On : 1 Nov 2017 5:29
Operator : SJ/JU
Sample : I5844-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Nov 01 09:43:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 09:37:39 2017
Response via : Initial Calibration

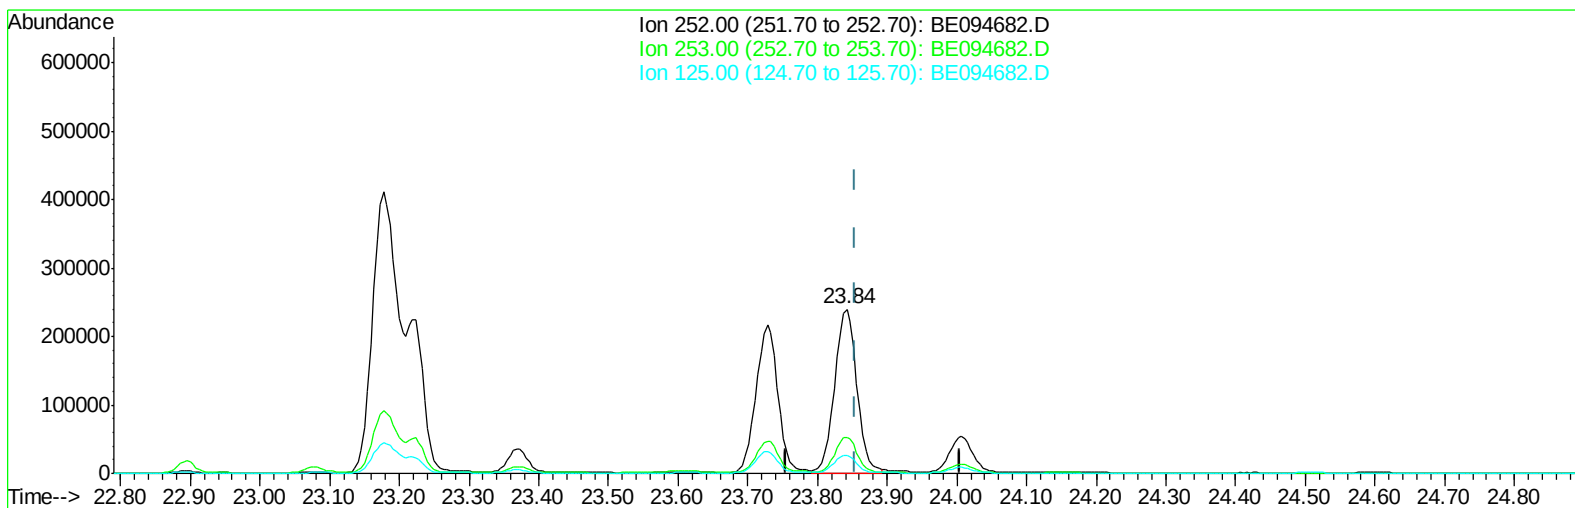

TIC: BE094682.D

(23) Benzo(a)pyrene (C)

23.842min (-0.013) 19.61ng/ul m

response 524084

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.24#
125.00	22.60	11.32#
0.00	0.00	0.00