

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094656.D
 Acq On : 31 Oct 2017 13:46
 Operator : SJ/JU
 Sample : PB103511BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 01:46:31 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 01:43:26 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1555	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	9758	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5741	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	12217	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	12289	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	17827	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2939	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	6850	0.19	ng/ul	0.00
Target Compounds						
17) Pyrene	19.65	202	898	0.02	ng/ul#	1
23) Benzo(a)pyrene	23.80	252	1742	0.03	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094656.D
Acq On : 31 Oct 2017 13:46
Operator : SJ/JU
Sample : PB103511BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 01:46:31 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration




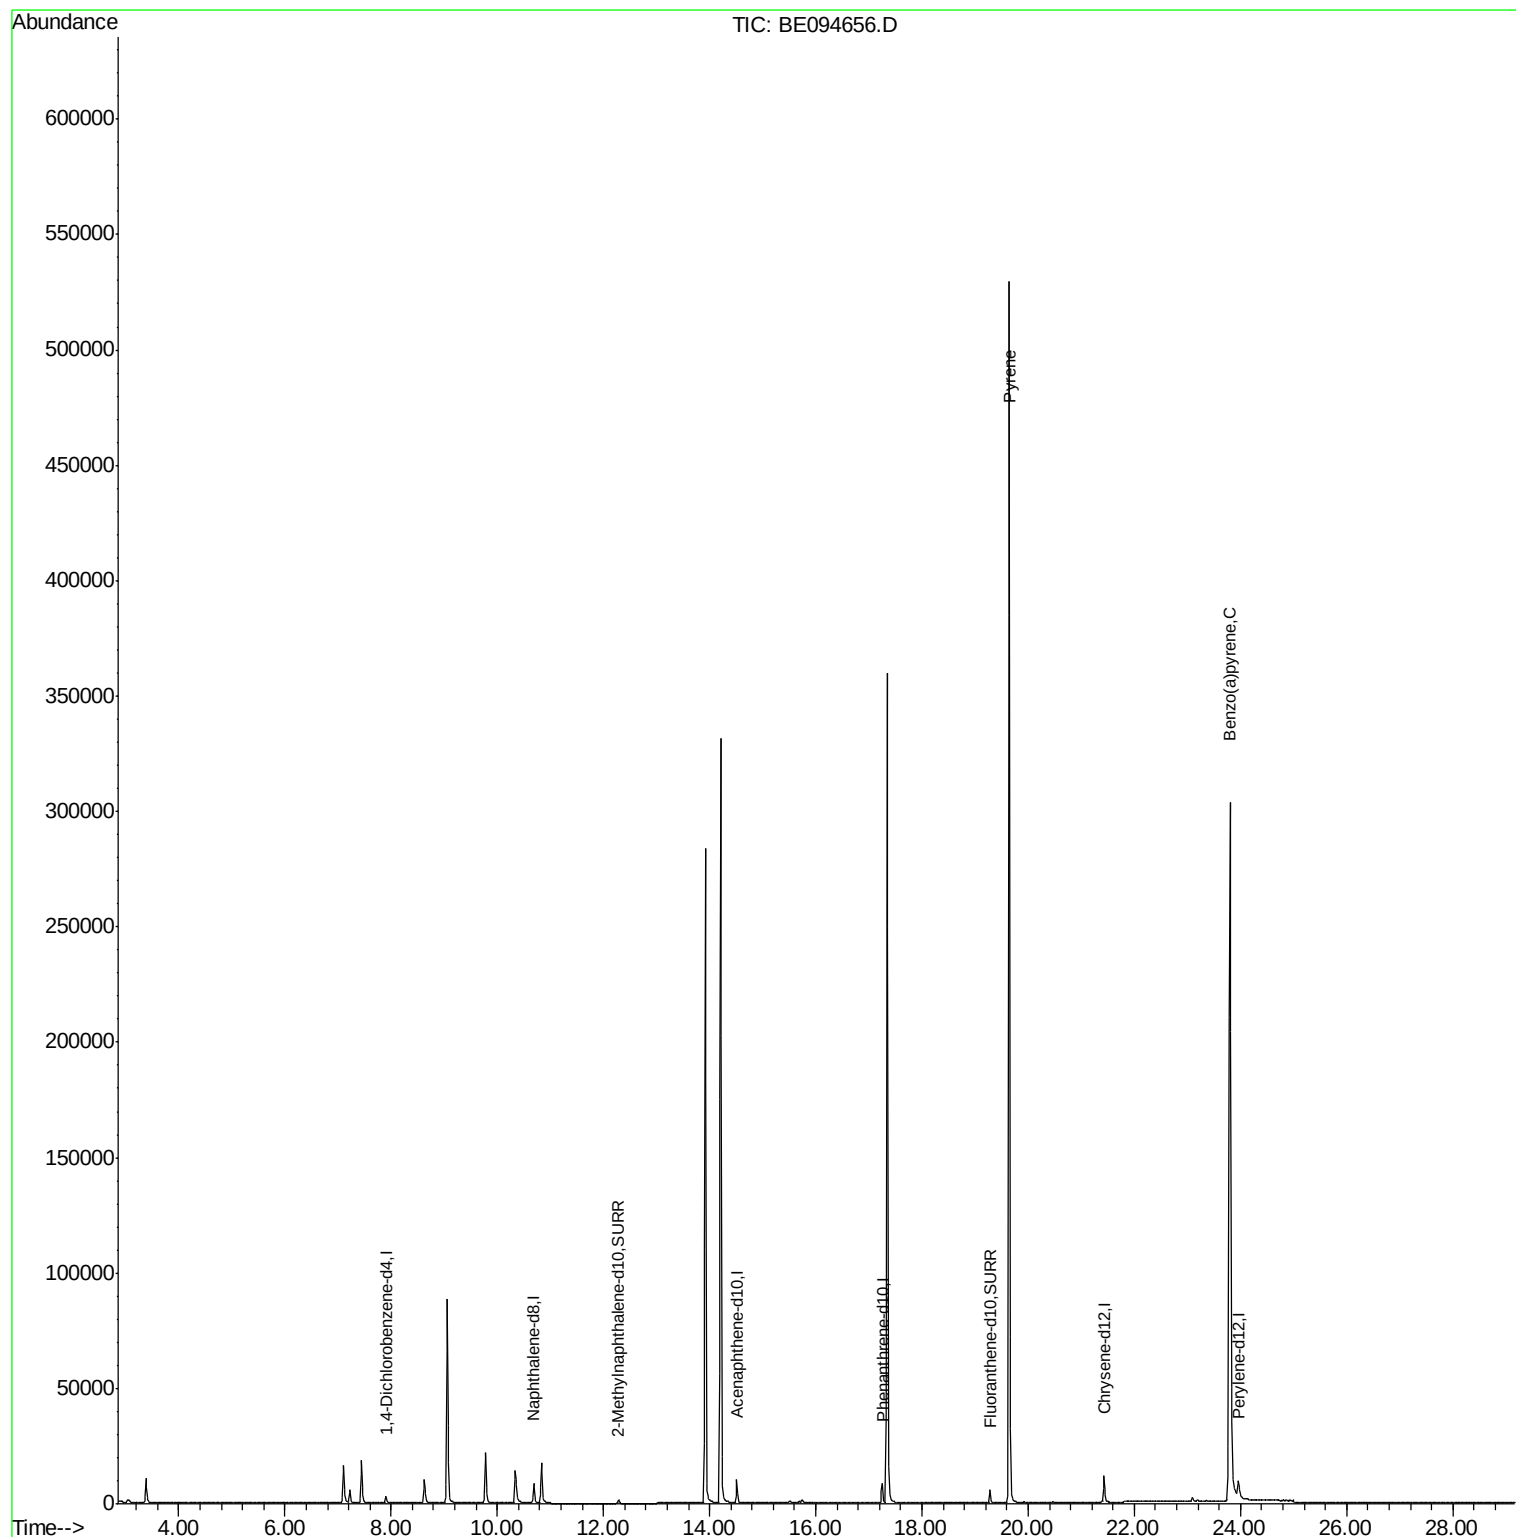


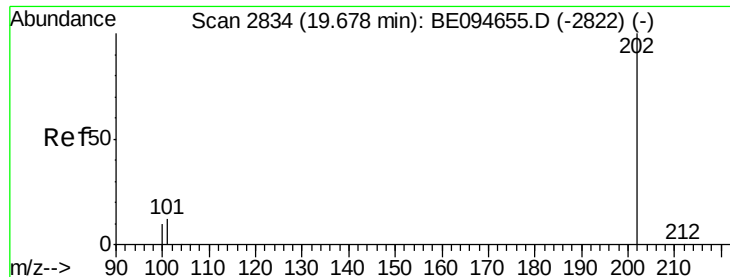

#17
Pvrene
Concen: 0.02 ng/ul
RT: 19.65 min Scan# 2827
Delta R.T. -0.03 min
Lab File: BE094656.D
Acq: 31 Oct 2017 13:46

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 898
Ion Ratio Lower Upper
202 100
101 140.9 18.2 27.4#
100 732.7 15.6 23.4#

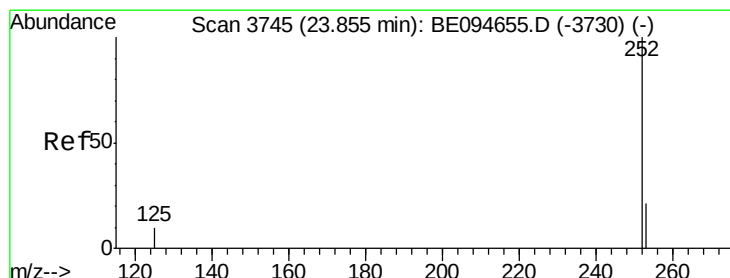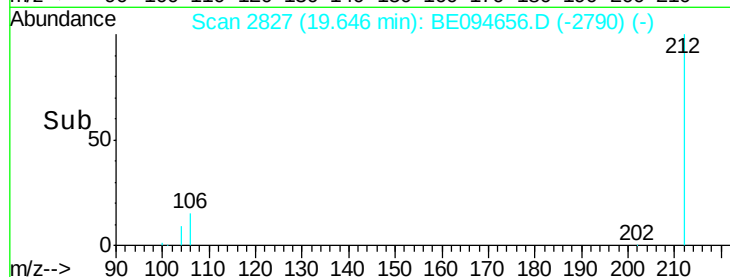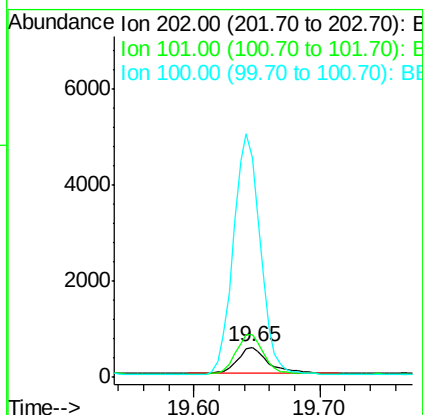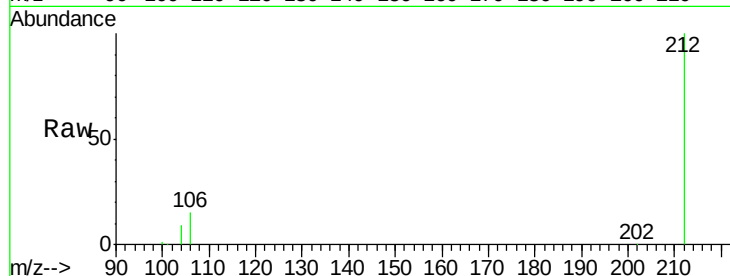

#23
Benzo(a)pyrene
Concen: 0.03 ng/ul
RT: 23.80 min Scan# 3733
Delta R.T. -0.05 min
Lab File: BE094656.D
Acq: 31 Oct 2017 13:46

Tgt Ion:252 Resp: 1742
Ion Ratio Lower Upper
252 100
253 55.9 28.5 42.7#
125 51.9 18.1 27.1#

