

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094658.D
 Acq On : 31 Oct 2017 14:58
 Operator : SJ/JU
 Sample : I5844-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 01:46:47 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 01:43:26 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1307	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	7968	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4635	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9620	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9627	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	13785	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2604	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	5986	0.21	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.80	252	1678	0.04	ng/ul#	Ovalue 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094658.D
Acq On : 31 Oct 2017 14:58
Operator : SJ/JU
Sample : I5844-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 01:46:47 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

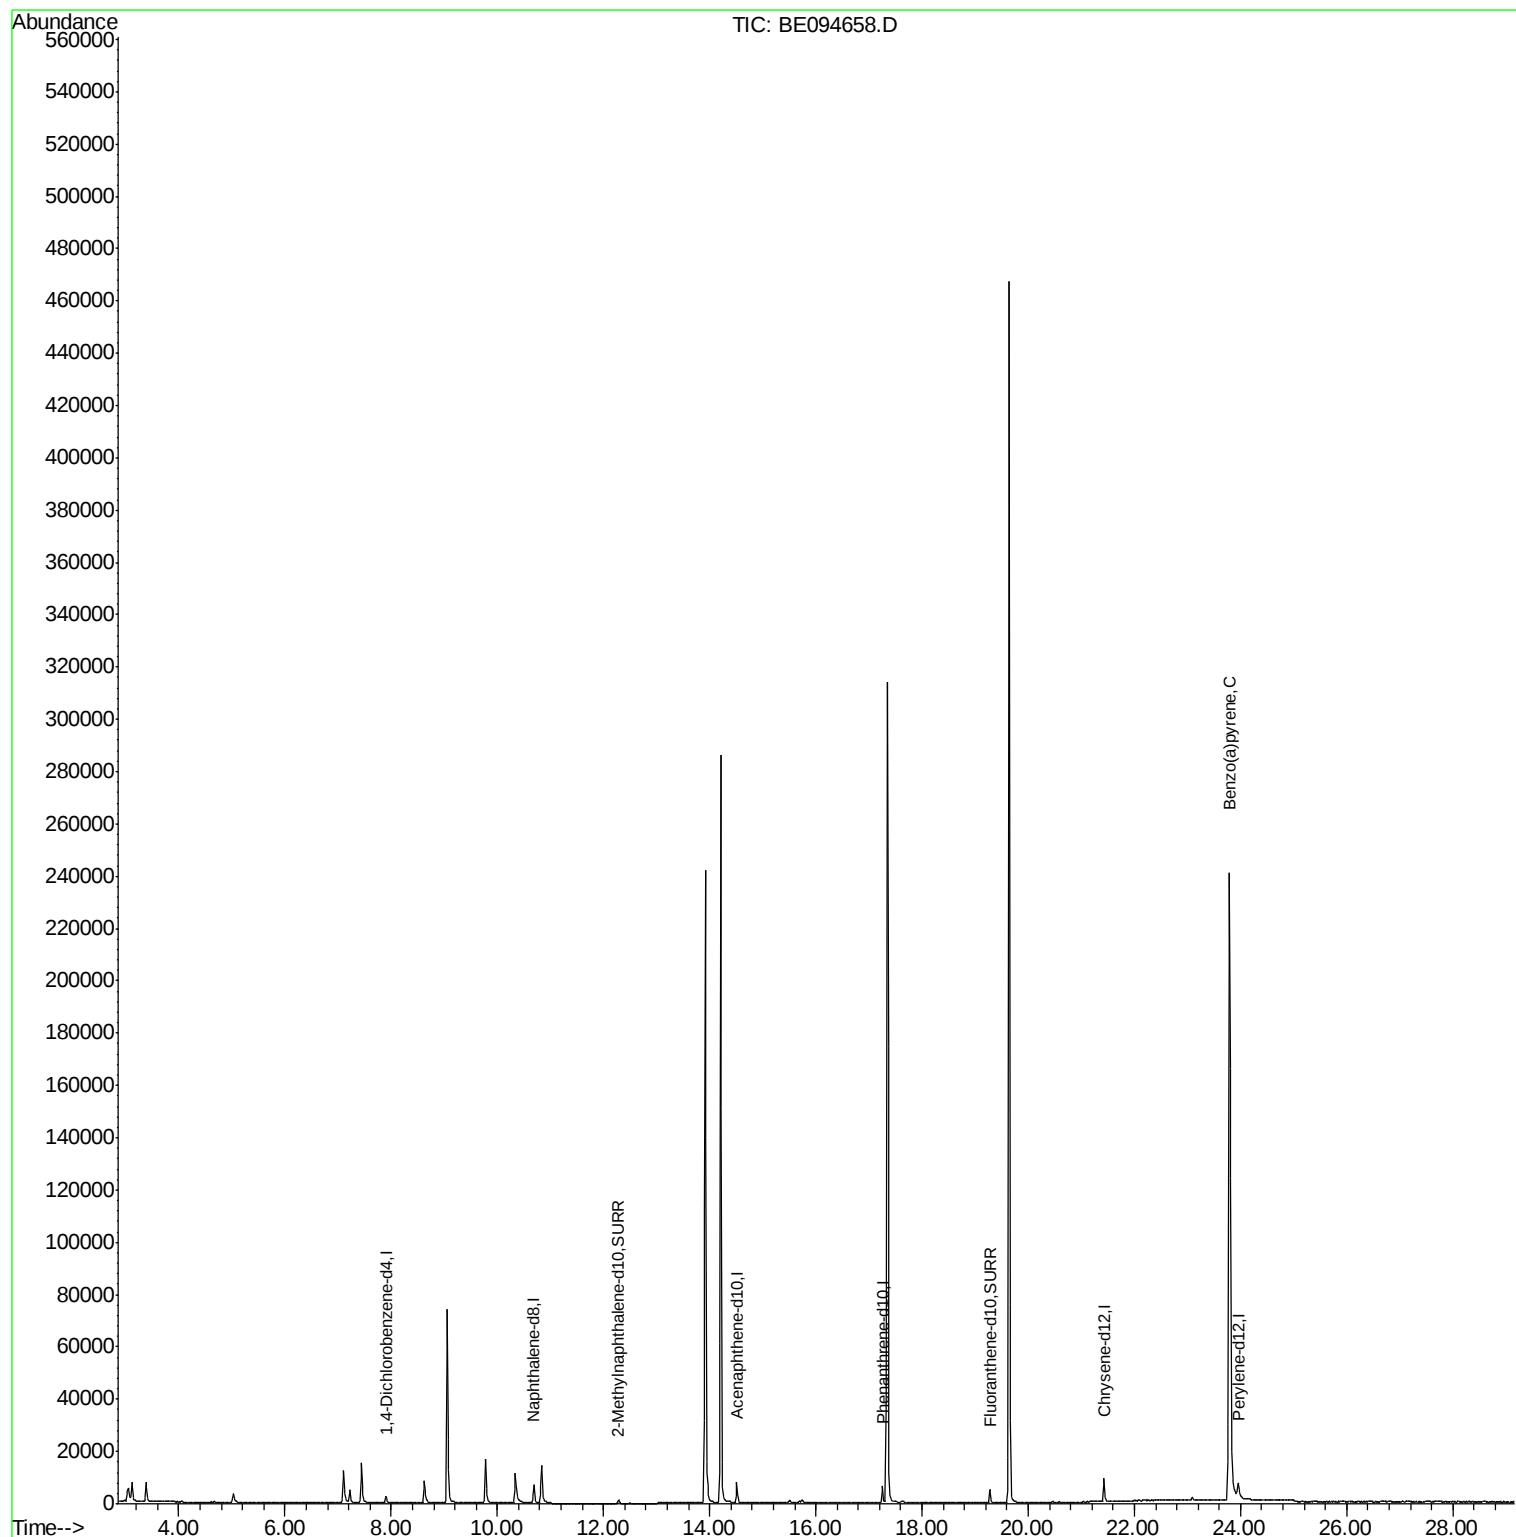

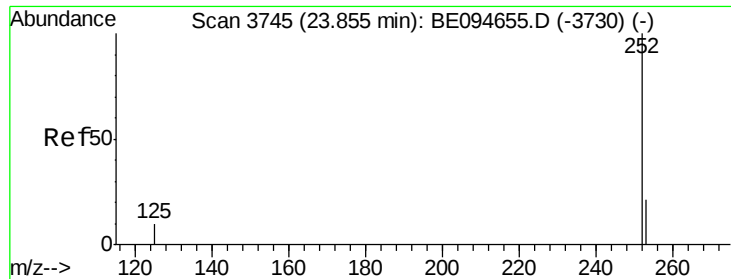

#23

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 23.80 min Scan# 3731

Delta R.T. -0.06 min


Lab File: BE094658.D

Acq: 31 Oct 2017 14:58

Instrument :

BNA_E

ClientSampleId :

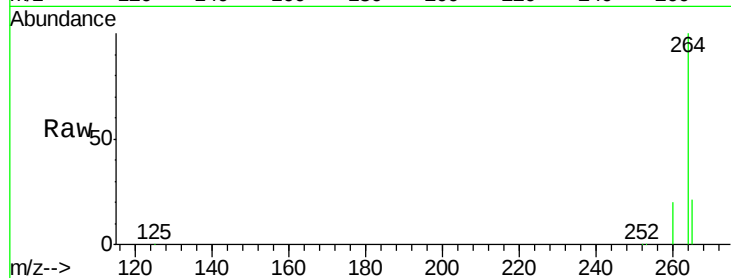


Tot Ion: 252 Resp: 1678

Ion Ratio Lower Upper

252 100

253 61.1 28.5 42.7#

125 57.8 18.1 27.1#

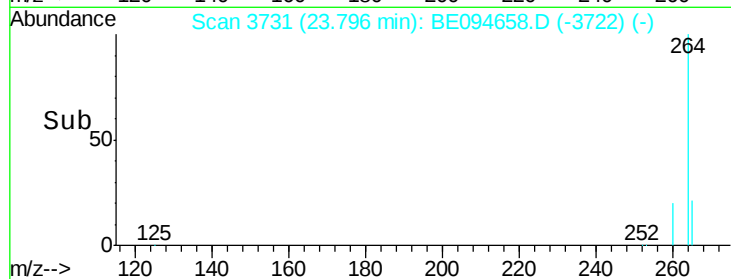

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

