

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094659.D
 Acq On : 31 Oct 2017 15:49
 Operator : SJ/JU
 Sample : PB103246BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 01:46:56 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 01:43:26 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1232	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	7641	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4370	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8953	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9049	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	15054	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3027	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	6906	0.26	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	797	0.05	ng/ul#	24
17) Pyrene	19.64	202	930	0.03	ng/ul#	1
23) Benzo(a)pyrene	23.80	252	1791	0.04	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094659.D
Acq On : 31 Oct 2017 15:49
Operator : SJ/JU
Sample : PB103246BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 01:46:56 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration




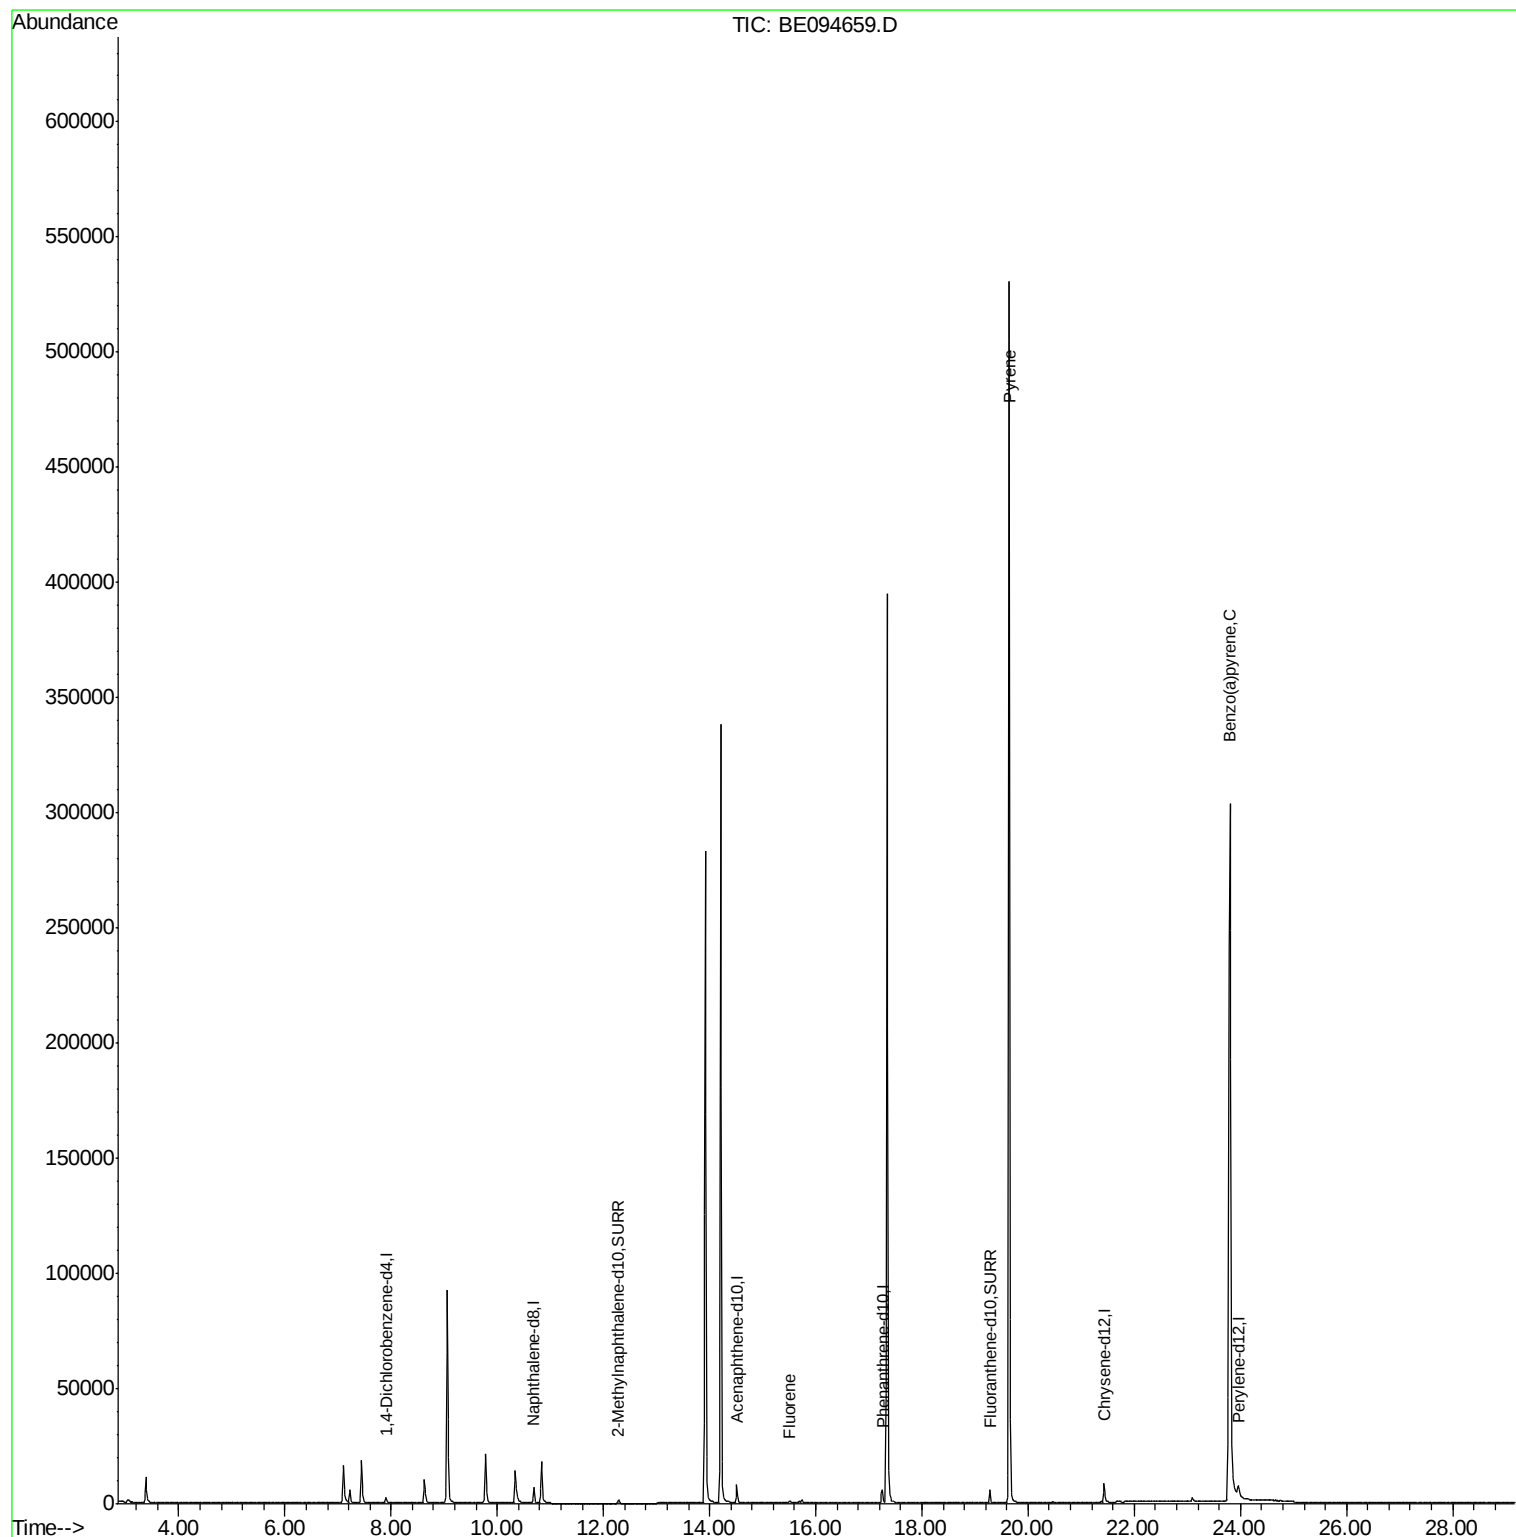


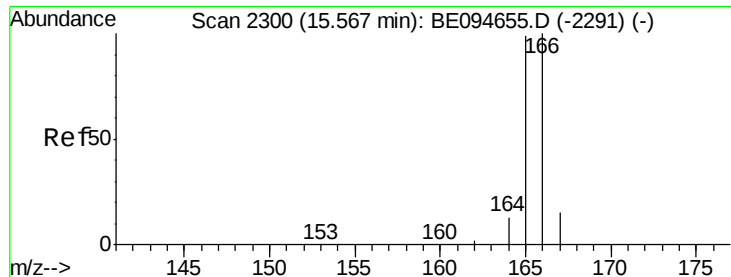

#9
Fluorene
Concen: 0.05 ng/ul
RT: 15.51 min Scan# 2292
Delta R.T. -0.06 min
Lab File: BE094659.D
Acq: 31 Oct 2017 15:49




Instrument :
BNA_E
ClientSampleId :


Tot Ion:166 Resp: 797
Ion Ratio Lower Upper
166 100
165 13.8 73.4 110.2#
167 38.0 14.6 22.0#

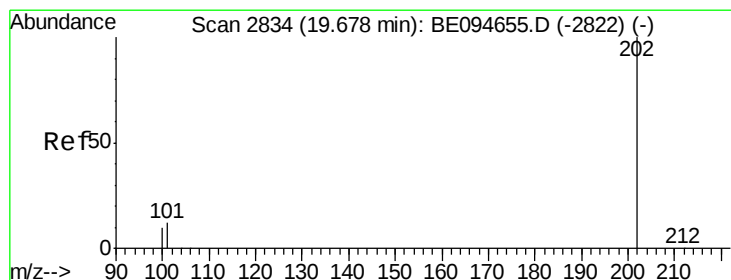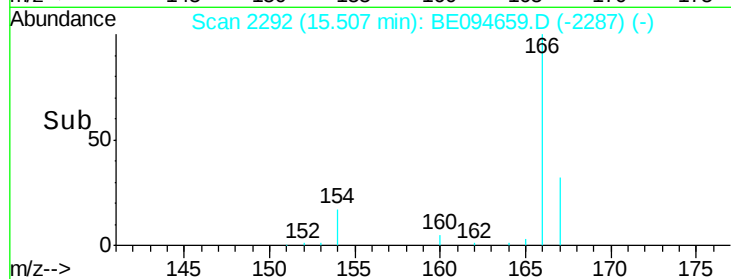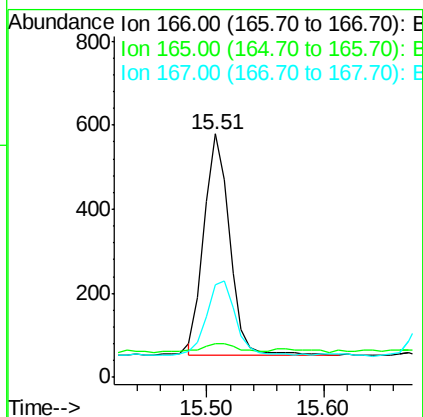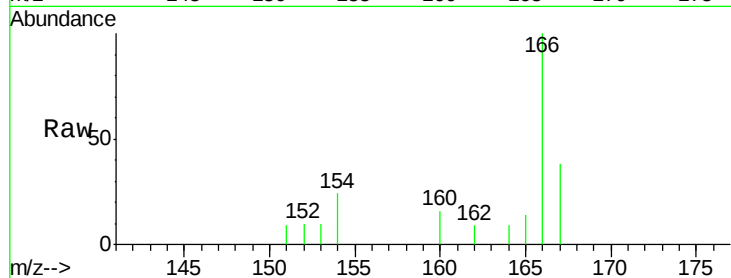

#17
Pyrene
Concen: 0.03 ng/ul
RT: 19.64 min Scan# 2826
Delta R.T. -0.03 min
Lab File: BE094659.D
Acq: 31 Oct 2017 15:49

Tgt Ion:202 Resp: 930
Ion Ratio Lower Upper
202 100
101 149.7 18.2 27.4#
100 773.2 15.6 23.4#

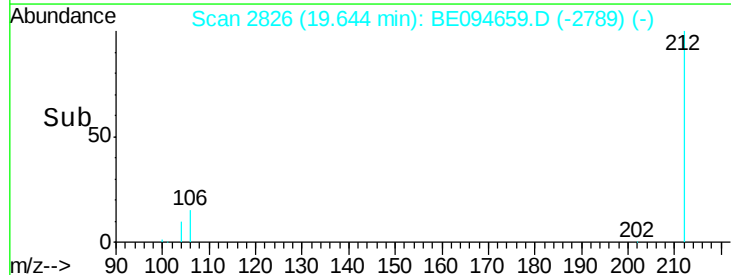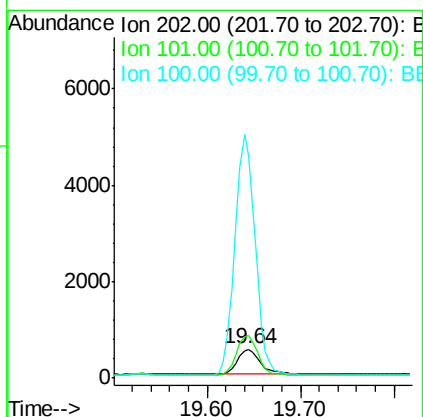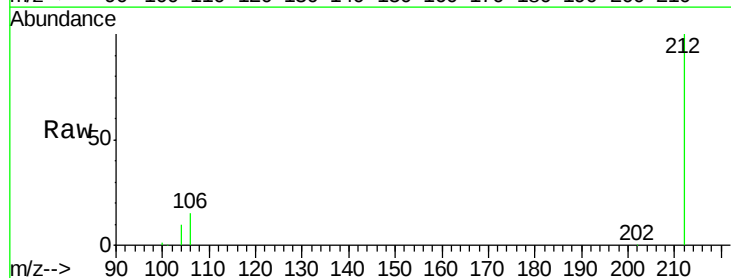

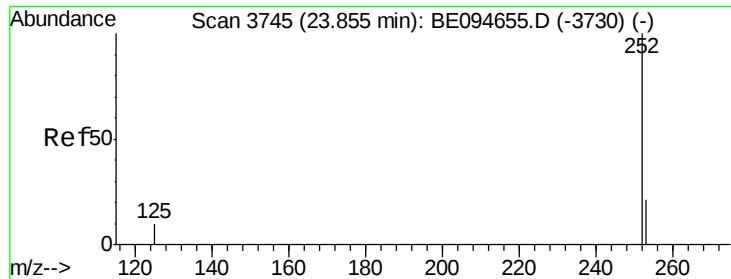

#23

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 23.80 min Scan# 3731

Delta R.T. -0.06 min


Lab File: BE094659.D

Acq: 31 Oct 2017 15:49

Instrument :

BNA_E

ClientSampleId :

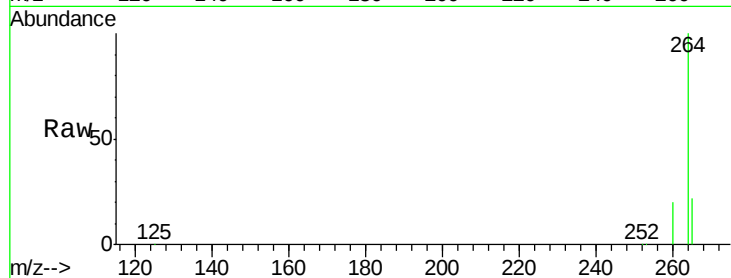

Tot Ion: 252 Resp: 1791

Ion Ratio Lower Upper

252 100

253 53.0 28.5 42.7#

125 49.4 18.1 27.1#

