

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094677.D
 Acq On : 1 Nov 2017 2:33
 Operator : SJ/JU
 Sample : I5844-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 09:13:06 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 08:49:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1315	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	7942	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4463	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9161	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9391	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	15152	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2178	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	5549	0.20	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	943	0.03	ng/ul#	1
23) Benzo(a)pyrene	23.79	252	1437	0.03	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094677.D
Acq On : 1 Nov 2017 2:33
Operator : SJ/JU
Sample : I5844-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 09:13:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

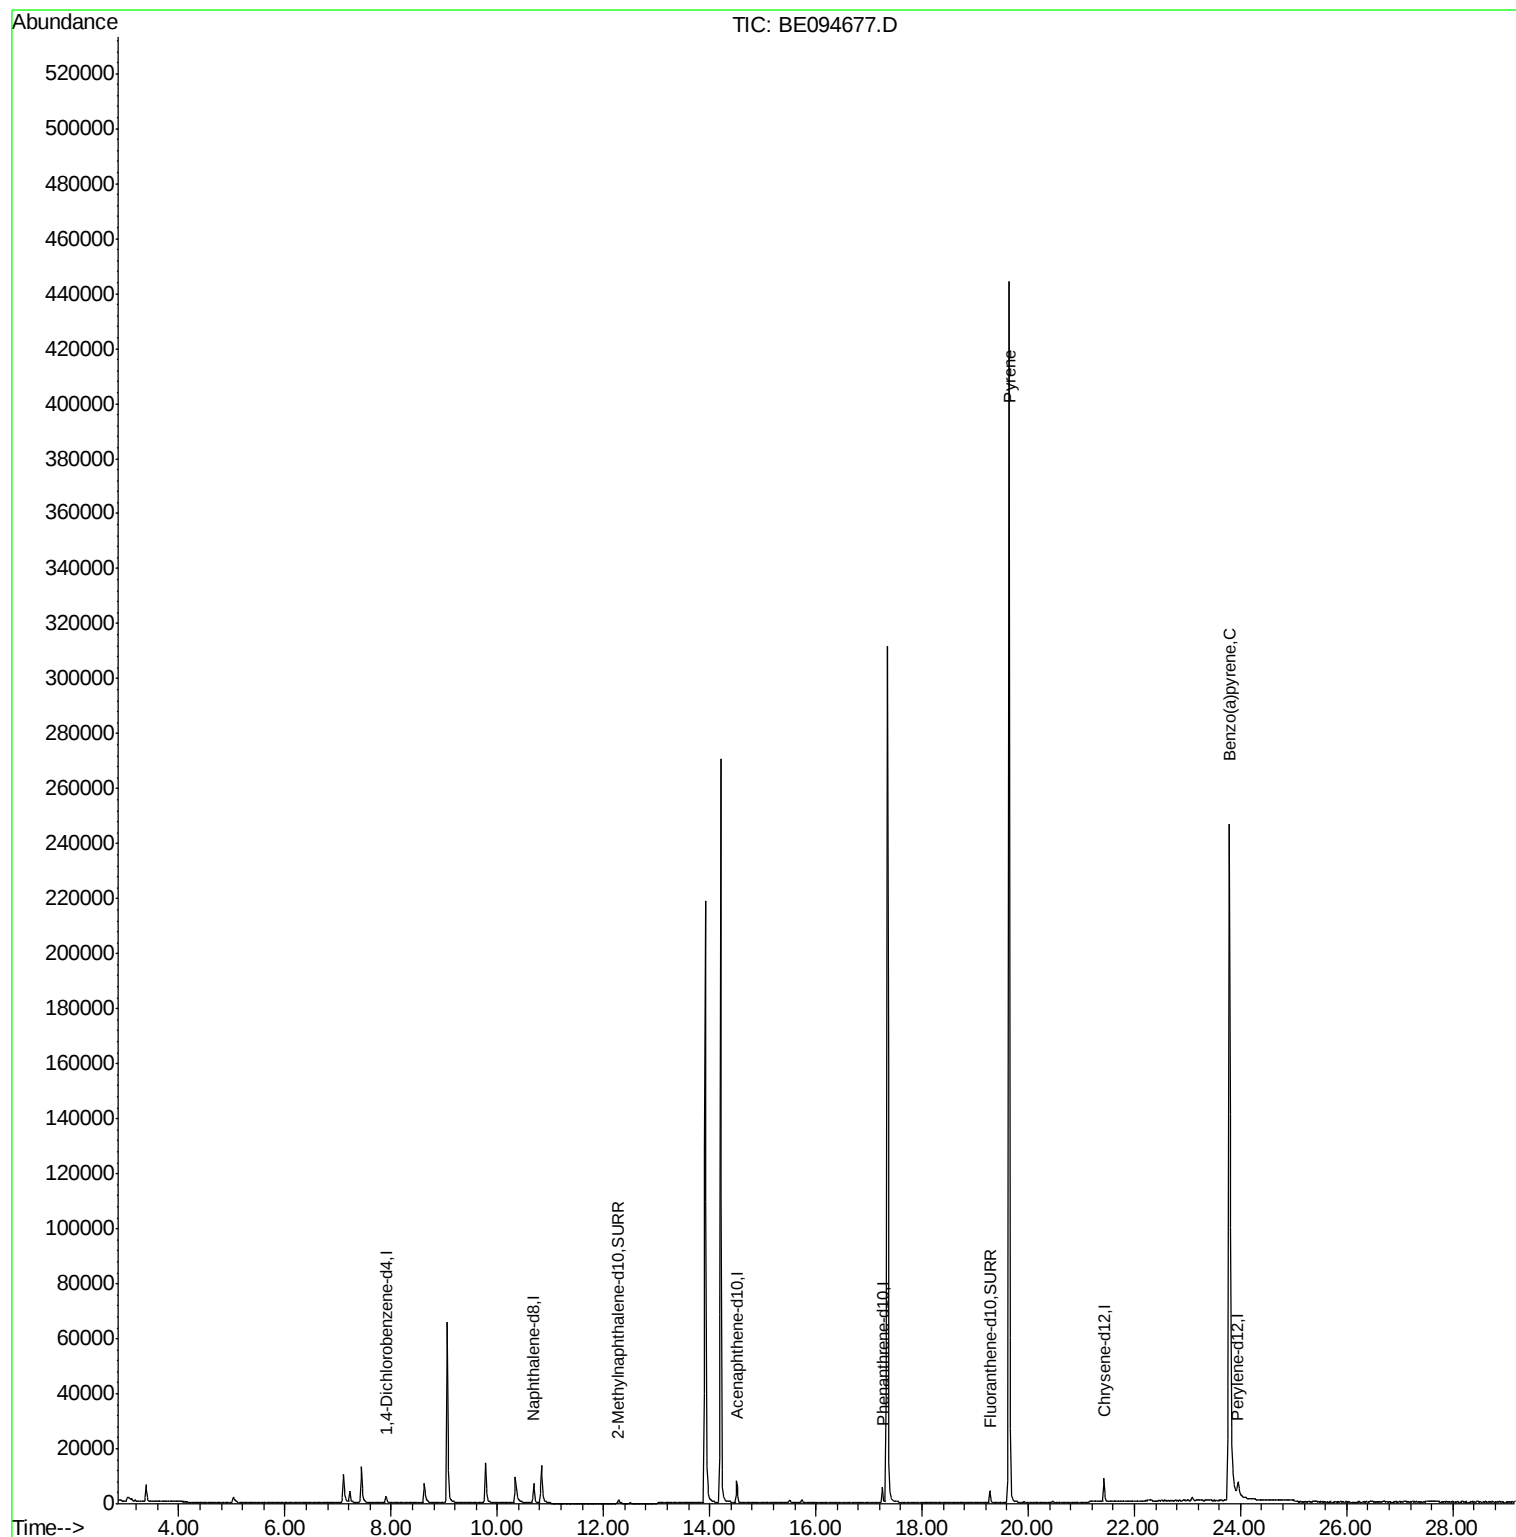


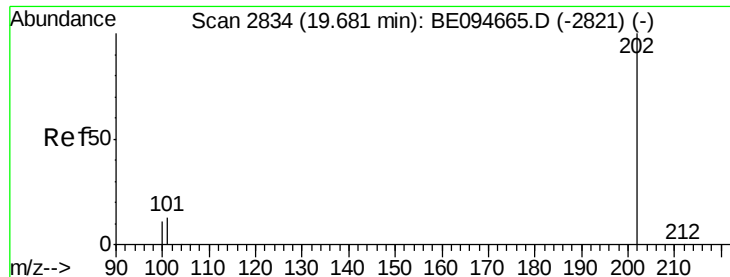




#17
Pvrene
Concen: 0.03 ng/ul
RT: 19.64 min Scan# 2825
Delta R.T. -0.04 min
Lab File: BE094677.D
Acq: 1 Nov 2017 2:33

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 943
Ion Ratio Lower Upper
202 100
101 150.4 18.2 27.4#
100 767.9 15.6 23.4#

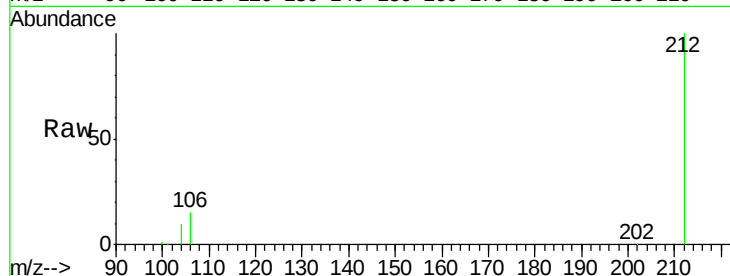


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): BE

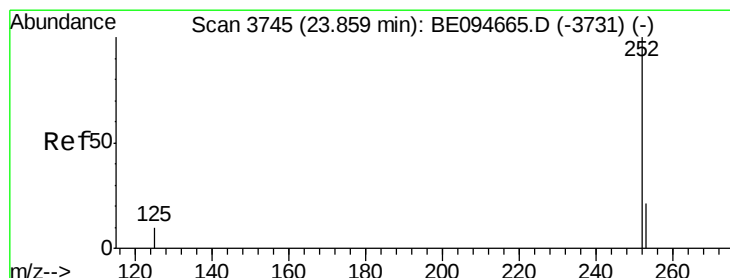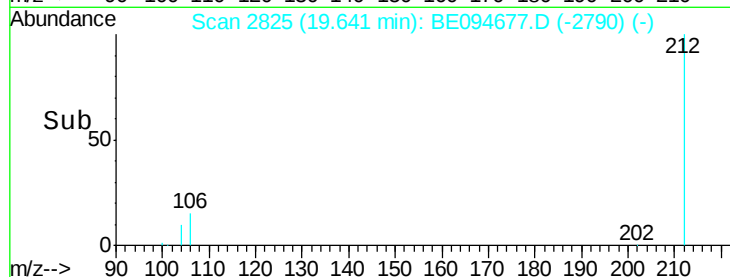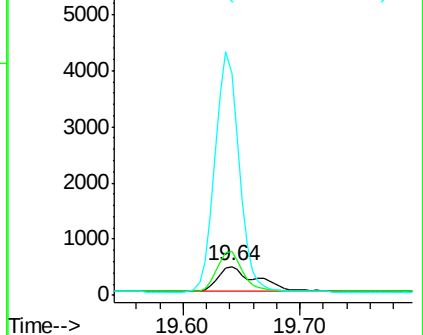

#23
Benzo(a)pyrene
Concen: 0.03 ng/ul
RT: 23.79 min Scan# 3730
Delta R.T. -0.07 min
Lab File: BE094677.D
Acq: 1 Nov 2017 2:33

Tgt Ion:252 Resp: 1437
Ion Ratio Lower Upper
252 100
253 54.4 28.5 42.7#
125 61.3 18.1 27.1#

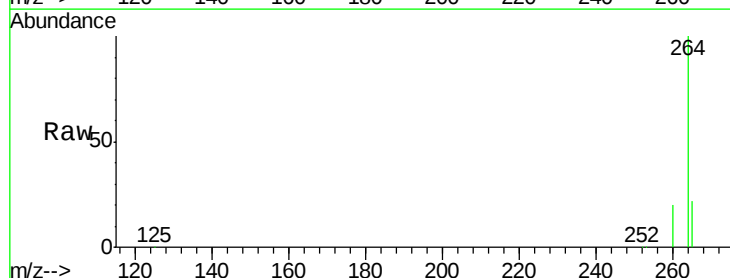

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

