

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094678.D
 Acq On : 1 Nov 2017 3:09
 Operator : SJ/JU
 Sample : I5844-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 09:13:15 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 08:49:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1419	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	8594	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4999	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.43	240	10304	0.40	ng/ul	0.00
20) Perylene-d12	23.95	264	19755	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	4106	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	9920	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	1330	0.04	ng/ul#	1
23) Benzo(a)pyrene	23.79	252	2464	0.04	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094678.D
Acq On : 1 Nov 2017 3:09
Operator : SJ/JU
Sample : I5844-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 09:13:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration




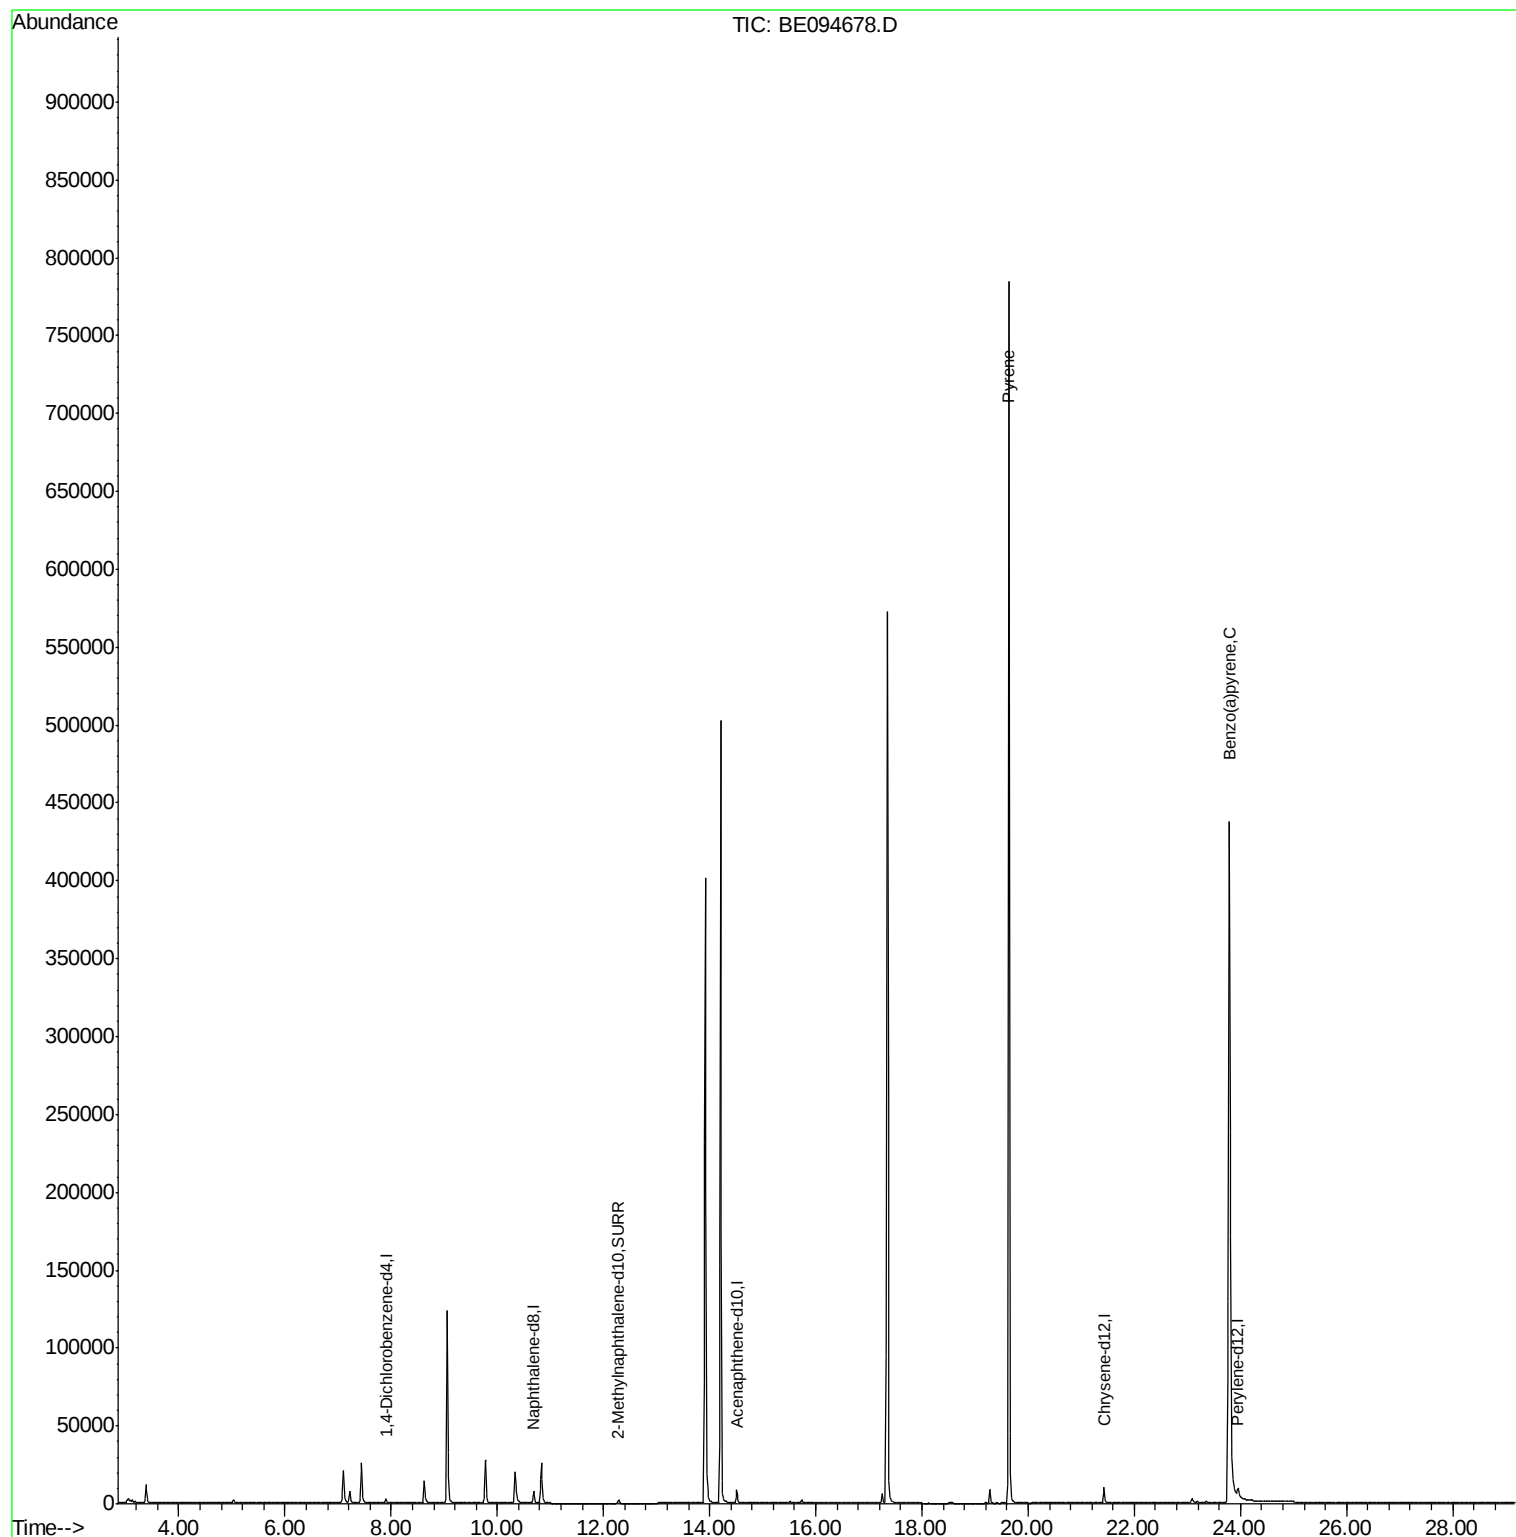


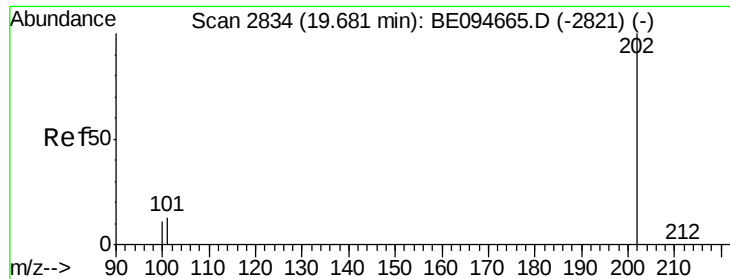

#17
Pvrene
Concen: 0.04 ng/ul
RT: 19.64 min Scan# 2825
Delta R.T. -0.04 min
Lab File: BE094678.D
Acq: 1 Nov 2017 3:09

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 1330
Ion Ratio Lower Upper
202 100
101 155.2 18.2 27.4#
100 837.3 15.6 23.4#

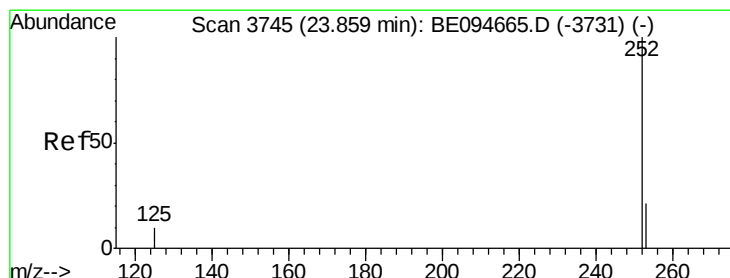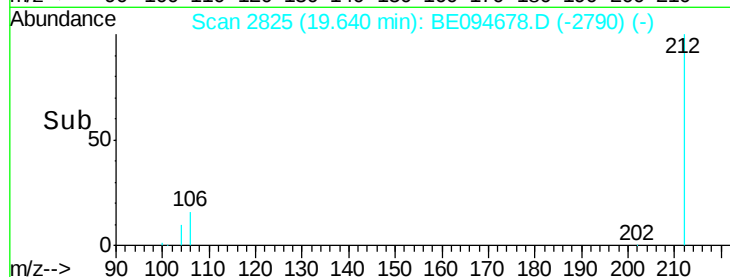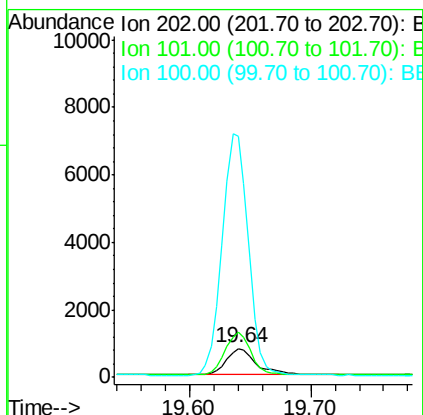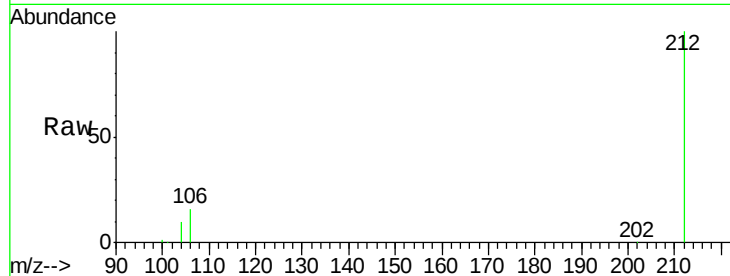

#23
Benzo(a)pyrene
Concen: 0.04 ng/ul
RT: 23.79 min Scan# 3730
Delta R.T. -0.07 min
Lab File: BE094678.D
Acq: 1 Nov 2017 3:09

Tgt Ion:252 Resp: 2464
Ion Ratio Lower Upper
252 100
253 46.8 28.5 42.7#
125 45.5 18.1 27.1#

