

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094680.D
 Acq On : 1 Nov 2017 4:18
 Operator : SJ/JU
 Sample : I5844-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Nov 01 09:13:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 08:49:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1544	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.68	136	9235	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	5270	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.43	240	10438	0.40	ng/ul	0.00
20) Perylene-d12	23.79	264	685257	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	4865	0.32	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	11588	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.51	166	1209	0.06	ng/ul#	21
17) Pyrene	19.64	202	1880	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Nov 01 09:13:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration




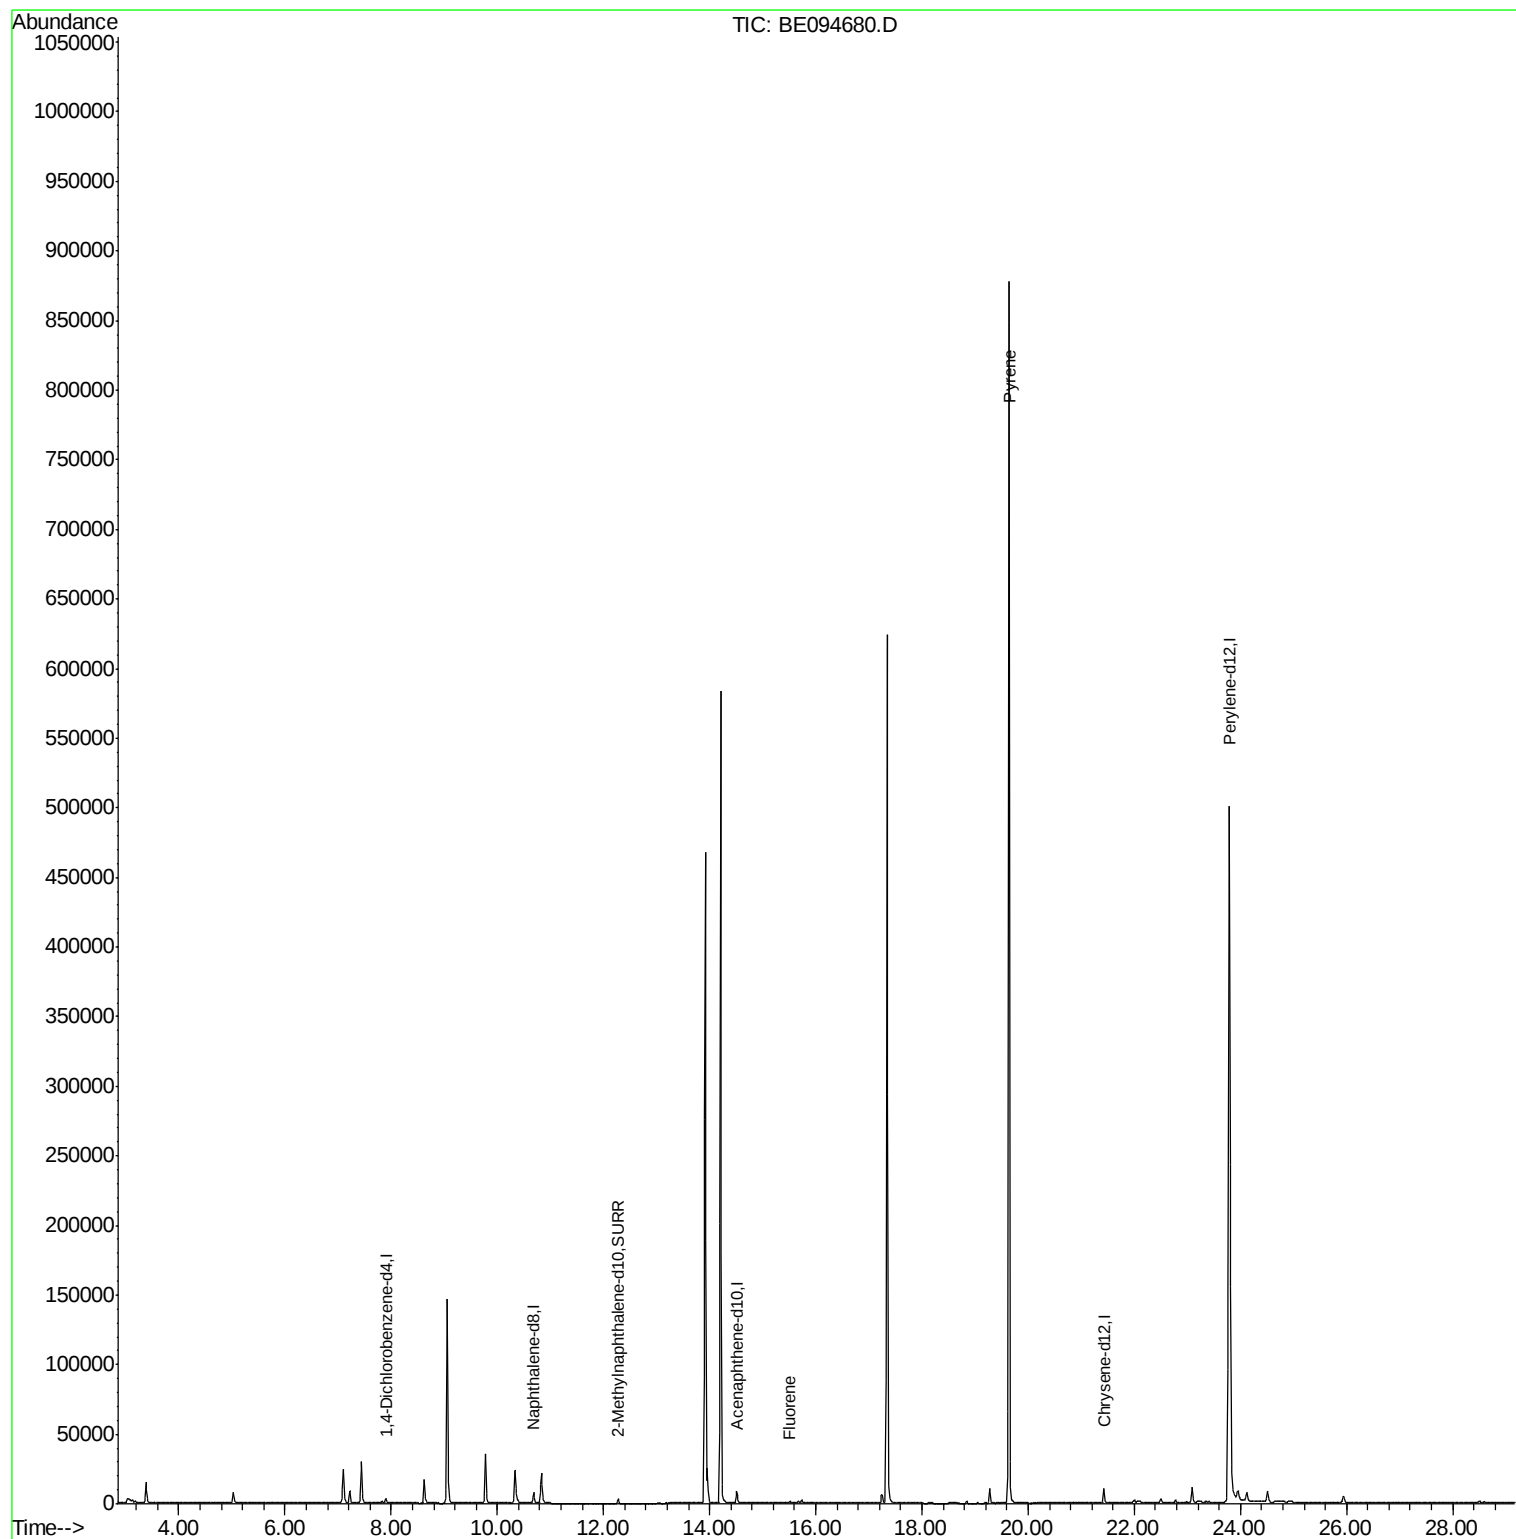


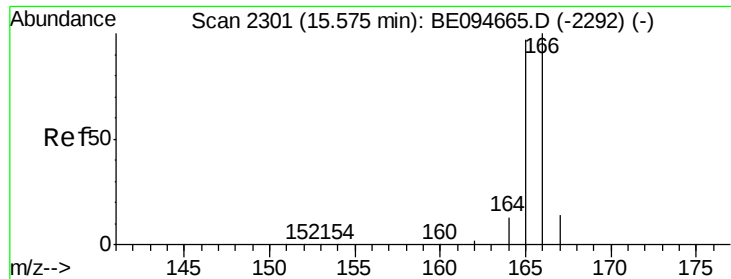

#9
Fluorene
 Concen: 0.06 ng/ul
 RT: 15.51 min Scan# 2292
 Delta R.T. -0.07 min
 Lab File: BE094680.D
 Acq: 1 Nov 2017 4:18

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:166 Resp: 1209
 Ion Ratio Lower Upper
 166 100
 165 10.6 73.4 110.2#
 167 39.7 14.6 22.0#

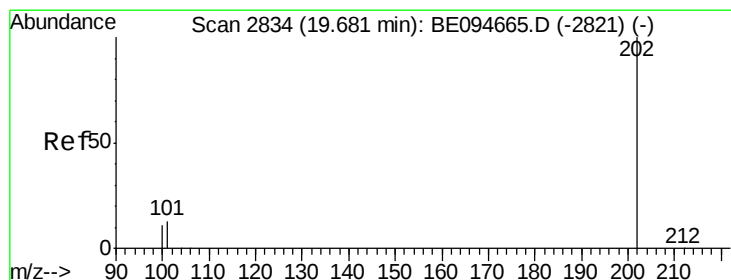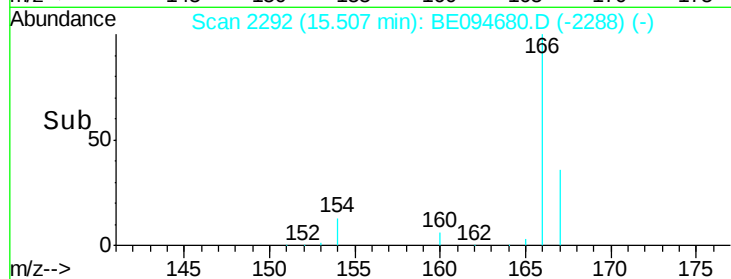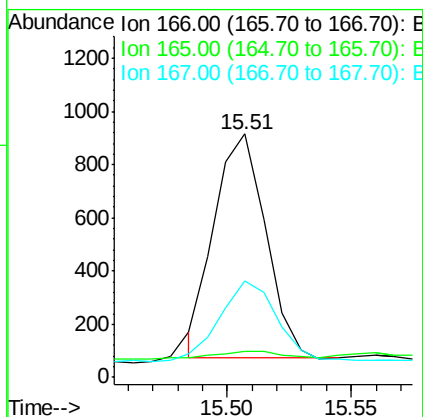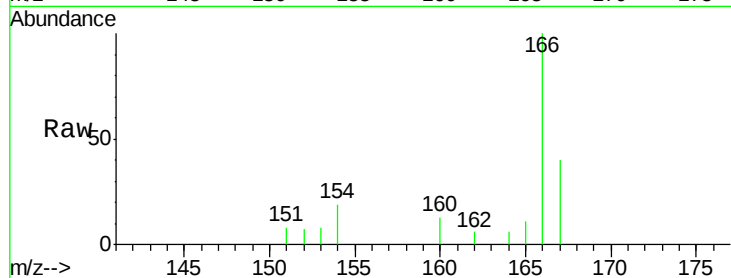

#17
Pyrene
 Concen: 0.06 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.04 min
 Lab File: BE094680.D
 Acq: 1 Nov 2017 4:18

Tgt Ion:202 Resp: 1880
 Ion Ratio Lower Upper
 202 100
 101 149.8 18.2 27.4#
 100 792.6 15.6 23.4#

