




Data Path : Z:\HPCHEM1\BNA E\Data\BE103117\
Data File : Be094656.d
Acq On : 31 Oct 2017 13:46
Operator : SJ/JU
Sample : PB103511BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK11

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:38 PM

Quant Time: Nov 01 01:56:59 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

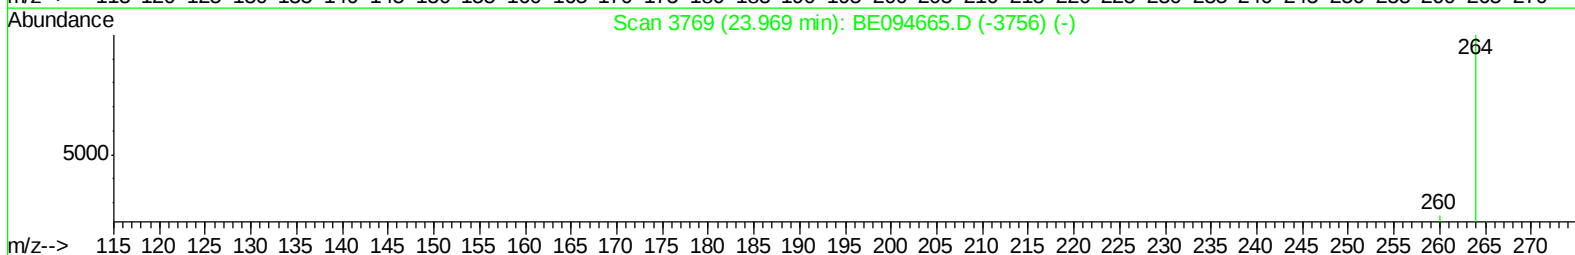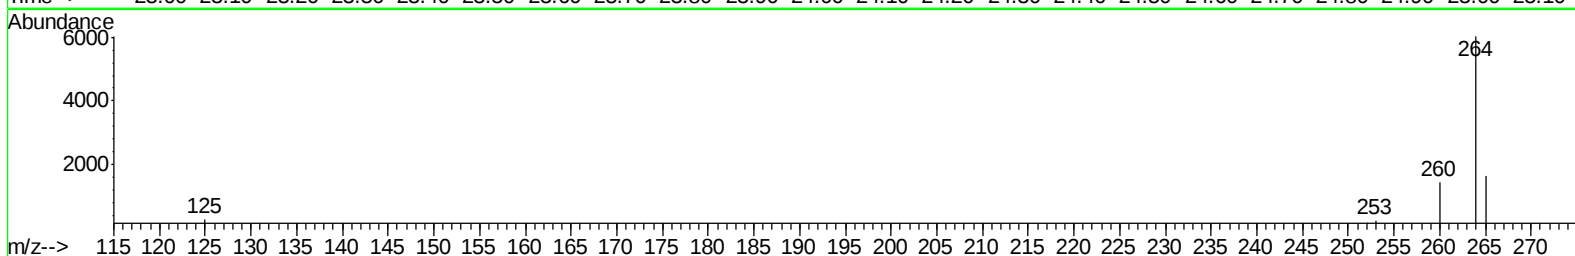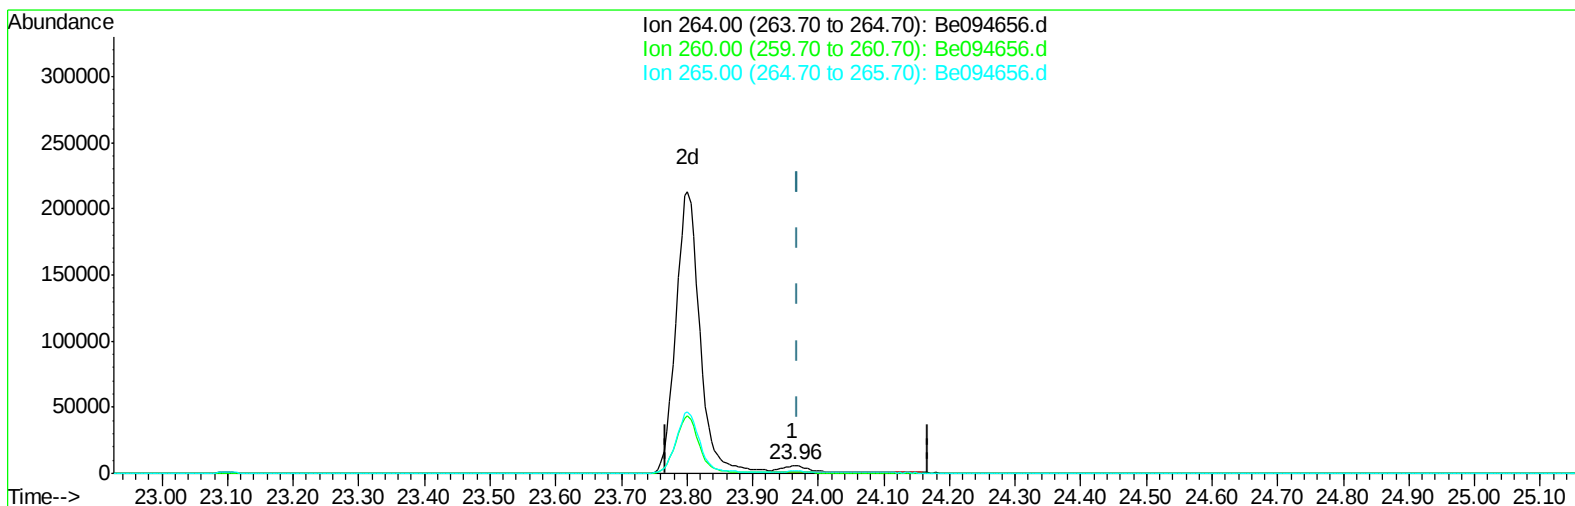

TIC: Be094656.d

(20) Perylene-d12 (I)

23.960min (-0.008) 0.40ng/ul

response 17827

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.12
265.00	103.50	27.53#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\Data\BE103117\
Data File : Be094656.d
Acq On : 31 Oct 2017 13:46
Operator : SJ/JU
Sample : PB103511BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK11

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:38 PM

Quant Time: Nov 01 01:56:59 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

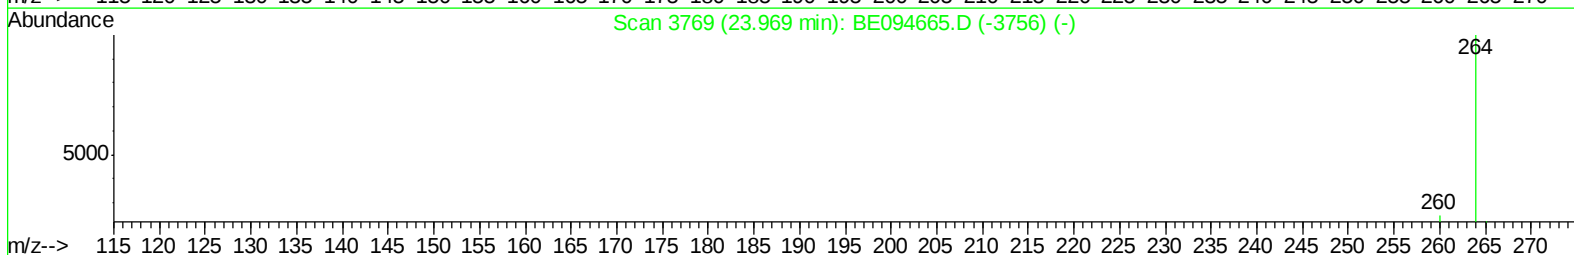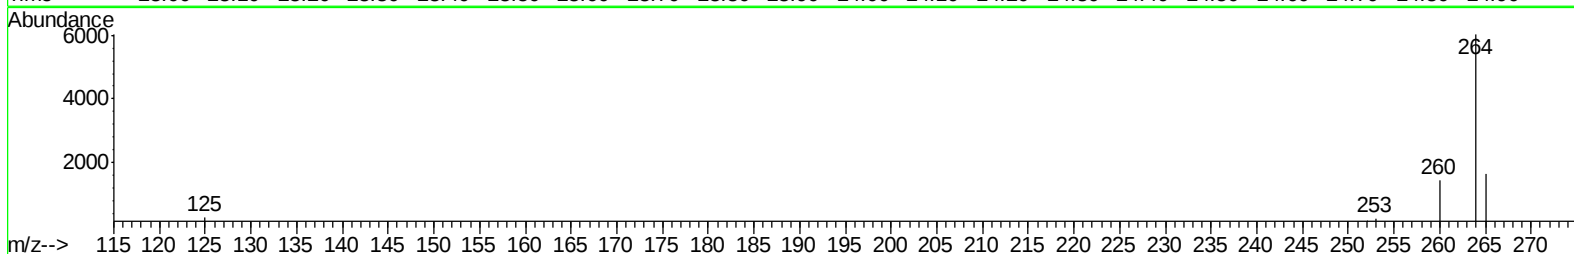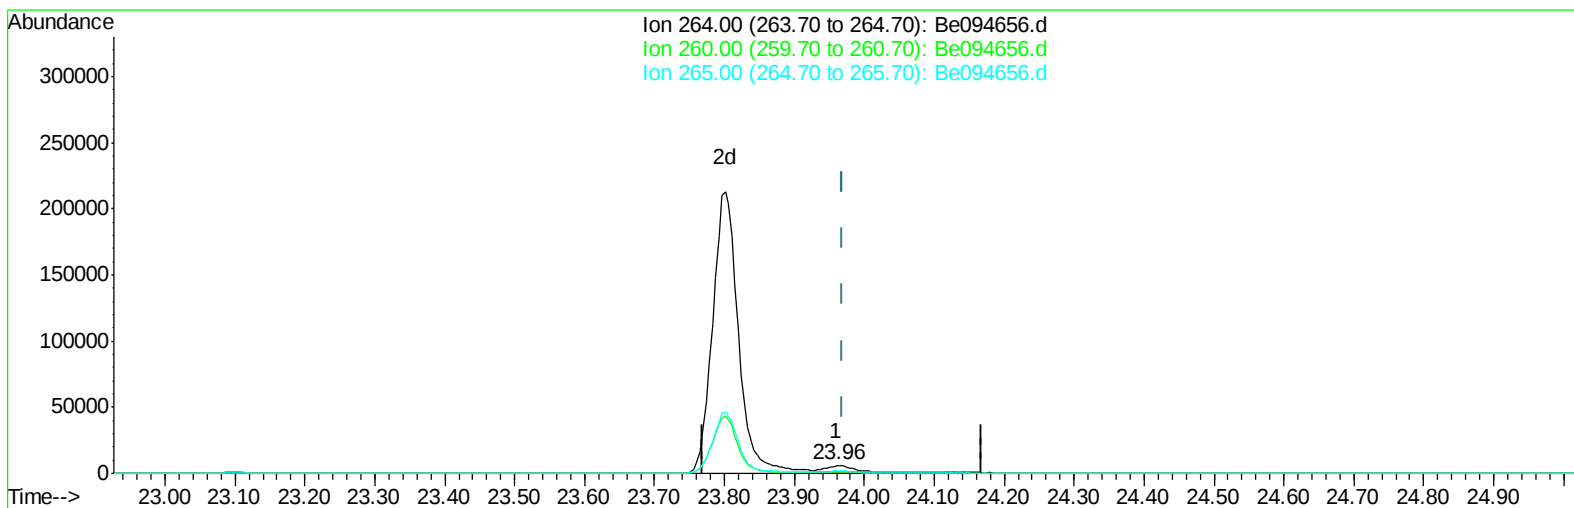

TIC: Be094656.d

(20) Perylene-d12 (I)

23.960min (-0.008) 0.40ng/ul m

response 12350

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.12
265.00	103.50	27.53#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE103117\
 Data File : Be094656.d
 Acq On : 31 Oct 2017 13:46
 Operator : SJ/JU
 Sample : PB103511BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK11

Manual Integrations
 APPROVED

Sohil
 11/1/2017 4:29:38 PM

Quant Time: Nov 01 05:06:52 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 01:43:26 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1555	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	9758	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5741	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	12217	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	12289	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	12350m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	2939	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	6850	0.19	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE103117\
Data File : Be094656.d
Acq On : 31 Oct 2017 13:46
Operator : SJ/JU
Sample : PB103511BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK11

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:38 PM

Quant Time: Nov 01 05:06:52 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

