




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094660.D
Acq On : 31 Oct 2017 16:24
Operator : SJ/JU
Sample : PB103650BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

Sohil
11/1/2017 9:31:56 AM

Quant Time: Nov 01 01:47:02 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

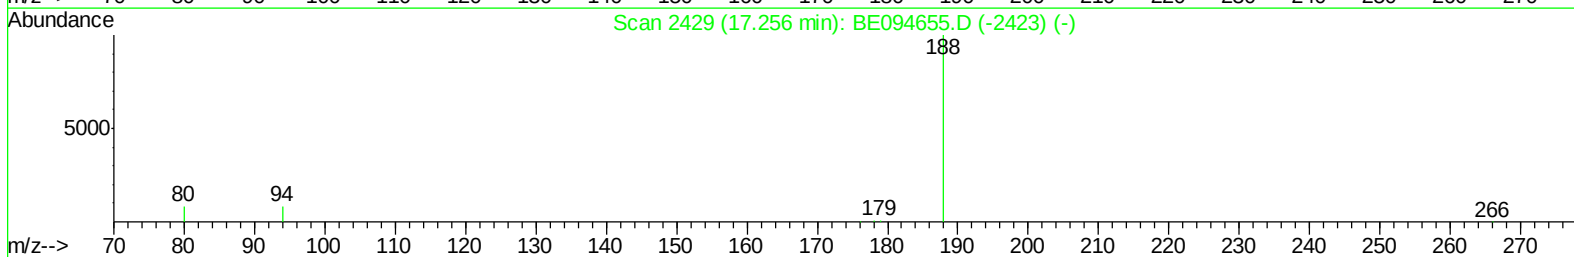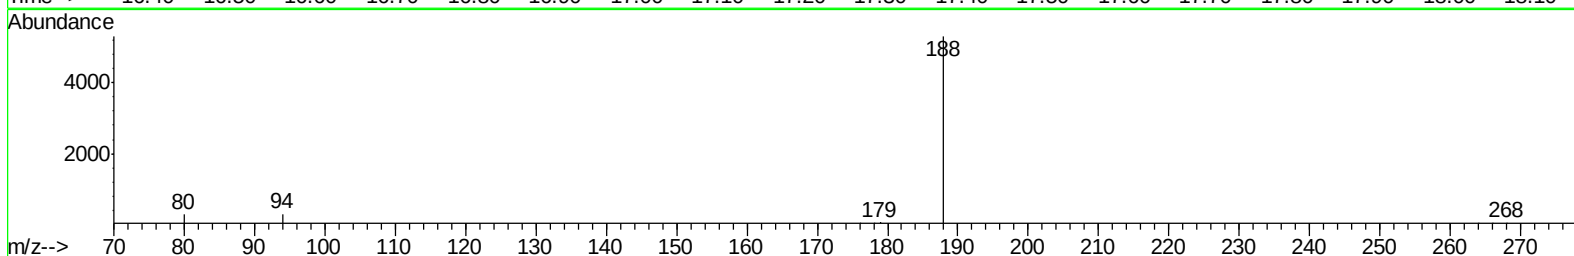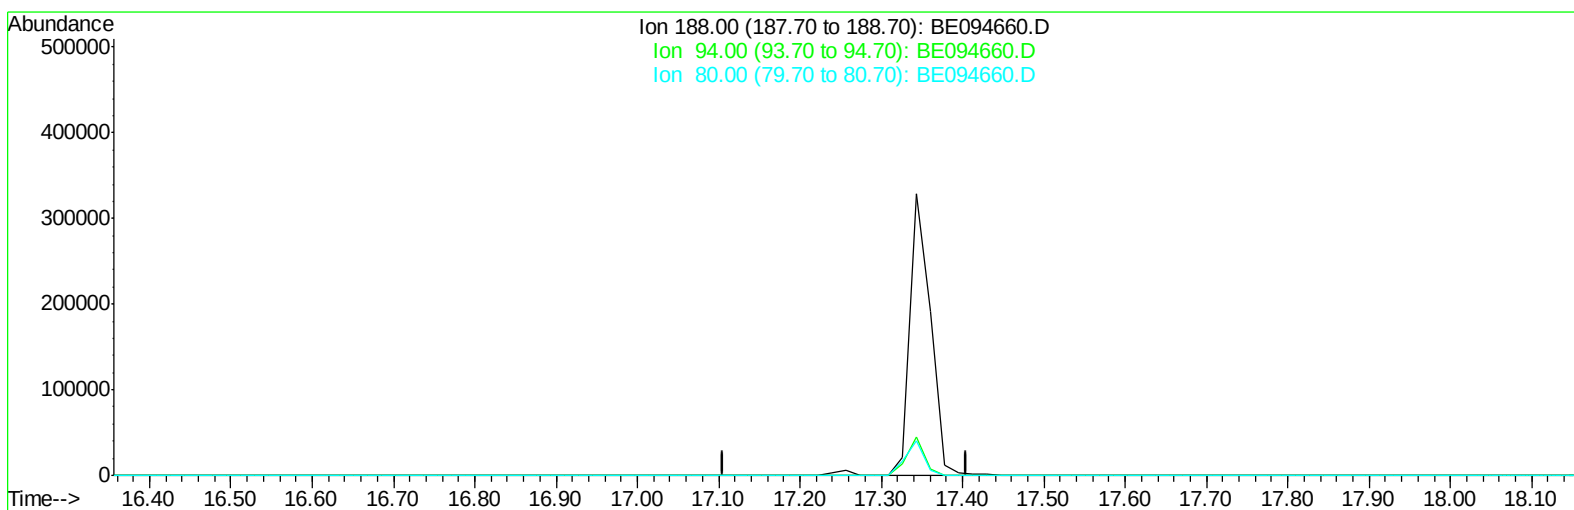

TIC: BE094660.D

(10) Phenanthrene-d10 (I)

17.256min (-17.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094660.D
Acq On : 31 Oct 2017 16:24
Operator : SJ/JU
Sample : PB103650BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

Sohil
11/1/2017 9:31:56 AM

Quant Time: Nov 01 01:47:02 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

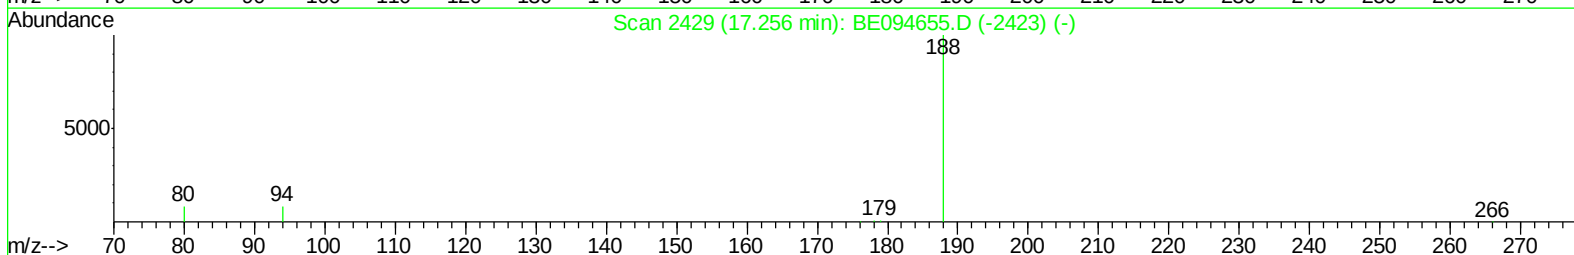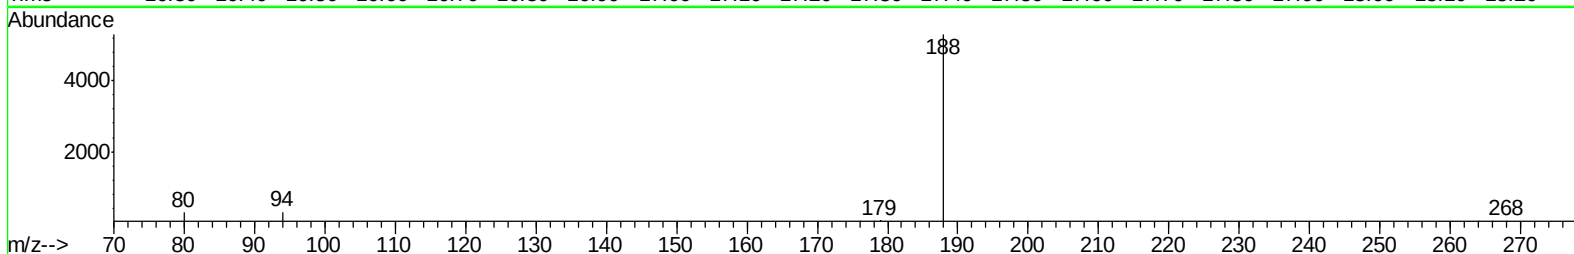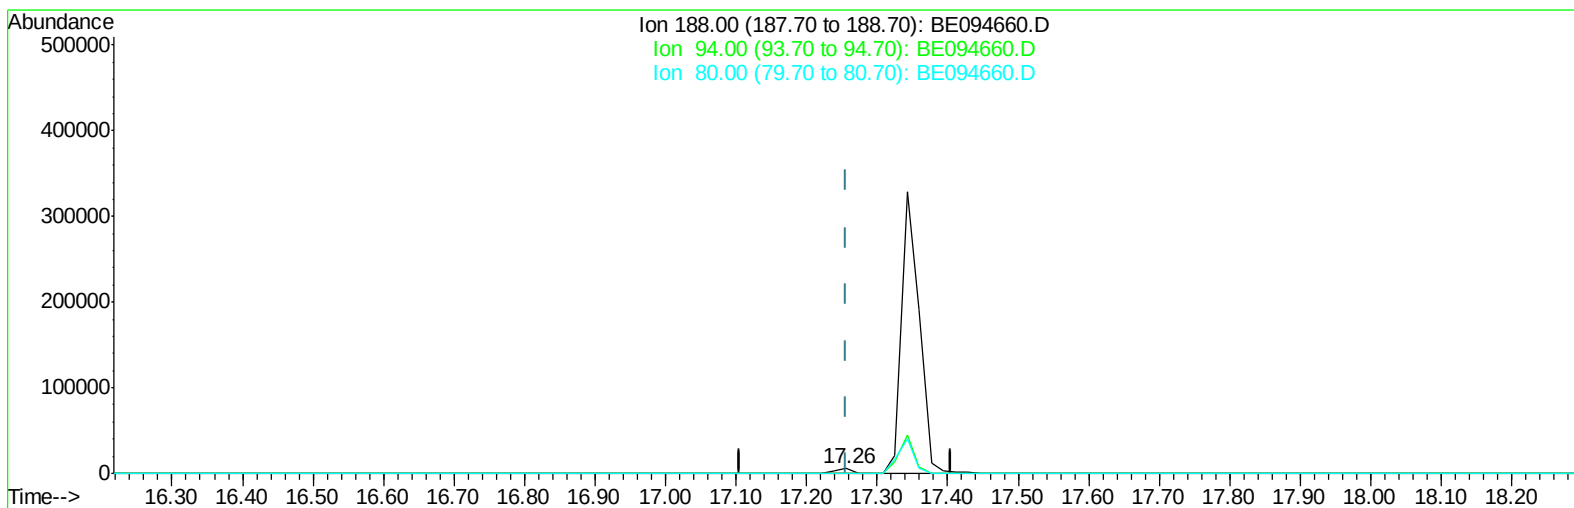

TIC: BE094660.D

(10) Phenanthrene-d10 (I)

17.256min (-0.000) 0.40ng/ul m

response 9209

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.87#
80.00	11.80	5.38#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094660.D
 Acq On : 31 Oct 2017 16:24
 Operator : SJ/JU
 Sample : PB103650BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK50

Manual Integrations
 APPROVED

Sohil
 11/1/2017 9:31:56 AM

Quant Time: Nov 01 02:34:22 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 01:43:26 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1255	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	7795	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4517	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9209m	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9230	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	15024	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3080	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	7105	0.26	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094660.D
Acq On : 31 Oct 2017 16:24
Operator : SJ/JU
Sample : PB103650BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

Sohil
11/1/2017 9:31:56 AM

Quant Time: Nov 01 02:34:22 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 01:43:26 2017
Response via : Initial Calibration

