

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094666.D
Acq On : 31 Oct 2017 20:05
Operator : SJ/JU
Sample : I5844-05
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil

11/1/2017 4:29:41 PM

Quant Time: Nov 01 02:58:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 02:55:07 2017
Response via : Initial Calibration

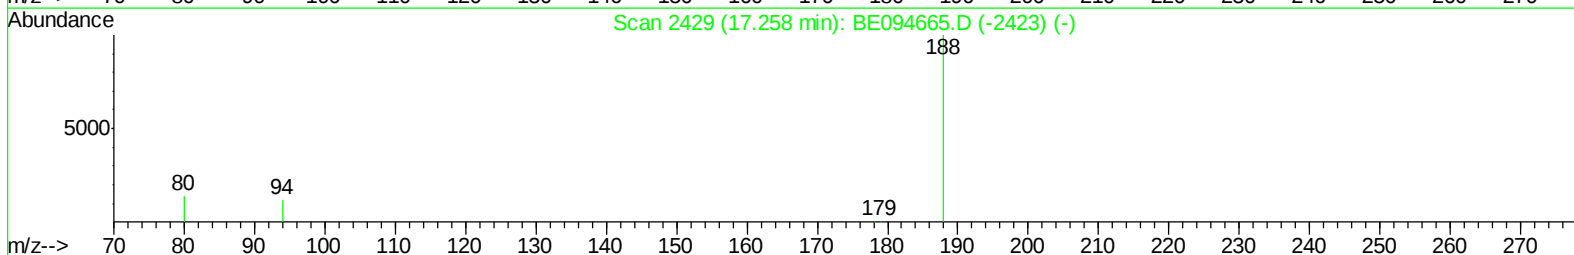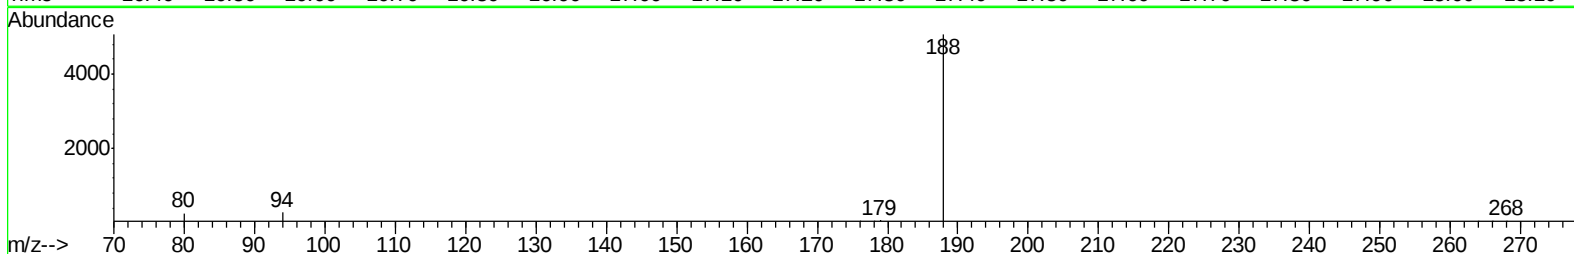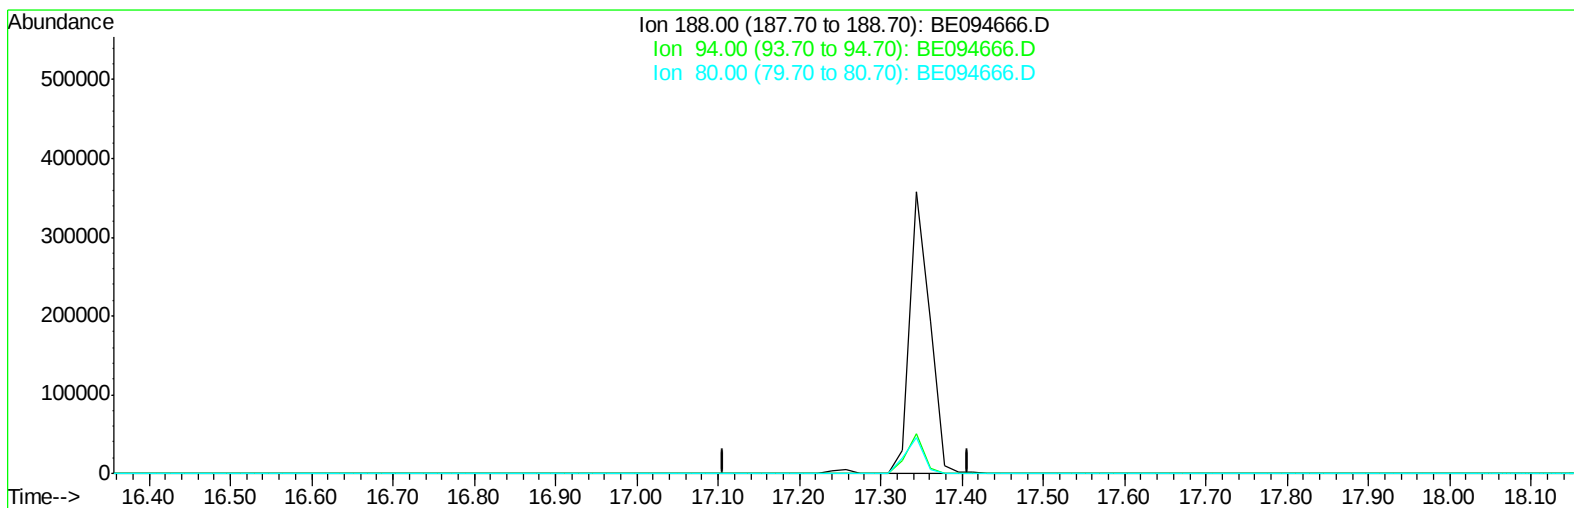

TIC: BE094666.D

(10) Phenanthrene-d10 (I)

17.258min (-17.258) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094666.D
Acq On : 31 Oct 2017 20:05
Operator : SJ/JU
Sample : I5844-05
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil

11/1/2017 4:29:41 PM

Quant Time: Nov 01 02:58:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 02:55:07 2017
Response via : Initial Calibration

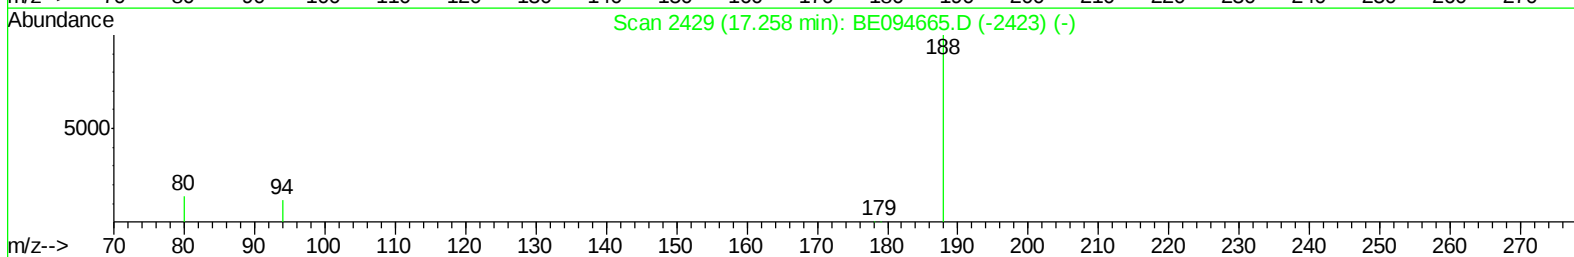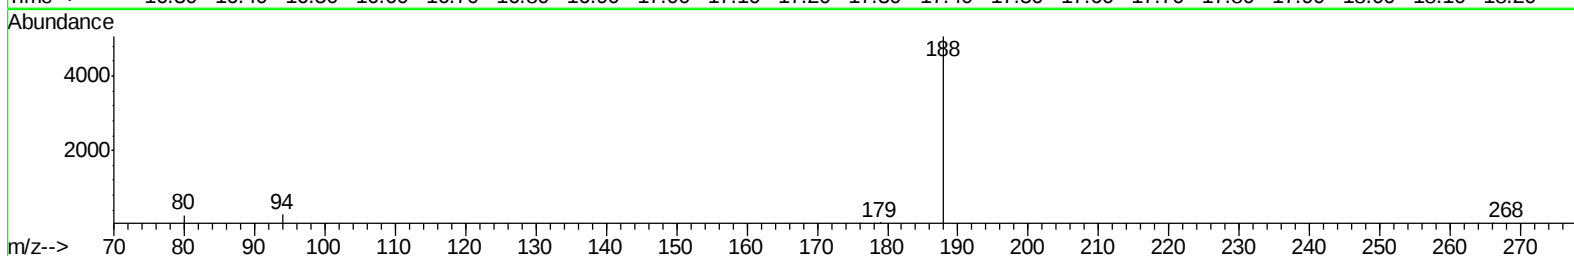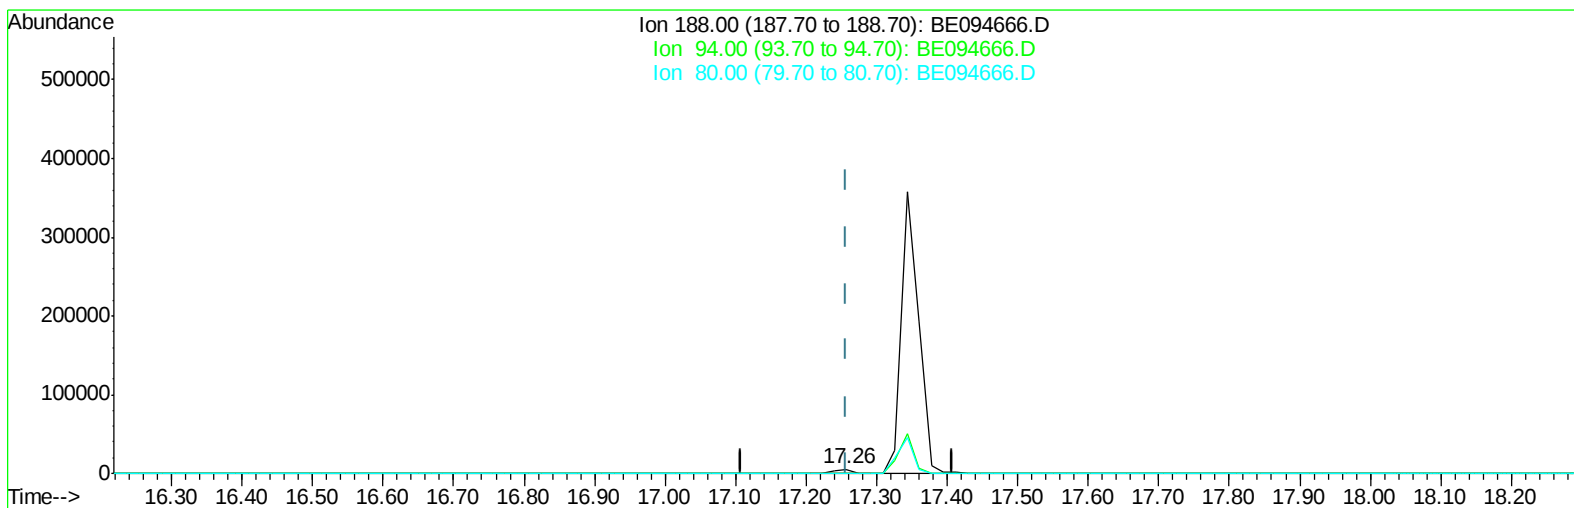

TIC: BE094666.D

(10) Phenanthrene-d10 (I)

17.257min (-0.001) 0.40ng/ul m

response 9647

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.51#
80.00	11.80	5.23#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
 Data File : BE094666.D
 Acq On : 31 Oct 2017 20:05
 Operator : SJ/JU
 Sample : I5844-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil

11/1/2017 4:29:41 PM

Quant Time: Nov 01 03:03:16 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 02:55:07 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1223	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	7427	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	4380	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9647m	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9393	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	15781	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3266	0.27	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	8328	0.29	ng/ul	-0.01

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094666.D
Acq On : 31 Oct 2017 20:05
Operator : SJ/JU
Sample : I5844-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil

Quant Time: Nov 01 03:03:16 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 02:55:07 2017
Response via : Initial Calibration

11/1/2017 4:29:41 PM

