




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:13:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

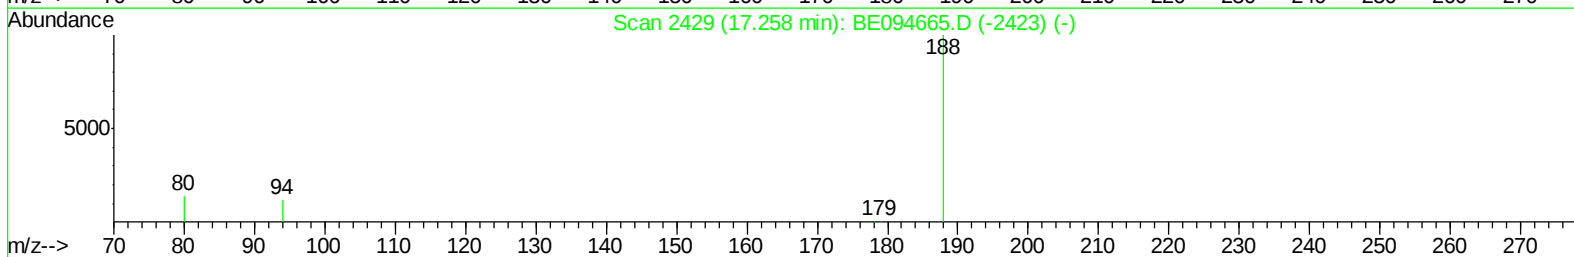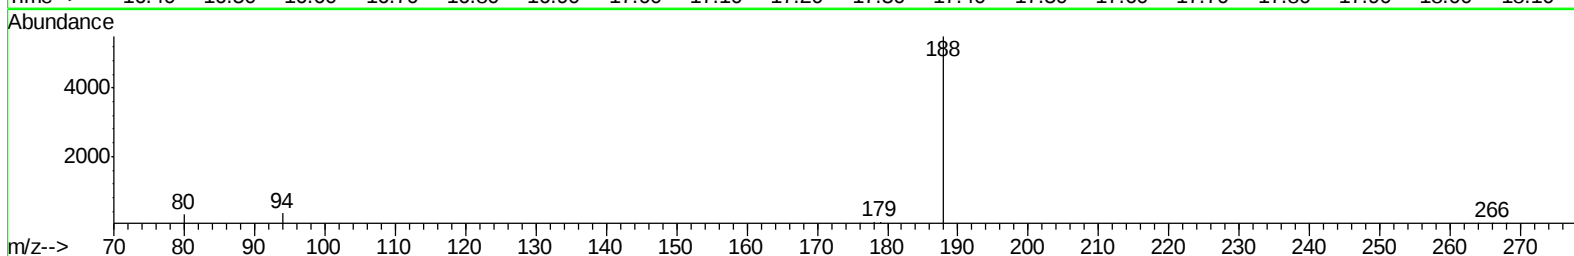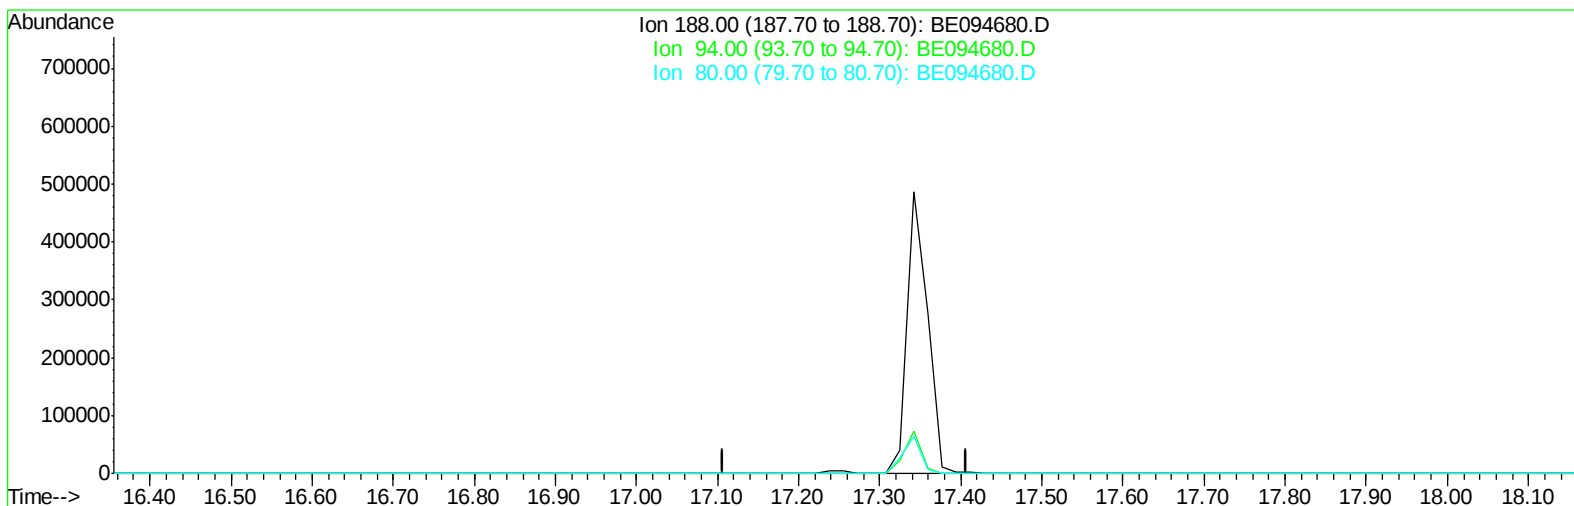

TIC: BE094680.D

(10) Phenanthrene-d10 (I)

17.258min (-17.258) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:13:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

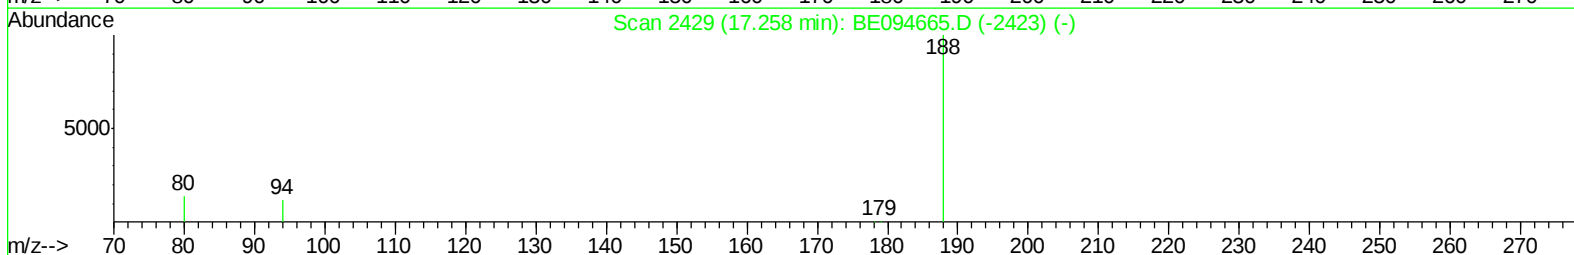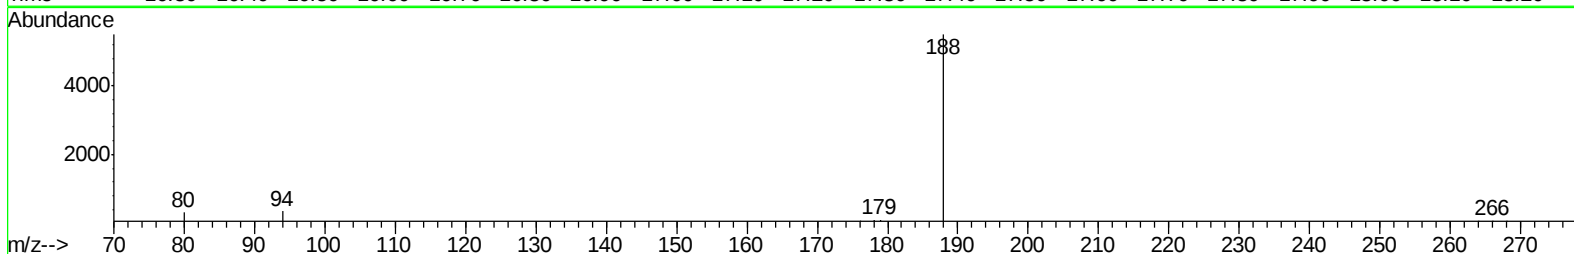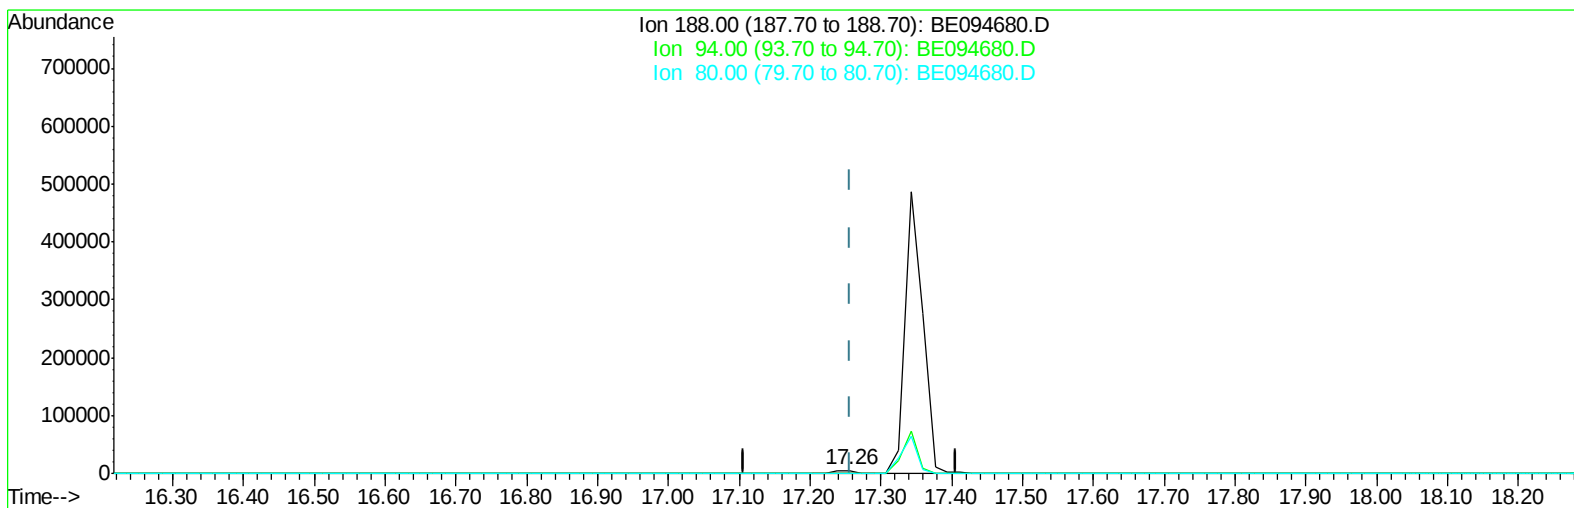

TIC: BE094680.D

(10) Phenanthrene-d10 (I)

17.256min (-0.002) 0.40ng/ul m

response 10812

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.08#
80.00	11.80	5.42#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:30:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

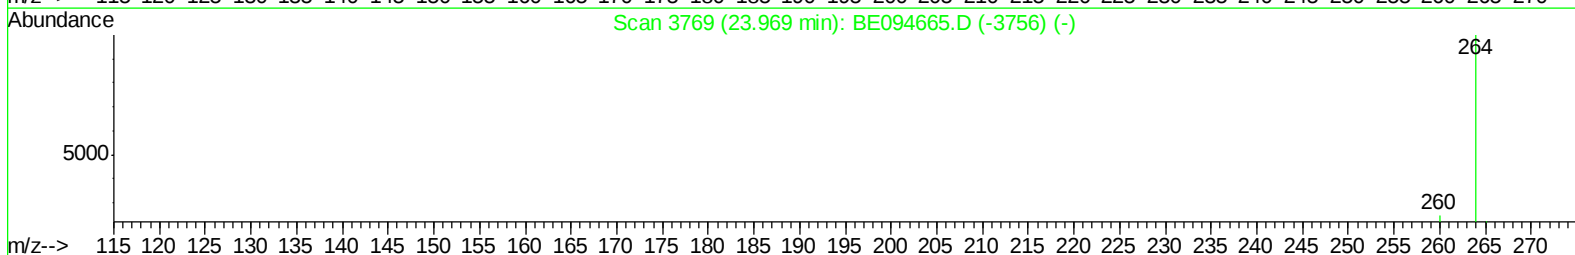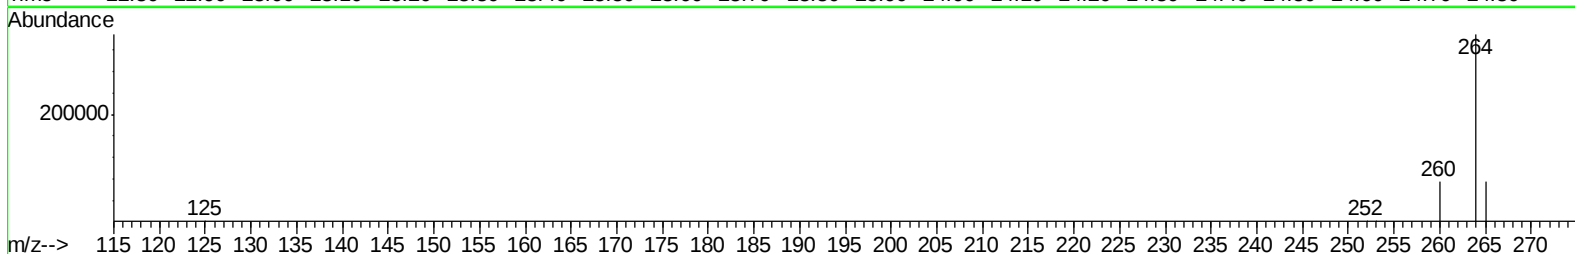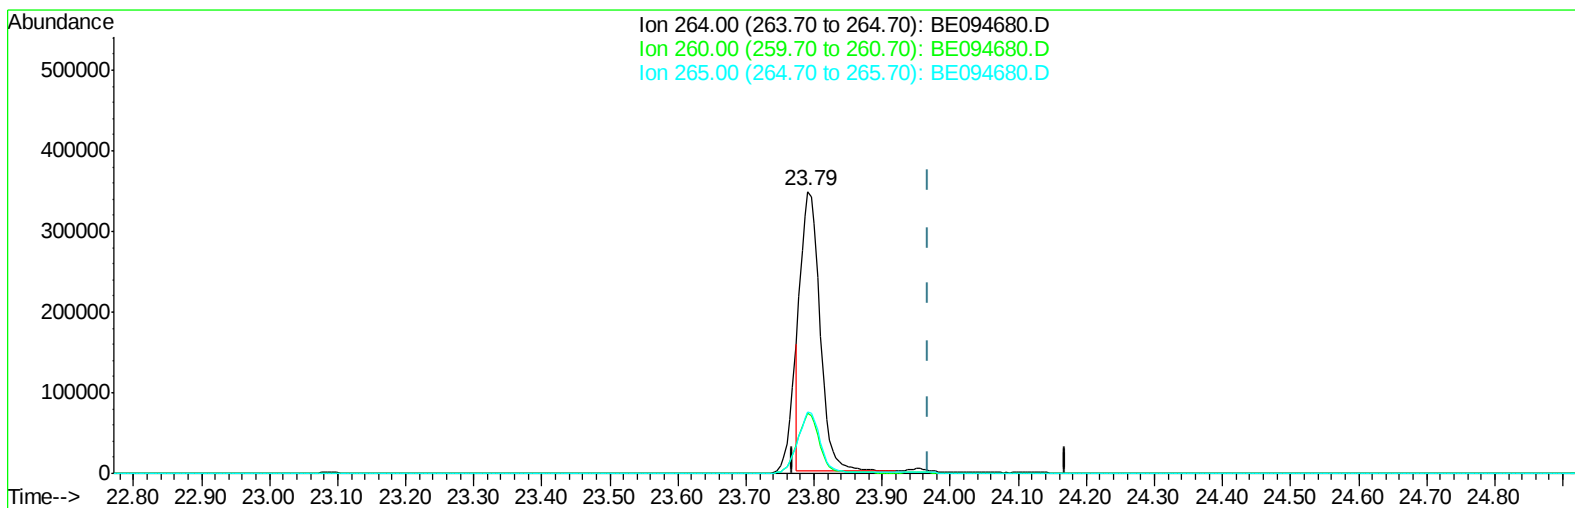

TIC: BE094680.D

(20) Perylene-d12 (I)

23.791min (-0.177) 0.40ng/ul

response 685257

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.17#
265.00	103.50	21.62#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:30:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

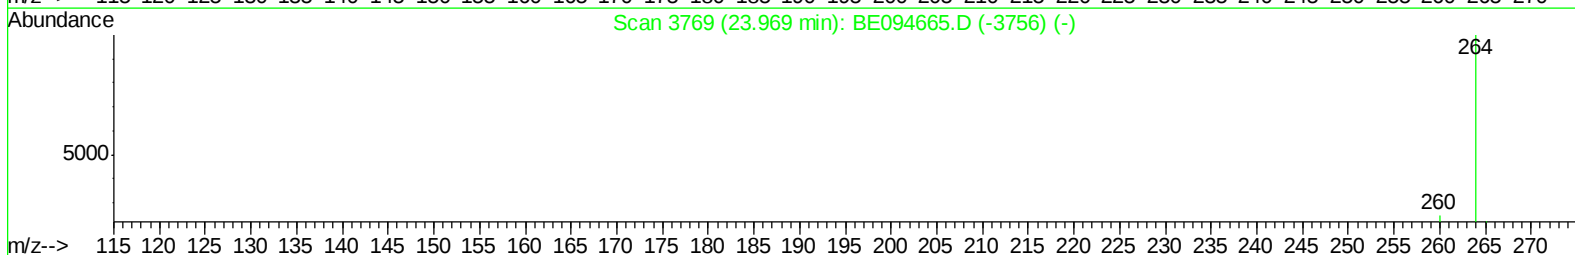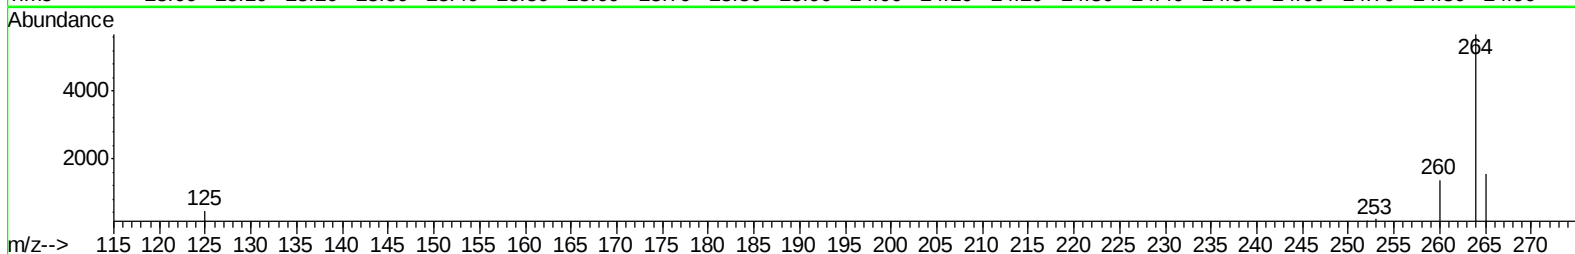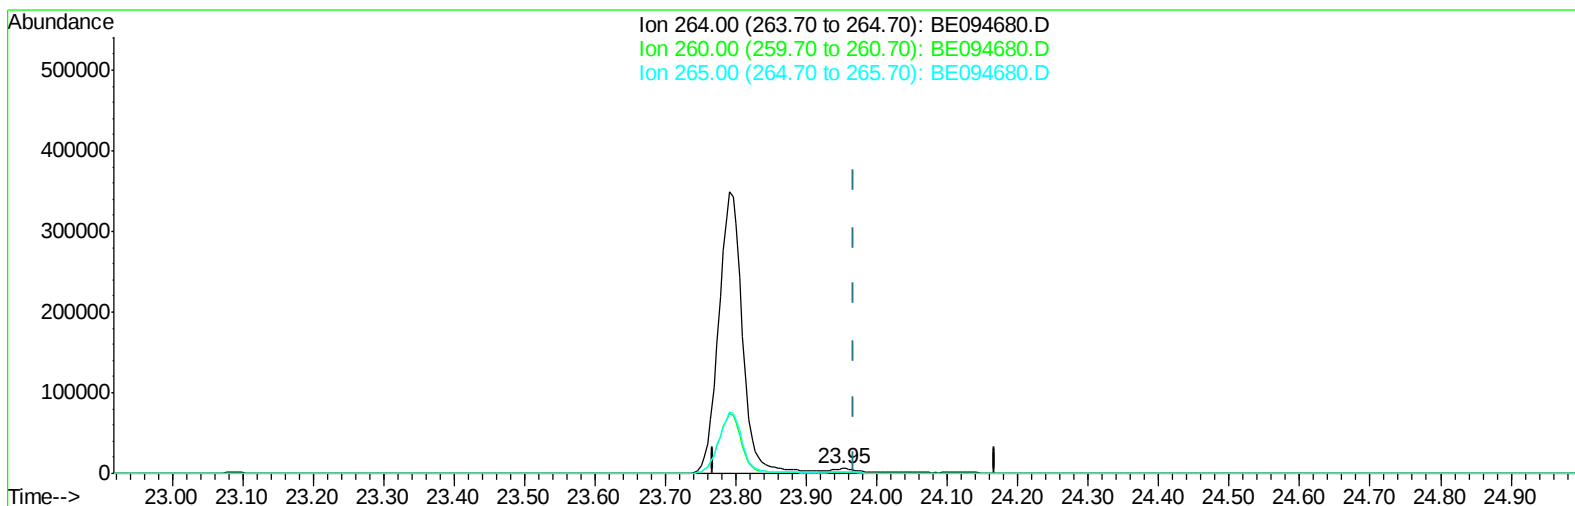

TIC: BE094680.D

(20) Perylene-d12 (I)

23.951min (-0.018) 0.40ng/ul m

response 12422

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.24
265.00	103.50	27.03#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:33:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1544	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.68	136	9235	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.51	164	5270	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	10812m	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	10438	0.40	ng/ul	0.00
20) Perylene-d12	23.95	264	12422m	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	4865	0.32	ng/ul	-0.01
14) Fluoranthene-d10	19.28	212	11588	0.36	ng/ul	-0.01

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE103117\
Data File : BE094680.D
Acq On : 1 Nov 2017 4:18
Operator : SJ/JU
Sample : I5844-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

Sohil
11/1/2017 4:29:58 PM

Quant Time: Nov 01 09:33:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 08:49:40 2017
Response via : Initial Calibration

