




Data Path : Z:\HPCHEM1\BNA_E\Data\BE103117\
Data File : BE094684.D
Acq On : 1 Nov 2017 10:10
Operator : SJ/JU
Sample : I5844-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
11/1/2017 4:30:04 PM

Quant Time: Nov 01 11:42:11 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 09:37:39 2017
Response via : Initial Calibration

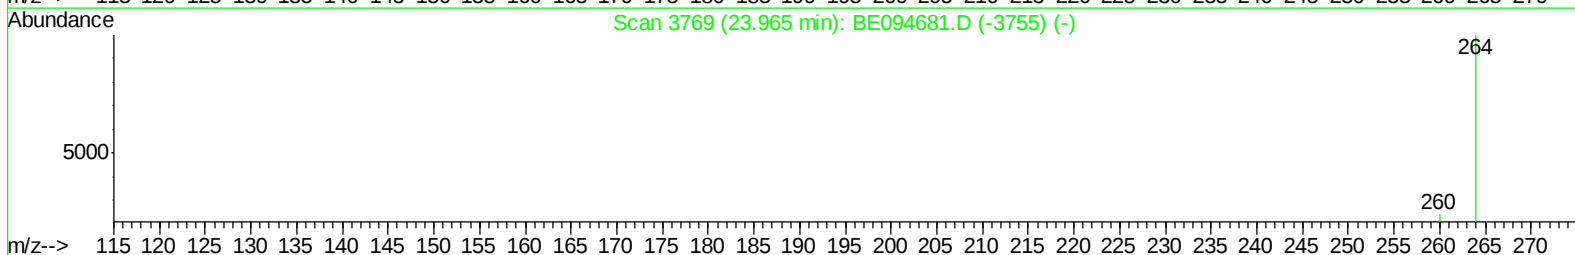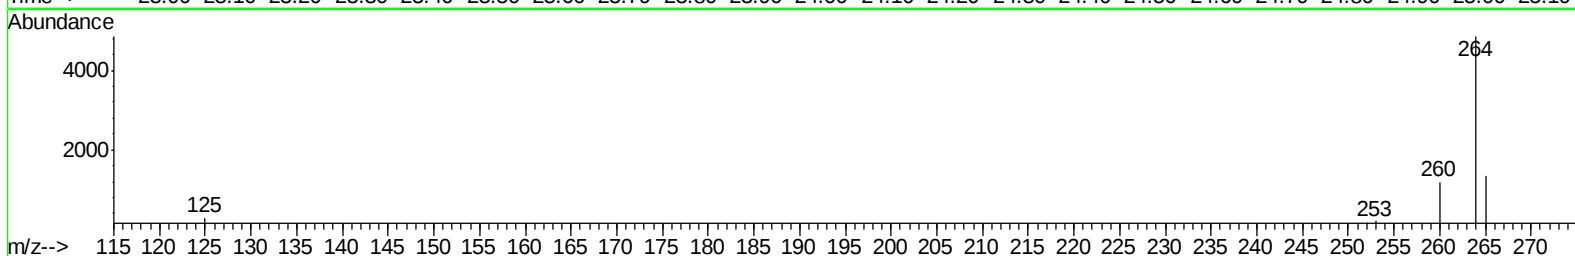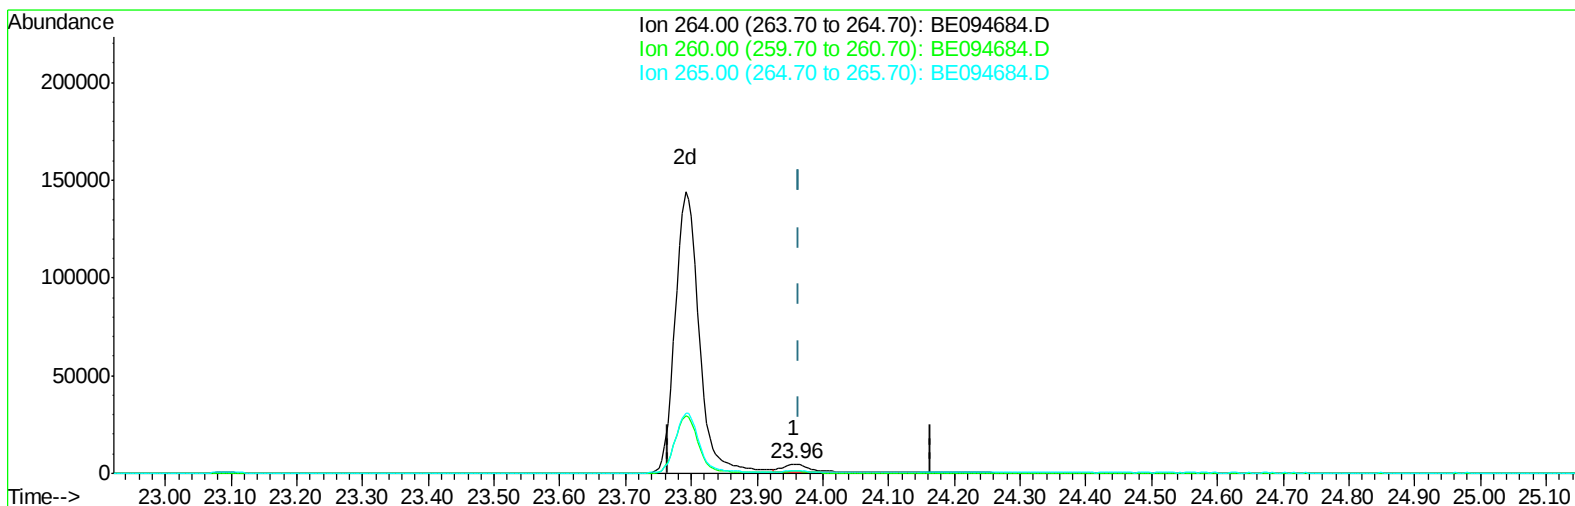

TIC: BE094684.D

(20) Perylene-d12 (I)

23.955min (-0.009) 0.40ng/ul

response 13763

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.53
265.00	103.50	27.79#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE103117\
Data File : BE094684.D
Acq On : 1 Nov 2017 10:10
Operator : SJ/JU
Sample : I5844-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
11/1/2017 4:30:04 PM

Quant Time: Nov 01 11:42:11 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 09:37:39 2017
Response via : Initial Calibration

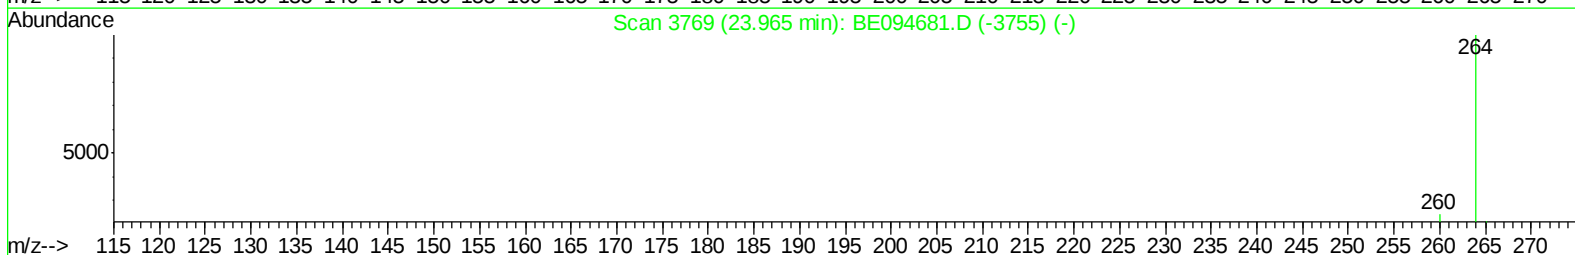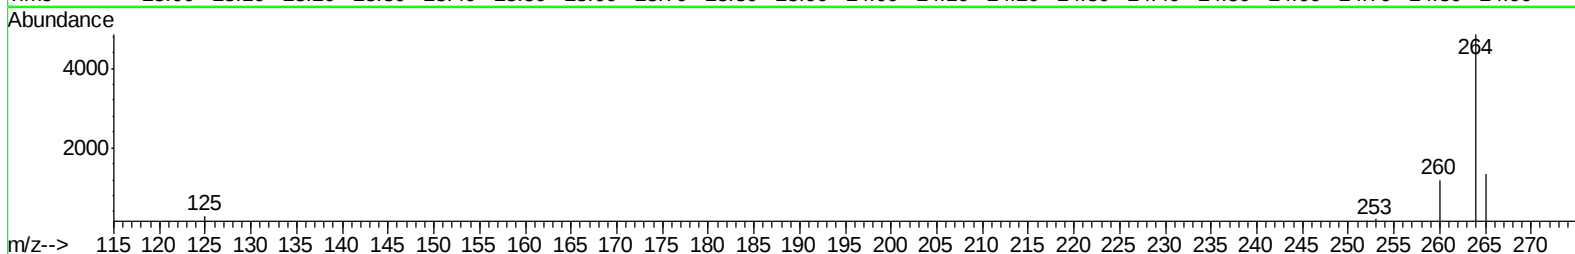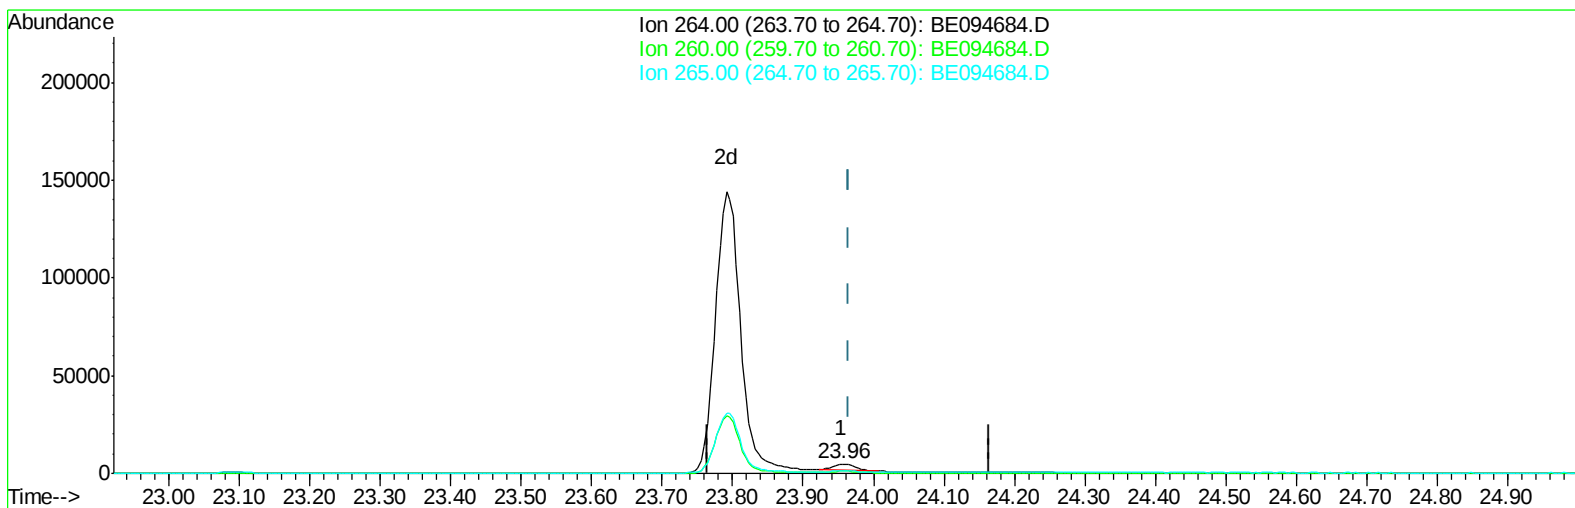

TIC: BE094684.D

(20) Perylene-d12 (I)

23.955min (-0.009) 0.40ng/ul m

response 7148

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.53
265.00	103.50	27.79#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE103117\
 Data File : BE094684.D
 Acq On : 1 Nov 2017 10:10
 Operator : SJ/JU
 Sample : I5844-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 11/1/2017 4:30:04 PM

Quant Time: Nov 01 11:46:27 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 09:37:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1398	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	8359	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4543	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9845	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	9802	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	7148m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	2945	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	9239	0.32	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE103117\
Data File : BE094684.D
Acq On : 1 Nov 2017 10:10
Operator : SJ/JU
Sample : I5844-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
11/1/2017 4:30:04 PM

Quant Time: Nov 01 11:46:27 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 09:37:39 2017
Response via : Initial Calibration

