

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
 Data File : BE101439.D
 Acq On : 31 Oct 2024 18:49
 Operator : RC/JU
 Sample : P4594-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 TP-4

Quant Time: Nov 01 06:15:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.576	152	147844	20.000	ng	0.00
21) Naphthalene-d8	10.343	136	703088	20.000	ng	0.00
39) Acenaphthene-d10	14.186	164	494682	20.000	ng	0.00
64) Phenanthrene-d10	16.924	188	1108938	20.000	ng	0.00
76) Chrysene-d12	21.084	240	1141345	20.000	ng	0.00
86) Perylene-d12	23.381	264	1476803	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.325	112	776719	92.079	ng	0.00
7) Phenol-d6	6.953	99	1009592	86.316	ng	0.00
23) Nitrobenzene-d5	8.786	82	619131	55.309	ng	0.00
42) 2,4,6-Tribromophenol	15.696	330	739741	85.320	ng	0.00
45) 2-Fluorobiphenyl	12.805	172	1531232	52.422	ng	0.00
79) Terphenyl-d14	19.515	244	2775495	55.969	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101439.D
Acq On : 31 Oct 2024 18:49
Operator : RC/JU
Sample : P4594-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-4

Quant Time: Nov 01 06:15:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

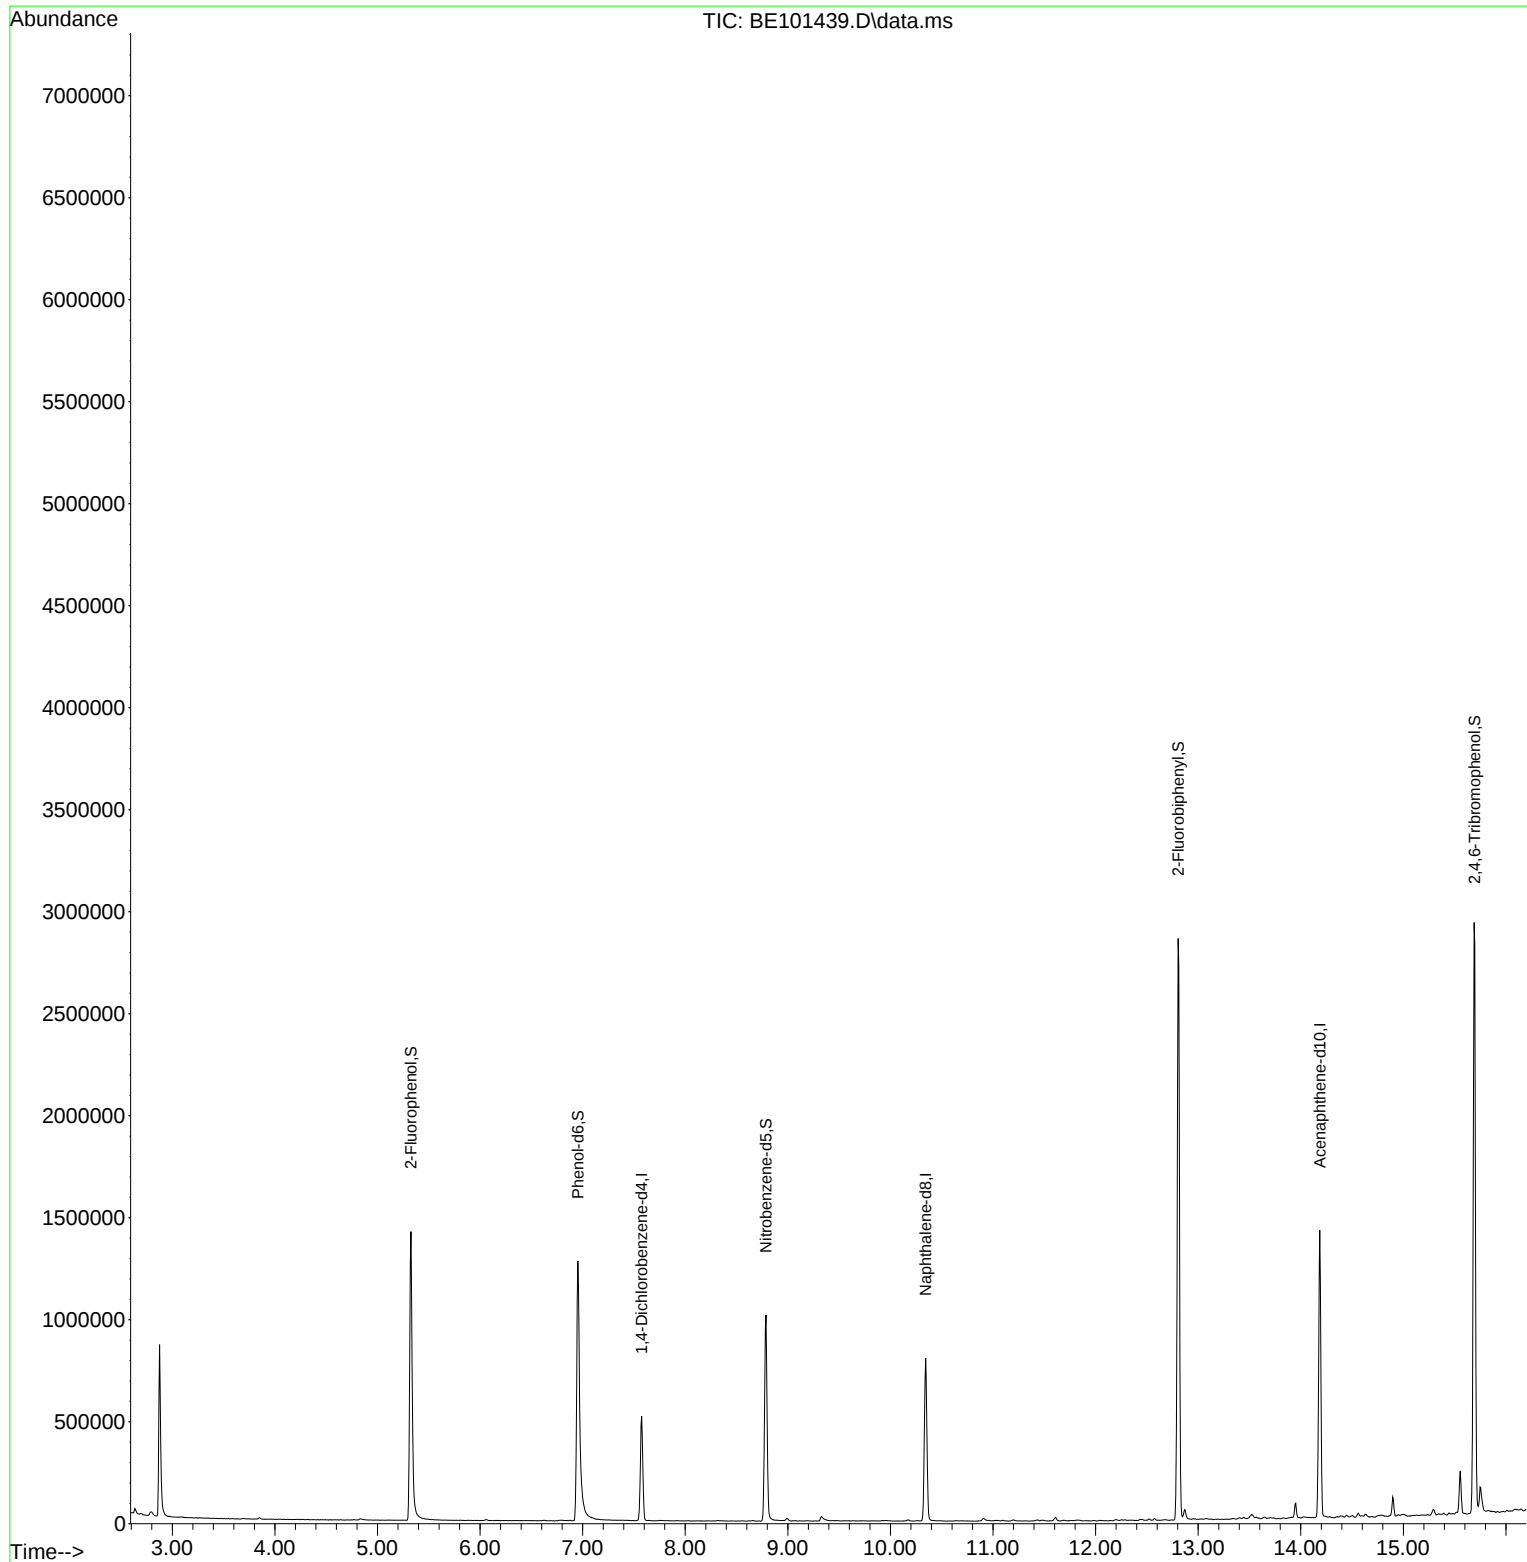

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101439.D
Acq On : 31 Oct 2024 18:49
Operator : RC/JU
Sample : P4594-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-4

Quant Time: Nov 01 06:15:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

