
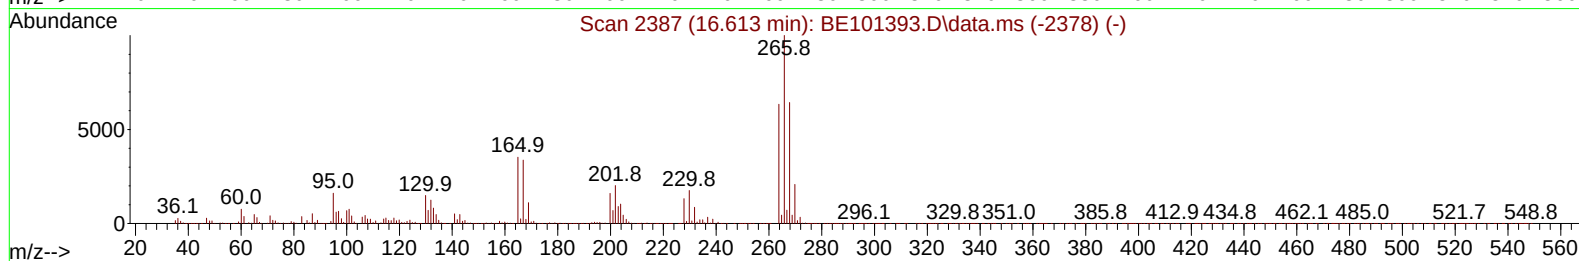
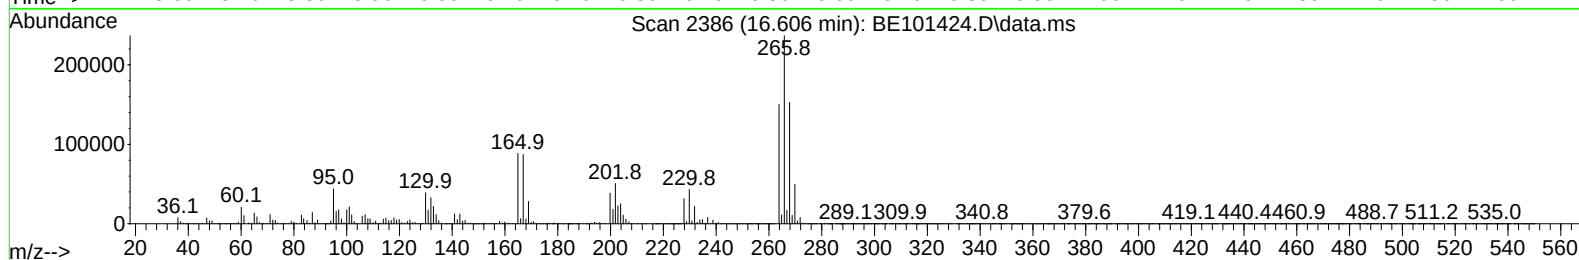


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101424.D
Acq On : 31 Oct 2024 9:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 18:55:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

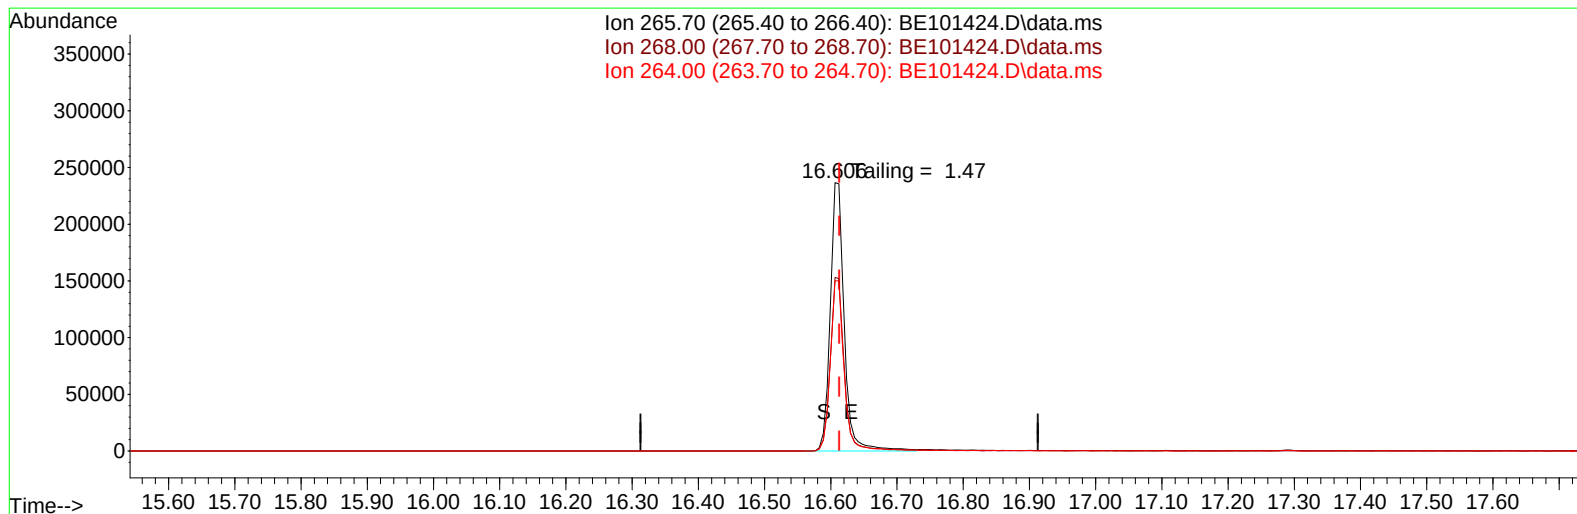

TIC: BE101424.D\data.ms

(70) Pentachlorophenol (C)




16.606min (-0.007) 35129.78 ng

response 348516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.63
264.00	63.40	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101424.D
Acq On : 31 Oct 2024 9:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 18:55:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

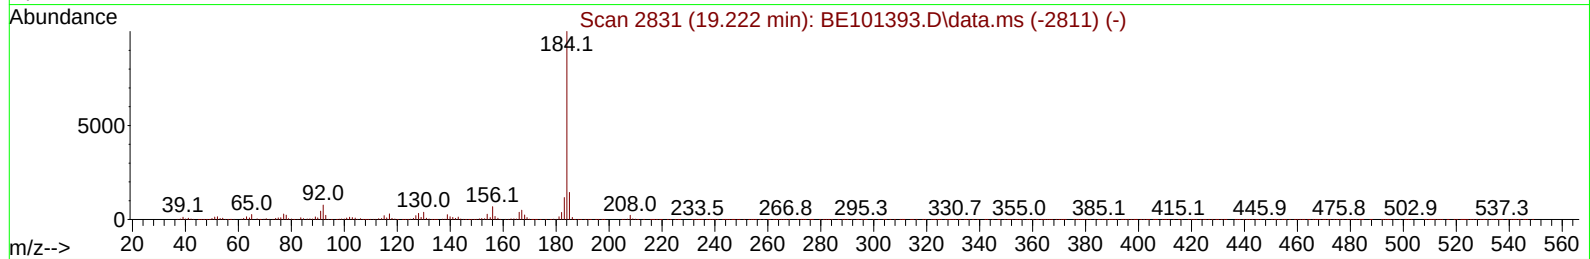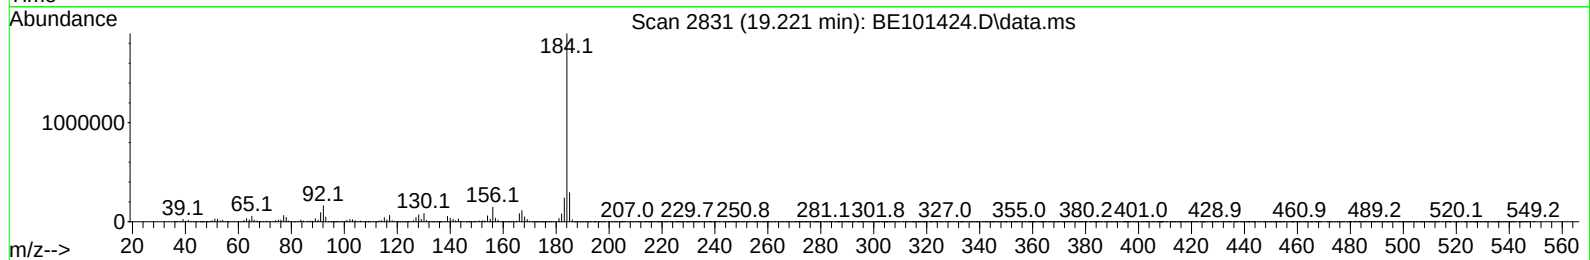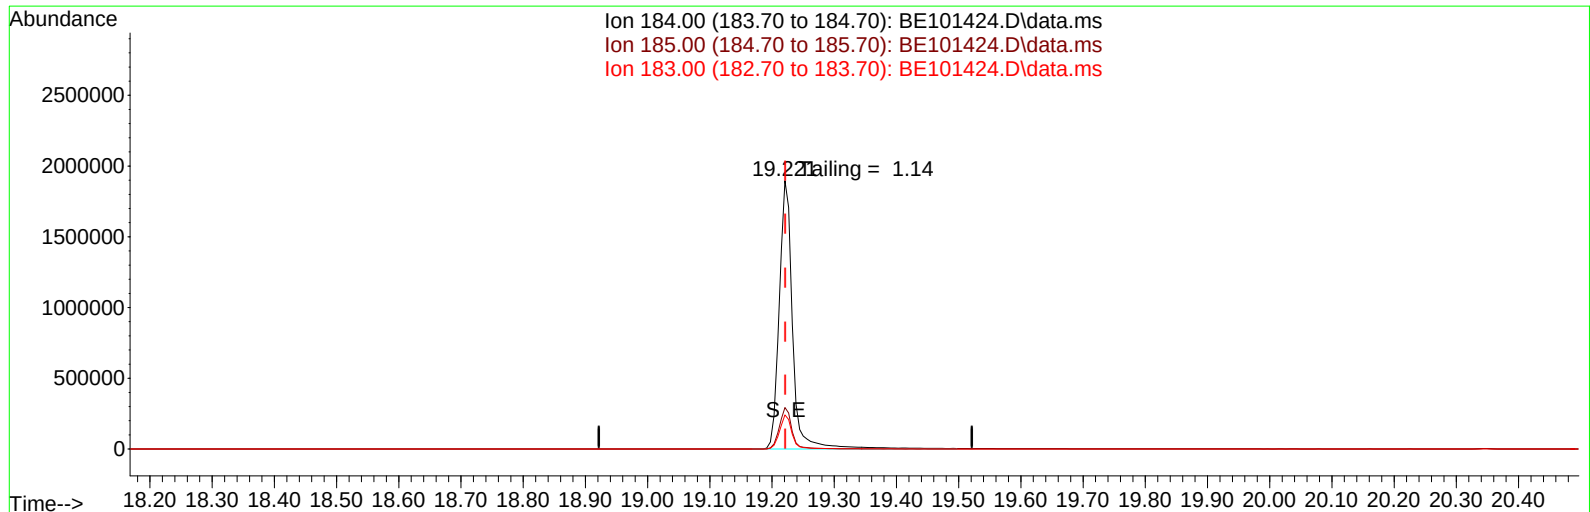

TIC: BE101424.D\data.ms

(77) Benzidine**19.221min (-0.001) 20555.57 ng****response 2867124**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.47
183.00	11.60	12.69
0.00	0.00	0.00