

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101426.D
Acq On : 31 Oct 2024 10:57
Operator : RC/JU
Sample : PB164533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164533BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.317	458	464	496	rBV	2087337	3291924	31.49%	8.061%
2	6.944	734	741	782	rBV	1934783	3476026	33.25%	8.511%
3	7.573	838	848	858	rBV	377109	626690	5.99%	1.535%
4	8.783	1045	1054	1078	rBV	1223310	2123328	20.31%	5.199%
5	10.340	1311	1319	1340	rBV	529149	937626	8.97%	2.296%
6	12.802	1730	1738	1759	rBV	3686589	5627324	53.83%	13.779%
7	14.177	1965	1972	1984	rBV	931398	1369332	13.10%	3.353%
8	15.687	2220	2229	2260	rBV	3326740	5202581	49.76%	12.739%
9	16.915	2431	2438	2452	rBV	1288833	1813390	17.35%	4.440%
10	19.512	2873	2880	2902	rBV	7487309	10454738	100.00%	25.599%
11	21.075	3140	3146	3164	rBV	2066648	2649913	25.35%	6.489%
12	23.361	3527	3535	3546	rBV	1667724	3266984	31.25%	7.999%




Sum of corrected areas: 40839856

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101426.D
Acq On : 31 Oct 2024 10:57
Operator : RC/JU
Sample : PB164533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

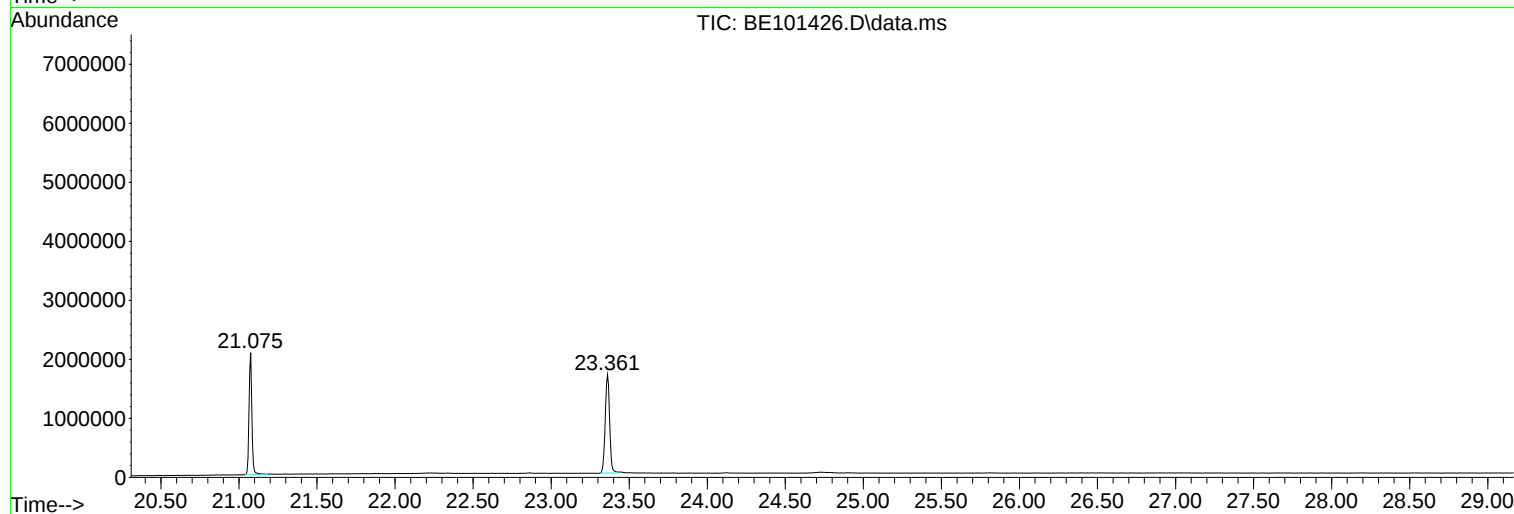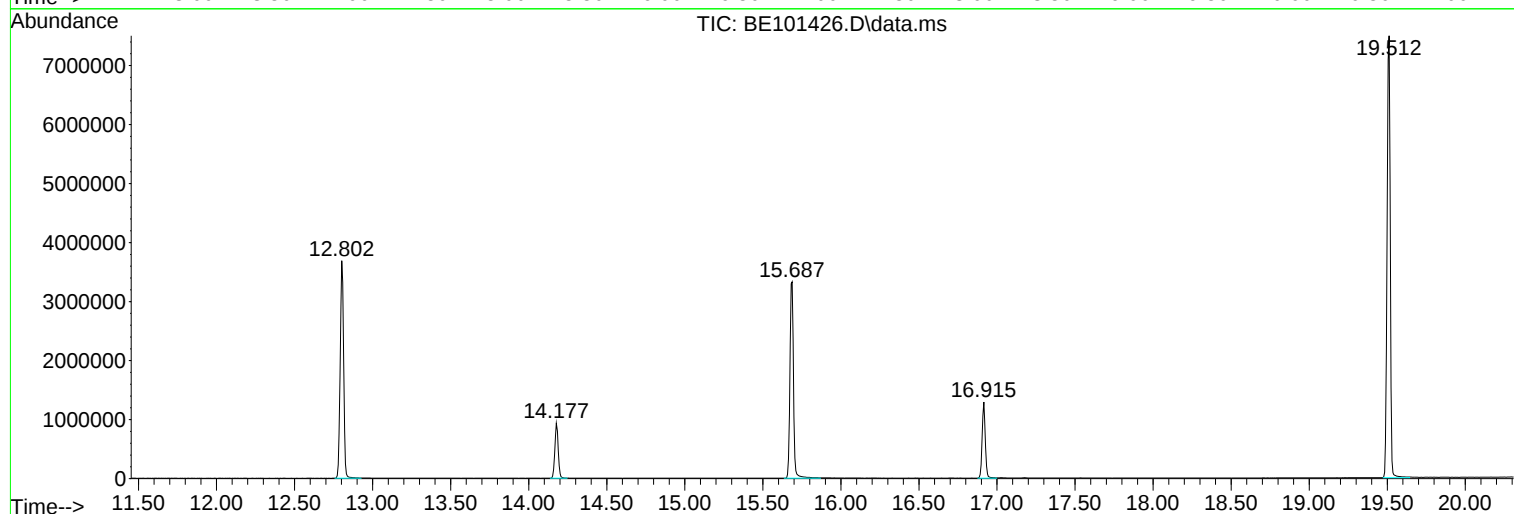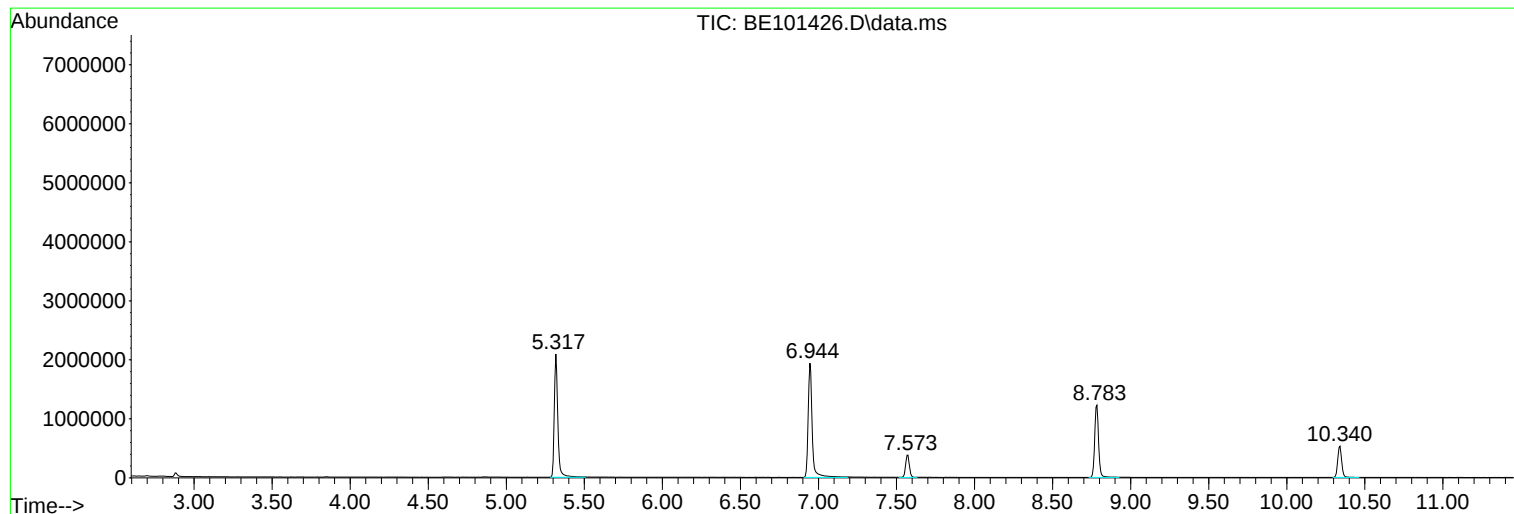

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101426.D
Acq On : 31 Oct 2024 10:57
Operator : RC/JU
Sample : PB164533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE103124\
Data File : BE101426.D
Acq On : 31 Oct 2024 10:57
Operator : RC/JU
Sample : PB164533BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164533BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------