


Data Path : Z:\HPCHEM1\BNA E\DATA\BE110117\
 Data File : BE094686.D
 Acq On : 1 Nov 2017 11:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 22:40:47 2017

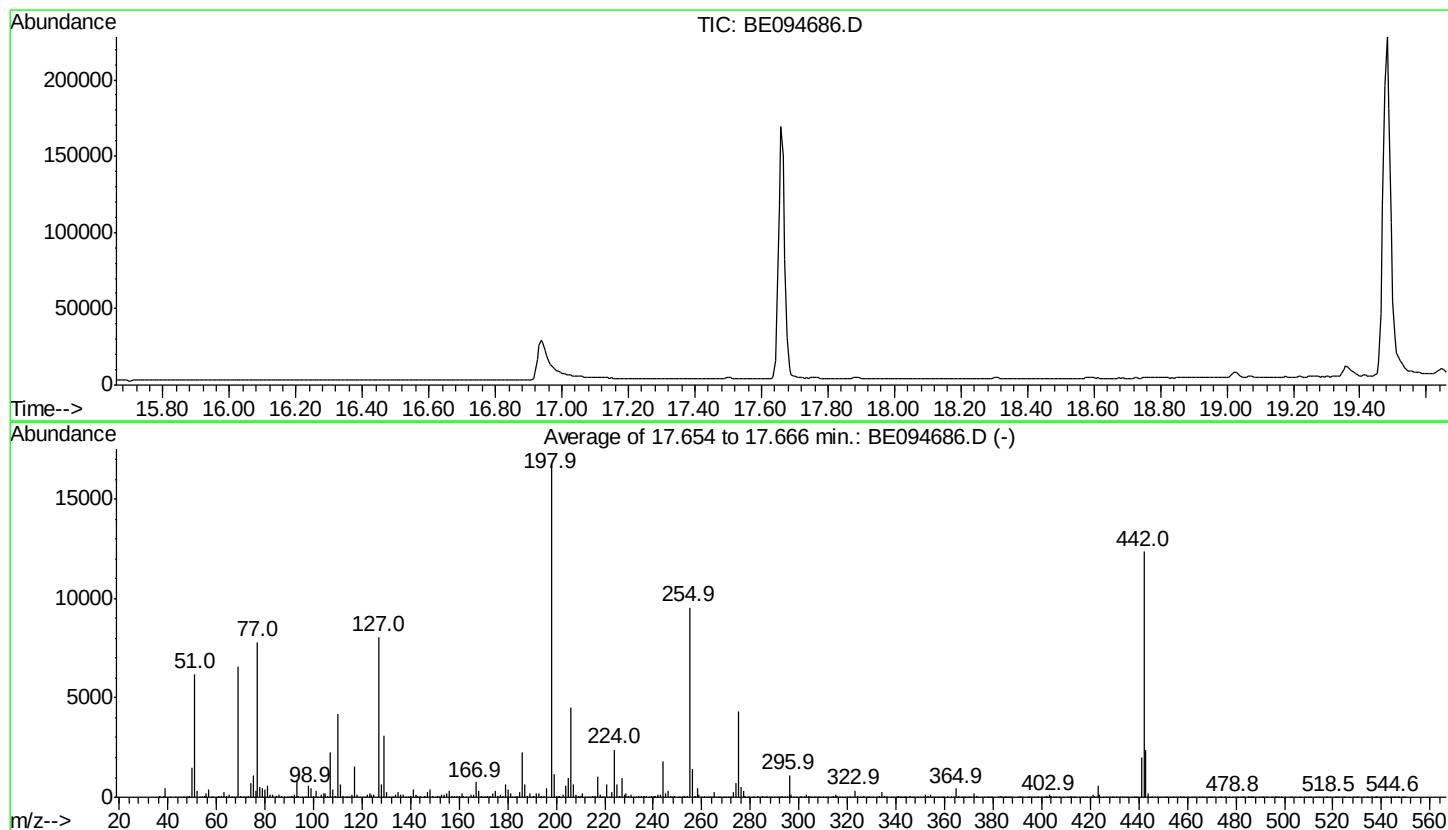

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	6209	PASS
68	69	0.00	2	0.4	24	PASS
69	198	0.00	100	39.4	6577	PASS
70	69	0.00	2	0.6	39	PASS
127	198	10	80	48.3	8065	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16684	PASS
199	198	5	9	7.0	1170	PASS
275	198	10	60	25.7	4285	PASS
365	198	1	100	2.5	422	PASS
441	442	0.01	24	16.2	2001	PASS
442	198	50	100	74.1	12362	PASS
443	442	15	24	19.4	2400	PASS