

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110317\
 Data File : BE094702.D
 Acq On : 3 Nov 2017 11:09
 Operator : SJ/JU
 Sample : PB103506BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK06

Quant Time: Nov 03 23:58:31 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 03 23:54:30 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1431	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	8651	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.51	164	5035	0.40	ng/ul	-0.02
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	10606	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	20608	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3220	0.23	ng/ul	-0.02
14) Fluoranthene-d10	19.28	212	7308	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	894	0.05	ng/ul#	22
17) Pyrene	19.64	202	936	0.03	ng/ul#	1
23) Benzo(a)pyrene	23.79	252	1813	0.03	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110317\
Data File : BE094702.D
Acq On : 3 Nov 2017 11:09
Operator : SJ/JU
Sample : PB103506BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK06

Quant Time: Nov 03 23:58:31 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 23:54:30 2017
Response via : Initial Calibration




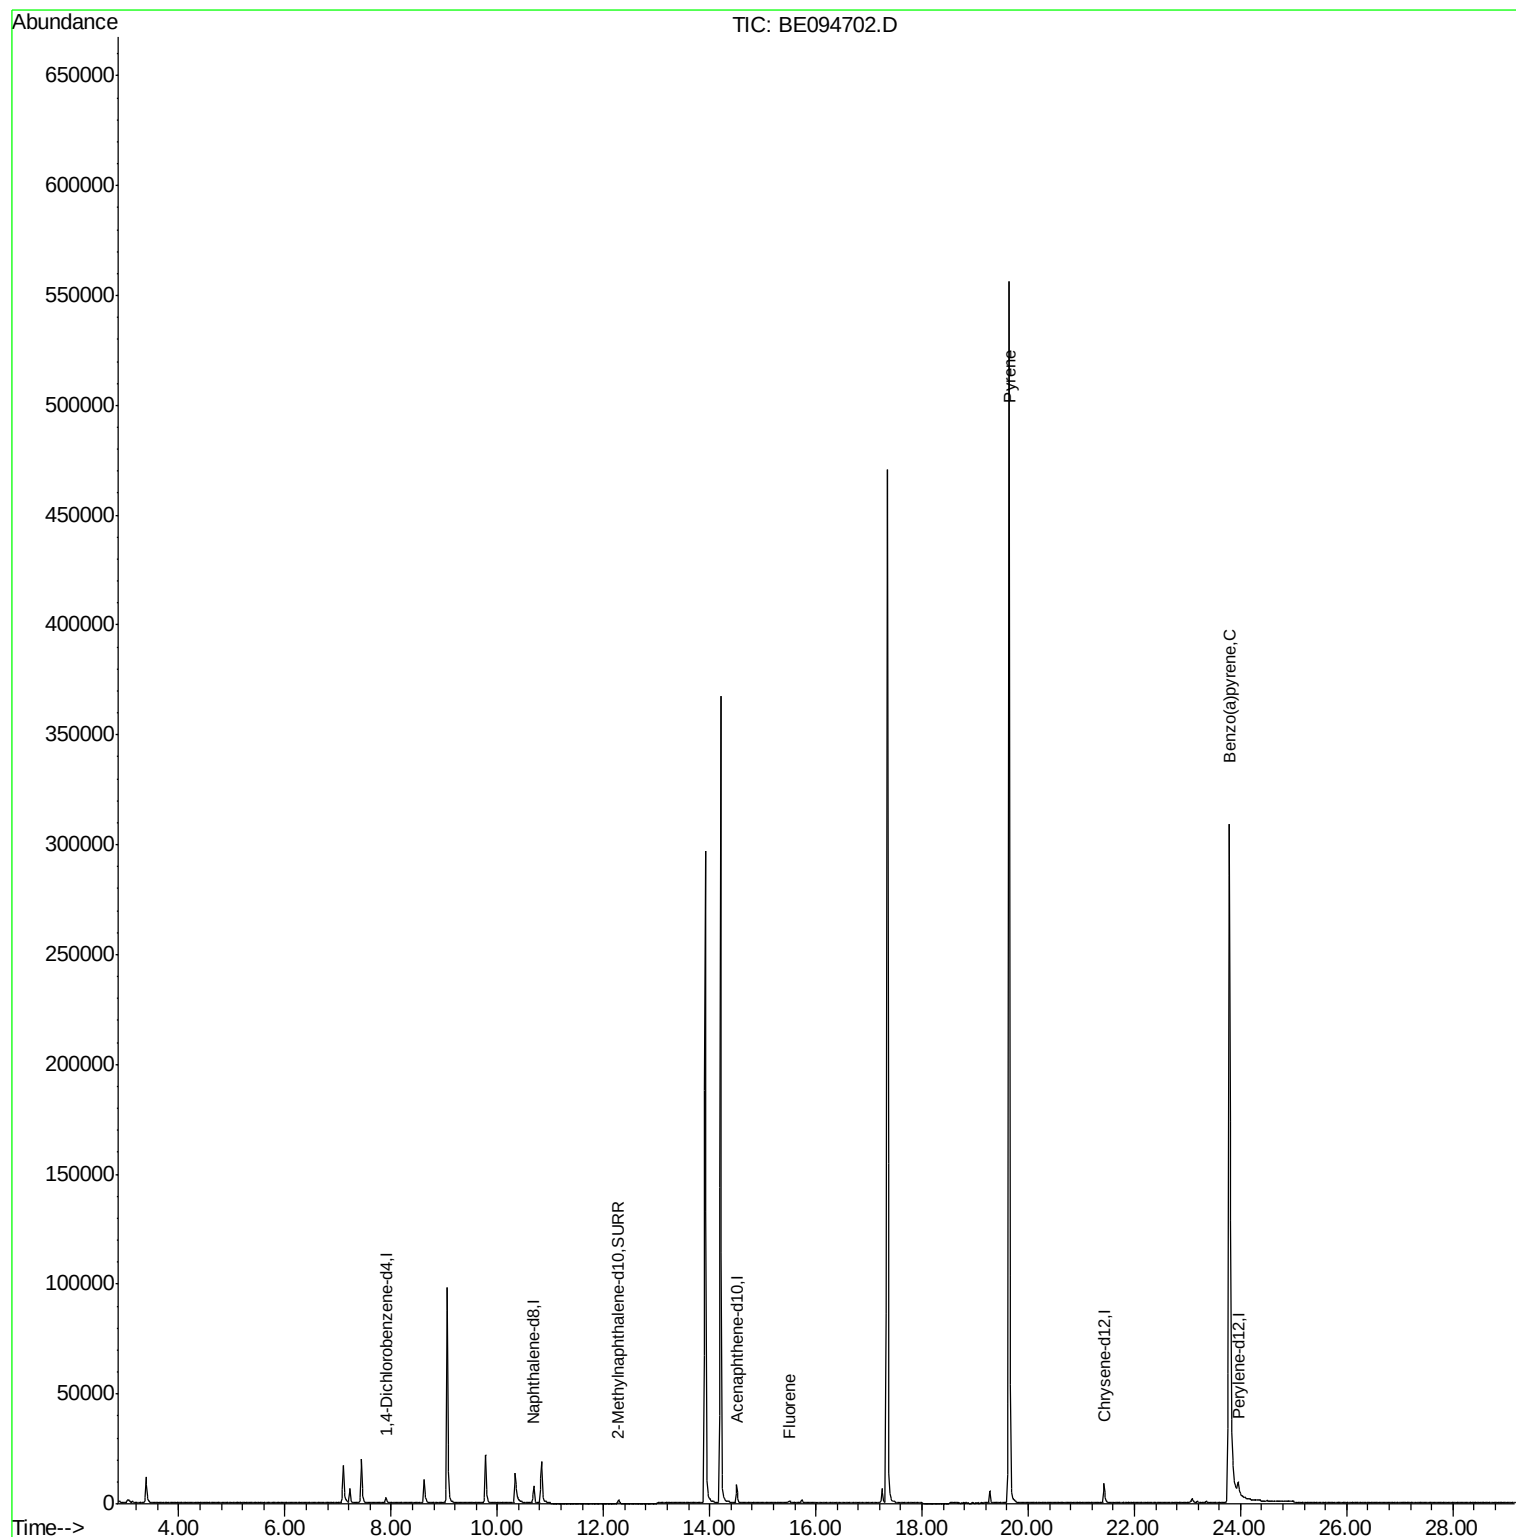


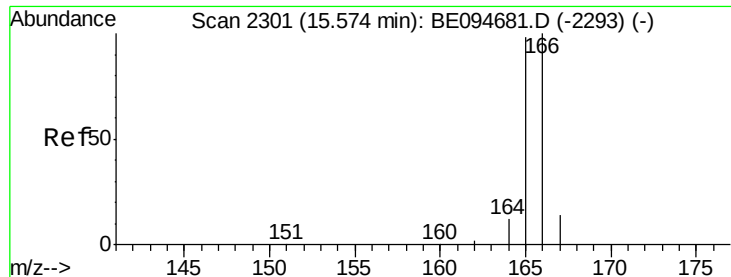

#9
Fluorene
 Concen: 0.05 ng/ul
 RT: 15.51 min Scan# 2292
 Delta R.T. -0.08 min
 Lab File: BE094702.D
 Acq: 3 Nov 2017 11:09




Instrument :
 BNA_E
 ClientSampleId :
 SBLK06




Tot Ion:166 Resp: 894
 Ion Ratio Lower Upper
 166 100
 165 12.1 73.4 110.2#
 167 39.9 14.6 22.0#

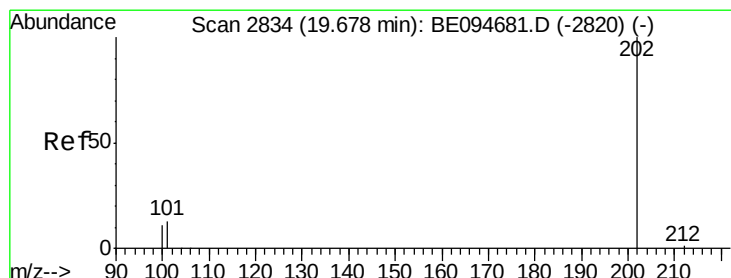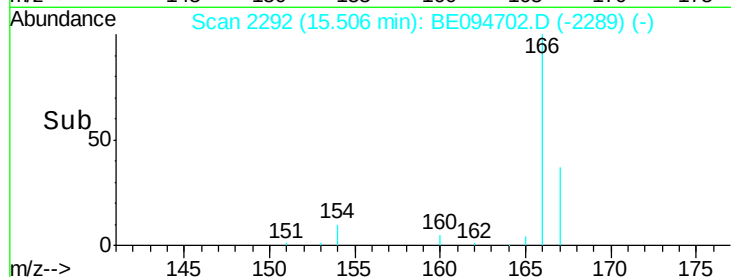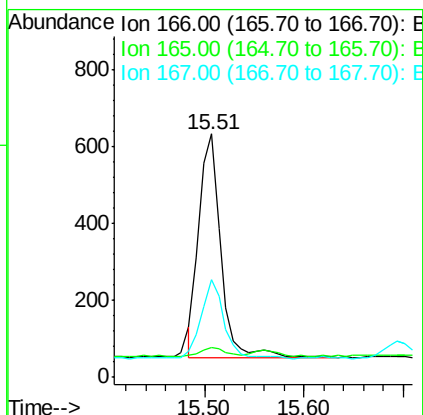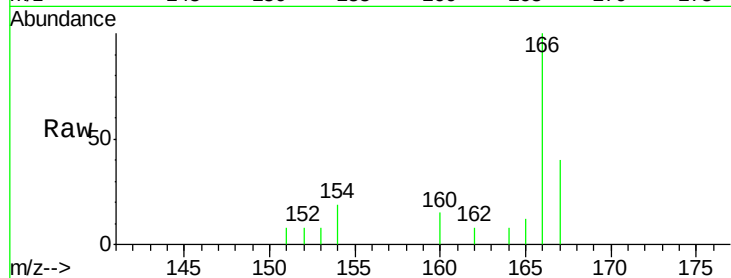

#17
Pyrene
 Concen: 0.03 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.04 min
 Lab File: BE094702.D
 Acq: 3 Nov 2017 11:09

Tgt Ion:202 Resp: 936
 Ion Ratio Lower Upper
 202 100
 101 149.8 18.2 27.4#
 100 804.6 15.6 23.4#

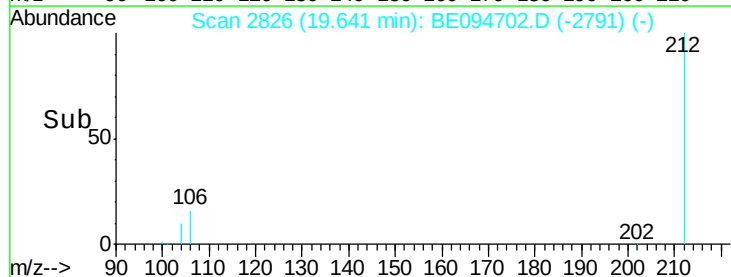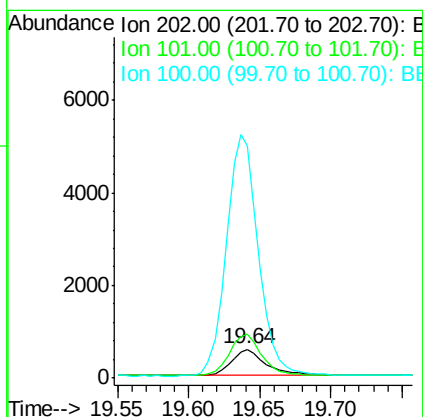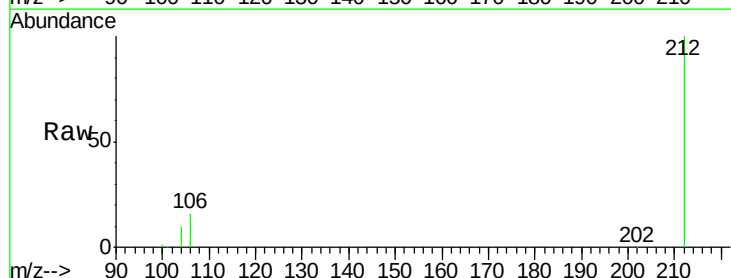

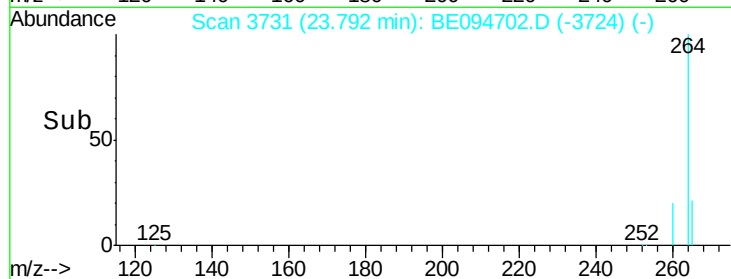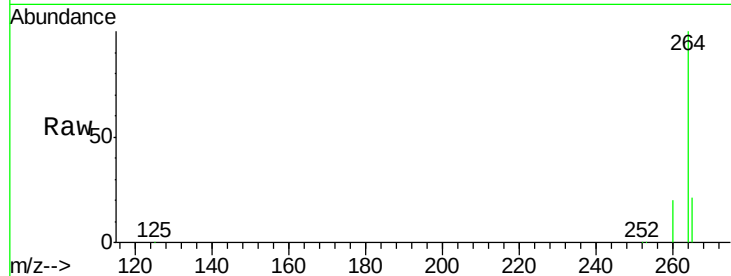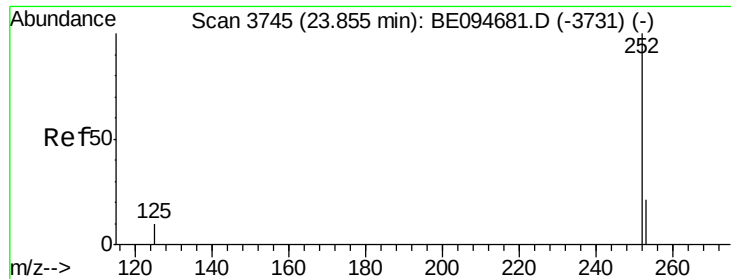

#23

Benzo(a)pyrene

Concen: 0.03 ng/ul

RT: 23.79 min Scan# 3731

Delta R.T. -0.07 min

Lab File: BE094702.D

Acq: 3 Nov 2017 11:09

Instrument :

BNA_E

ClientSampleId :

SBLK06

Tot Ion: 252 Resp: 1813

Ion Ratio Lower Upper

252 100

253 45.2 28.5 42.7#

125 39.3 18.1 27.1#

