

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110317\
 Data File : BE094703.D
 Acq On : 3 Nov 2017 11:48
 Operator : SJ/JU
 Sample : PB103624BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK24

Quant Time: Nov 03 23:58:36 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 03 23:54:30 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1414	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	8700	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.51	164	4985	0.40	ng/ul	-0.02
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	10542	0.40	ng/ul	0.00
20) Perylene-d12	23.79	264	514356	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3233	0.23	ng/ul	-0.02
14) Fluoranthene-d10	19.28	212	7256	0.00	ng/ul	-0.01
Target Compounds						
9) Fluorene	15.50	166	911	0.05	ng/ul#	24
17) Pyrene	19.64	202	943	0.03	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110317\
Data File : BE094703.D
Acq On : 3 Nov 2017 11:48
Operator : SJ/JU
Sample : PB103624BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK24

Quant Time: Nov 03 23:58:36 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 23:54:30 2017
Response via : Initial Calibration




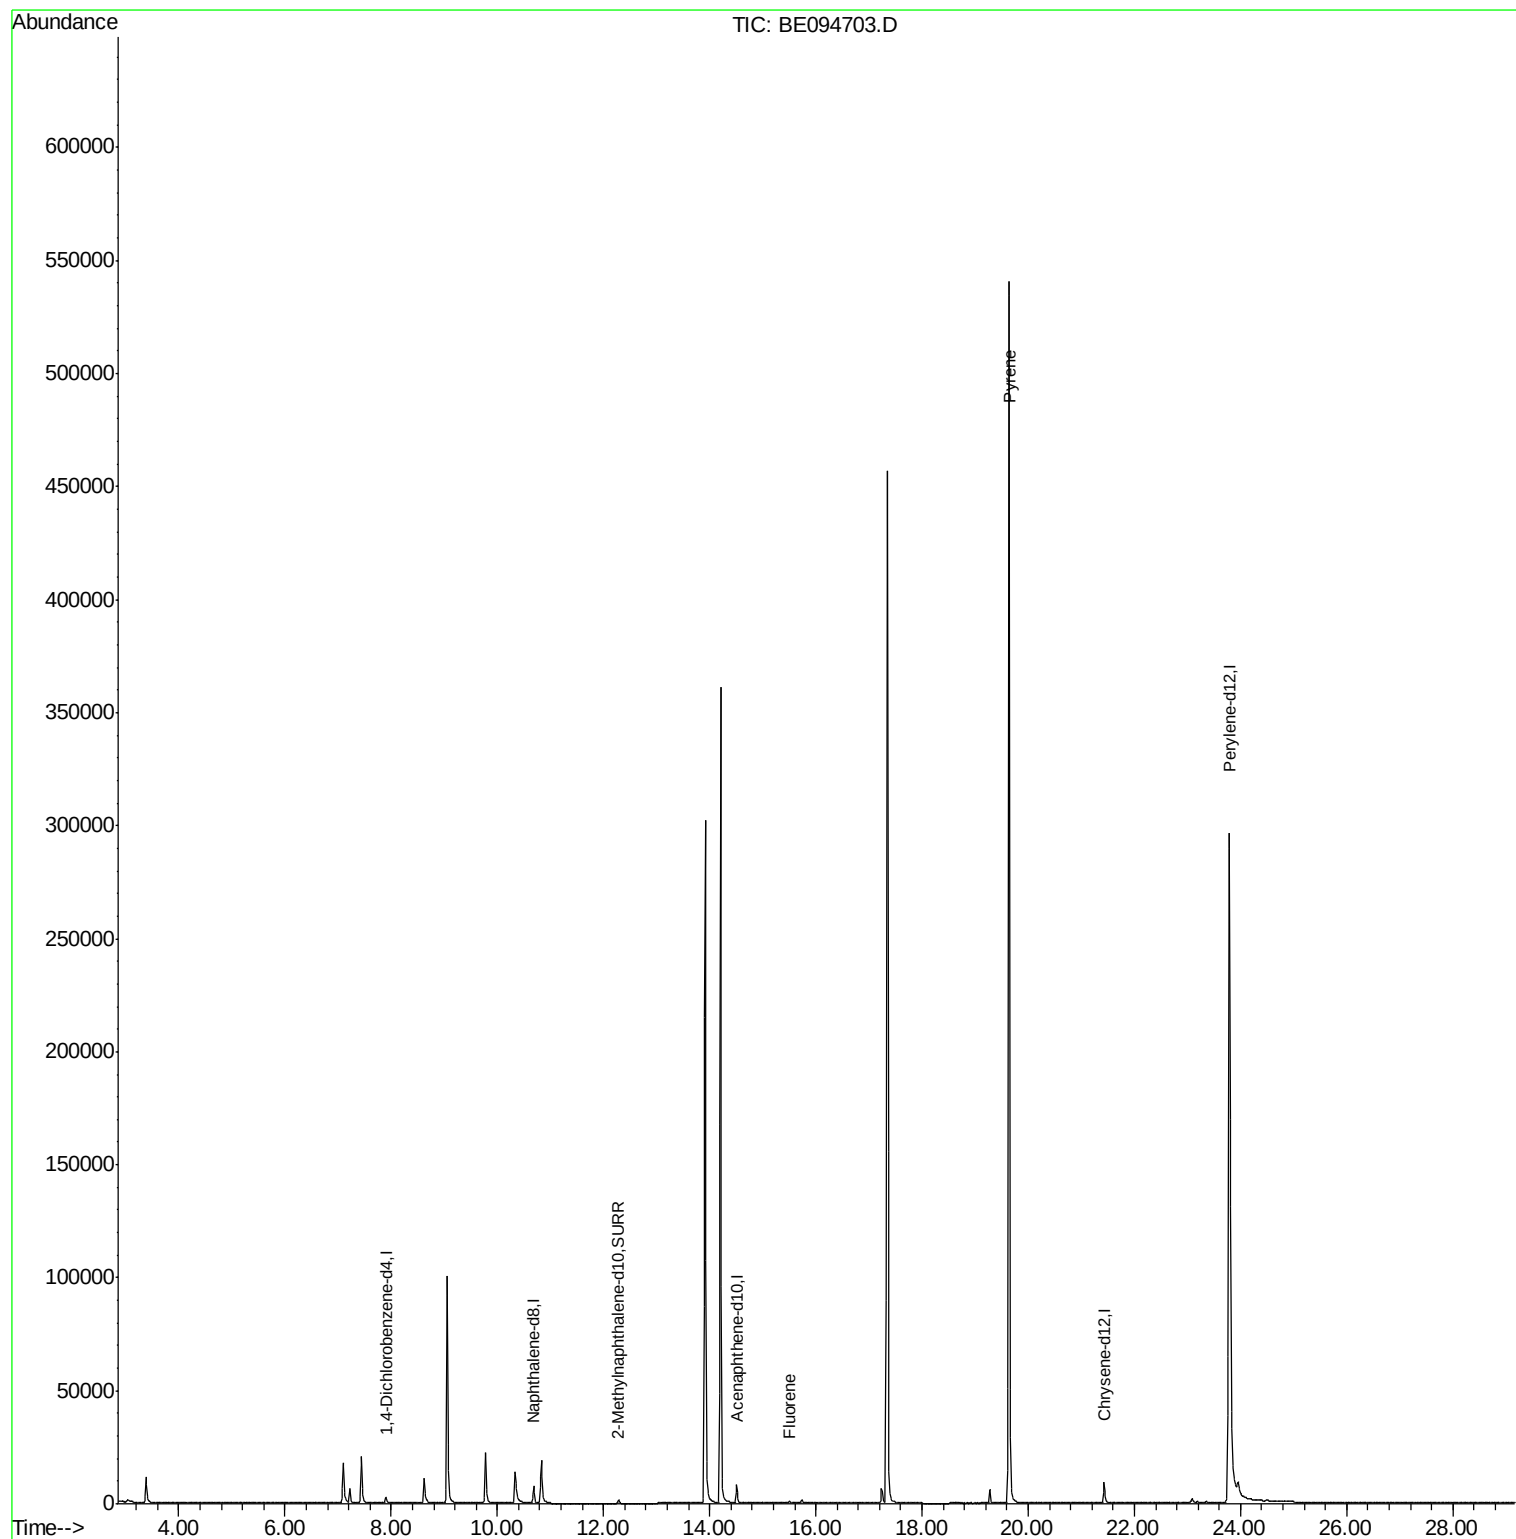


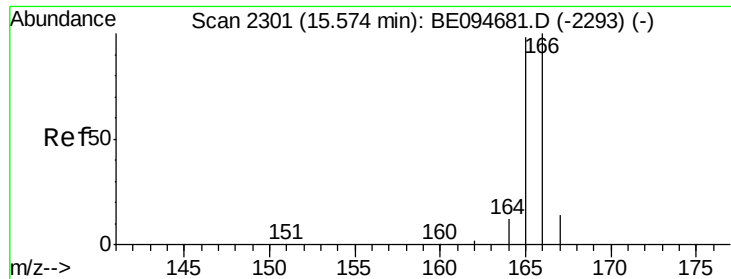

#9
Fluorene
 Concen: 0.05 ng/ul
 RT: 15.50 min Scan# 2291
 Delta R.T. -0.08 min
 Lab File: BE094703.D
 Acq: 3 Nov 2017 11:48

Instrument :
 BNA_E
 ClientSampleId :
 SBLK24

Tot Ion:166 Resp: 911
 Ion Ratio Lower Upper
 166 100
 165 11.9 73.4 110.2#
 167 35.2 14.6 22.0#

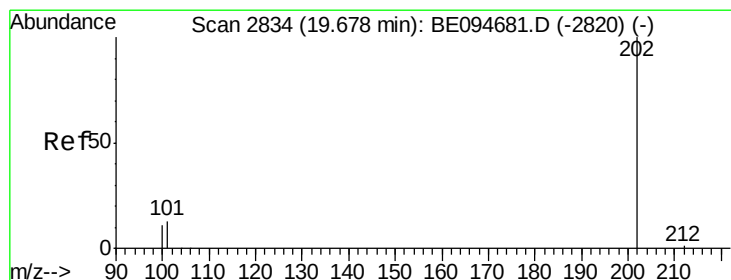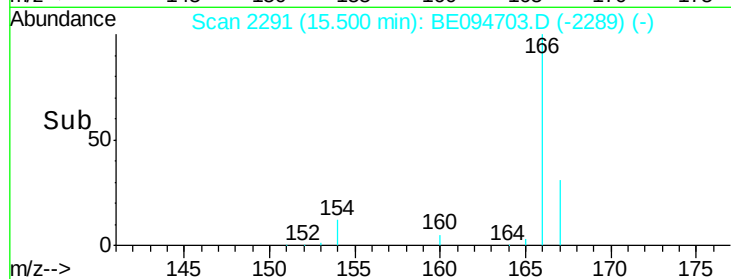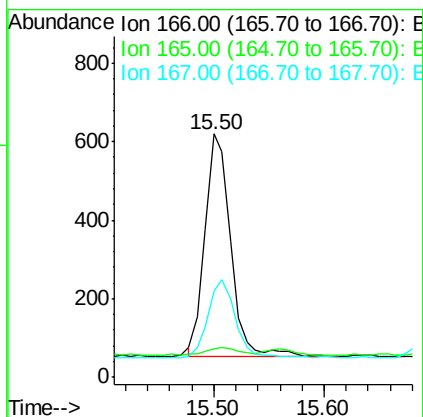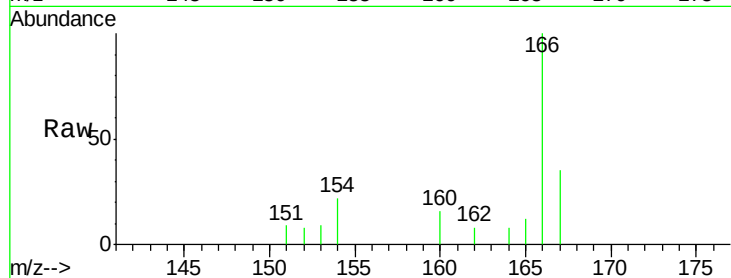

#17
Pyrene
 Concen: 0.03 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.04 min
 Lab File: BE094703.D
 Acq: 3 Nov 2017 11:48

Tgt Ion:202 Resp: 943
 Ion Ratio Lower Upper
 202 100
 101 155.0 18.2 27.4#
 100 789.6 15.6 23.4#

