

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110424\  
 Data File : BE101454.D  
 Acq On : 4 Nov 2024 13:25  
 Operator : RC/JU  
 Sample : PB164593BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 PB164593BL

Quant Time: Nov 04 13:19:19 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Oct 29 01:26:30 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc    | Units | Dev(Min) |
|-----------------------------|--------|------|----------|---------|-------|----------|
| -----                       |        |      |          |         |       |          |
| Internal Standards          |        |      |          |         |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.573  | 152  | 83697    | 20.000  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.341 | 136  | 332383   | 20.000  | ng    | 0.00     |
| 39) Acenaphthene-d10        | 14.177 | 164  | 209474   | 20.000  | ng    | 0.00     |
| 64) Phenanthrene-d10        | 16.915 | 188  | 478774   | 20.000  | ng    | 0.00     |
| 76) Chrysene-d12            | 21.075 | 240  | 637683   | 20.000  | ng    | 0.00     |
| 86) Perylene-d12            | 23.372 | 264  | 926419   | 20.000  | ng    | 0.00     |
| System Monitoring Compounds |        |      |          |         |       |          |
| 5) 2-Fluorophenol           | 5.323  | 112  | 599545   | 125.548 | ng    | 0.00     |
| 7) Phenol-d6                | 6.951  | 99   | 740437   | 111.822 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 8.784  | 82   | 428697   | 81.009  | ng    | 0.00     |
| 42) 2,4,6-Tribromophenol    | 15.687 | 330  | 459560   | 125.173 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 12.802 | 172  | 1067682  | 86.319  | ng    | 0.00     |
| 79) Terphenyl-d14           | 19.512 | 244  | 2218492  | 80.071  | ng    | 0.00     |


|                  |        |
|------------------|--------|
| Target Compounds | Qvalue |
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110424\  
Data File : BE101454.D  
Acq On : 4 Nov 2024 13:25  
Operator : RC/JU  
Sample : PB164593BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PB164593BL

Quant Time: Nov 04 13:19:19 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

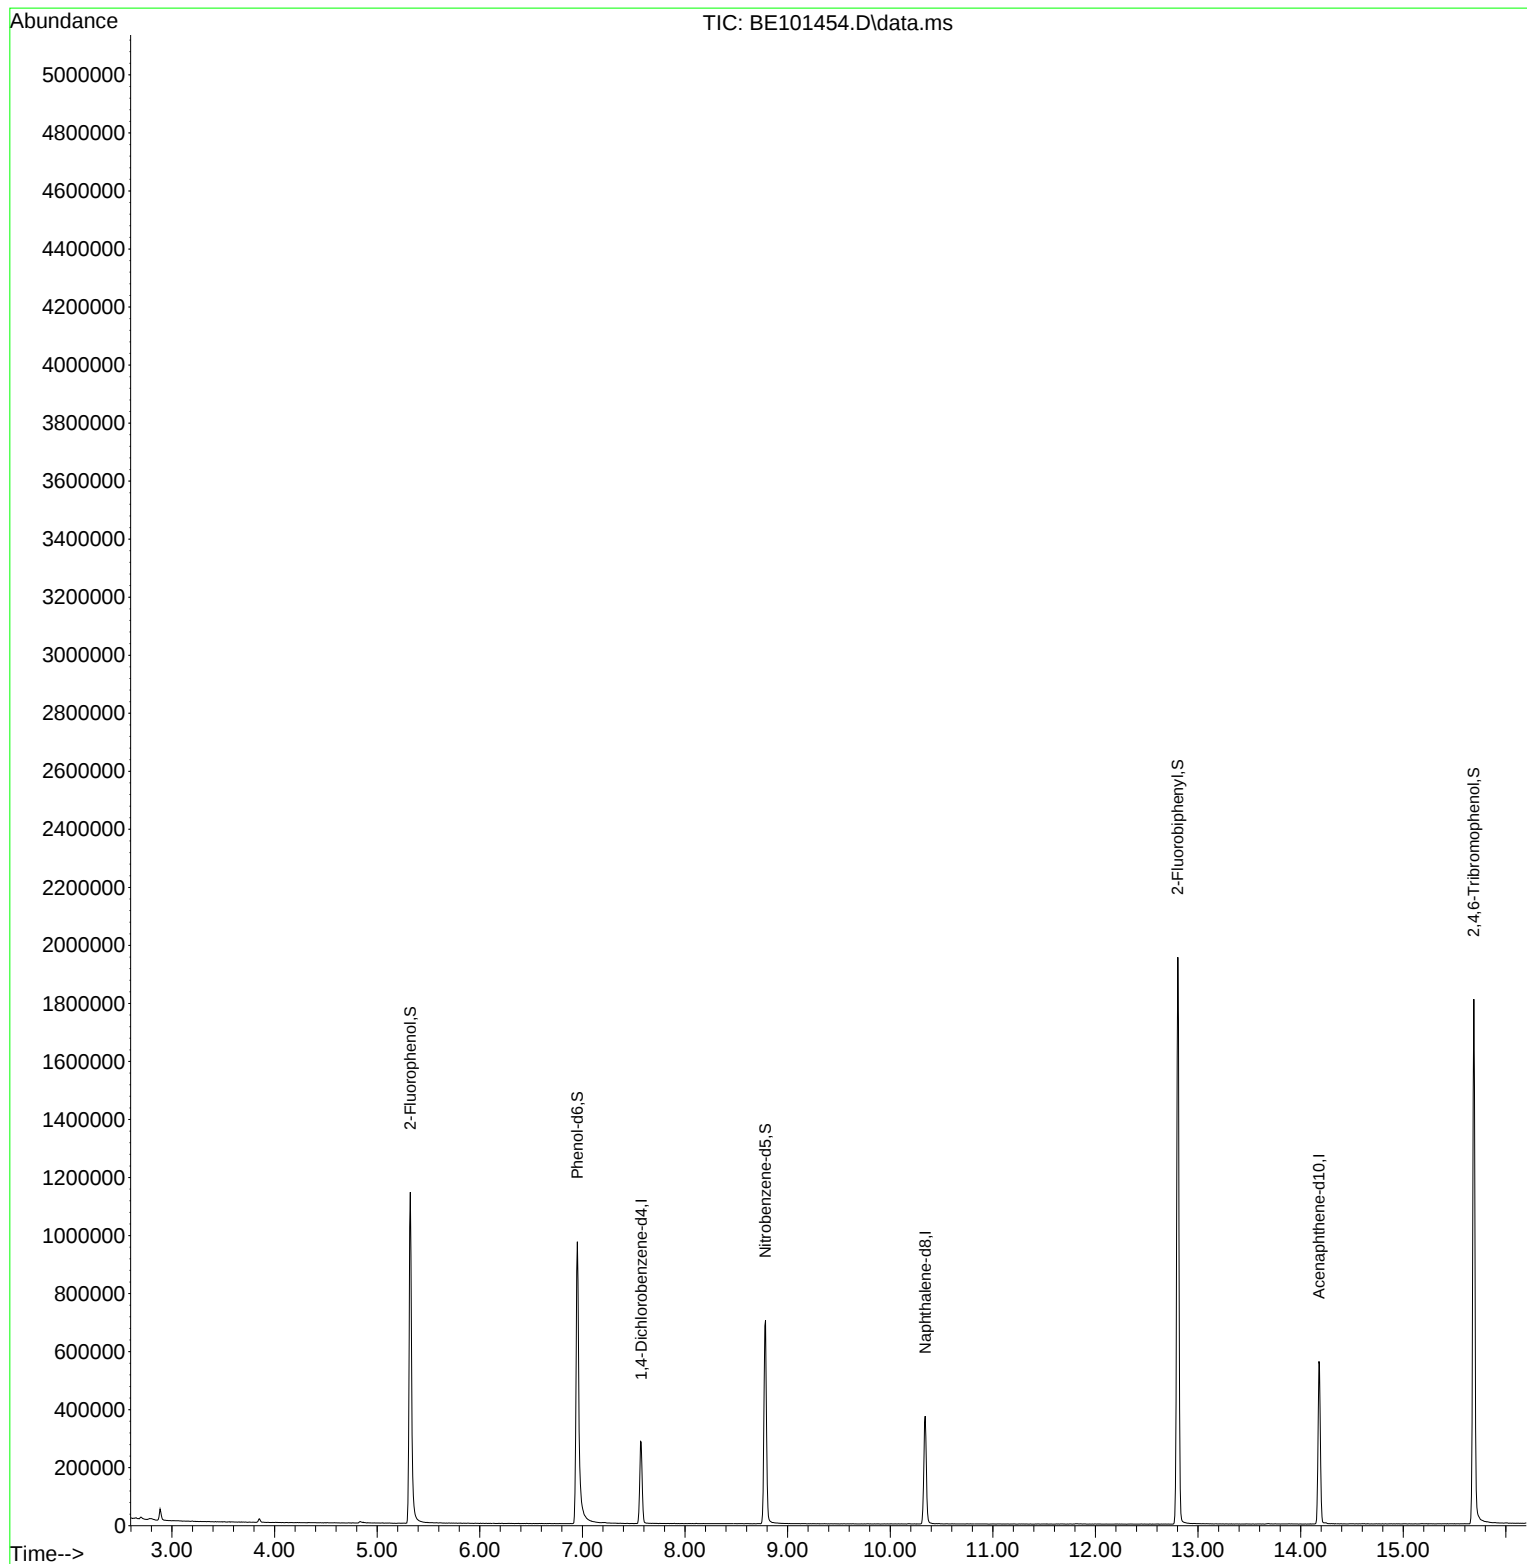

Data Path : Z:\svoasrv\HPCHEM1\BNA\_E\Data\BE110424\  
Data File : BE101454.D  
Acq On : 4 Nov 2024 13:25  
Operator : RC/JU  
Sample : PB164593BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
PB164593BL

Quant Time: Nov 04 13:19:19 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_E\Methods\8270-BE102824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 29 01:26:30 2024  
Response via : Initial Calibration

