
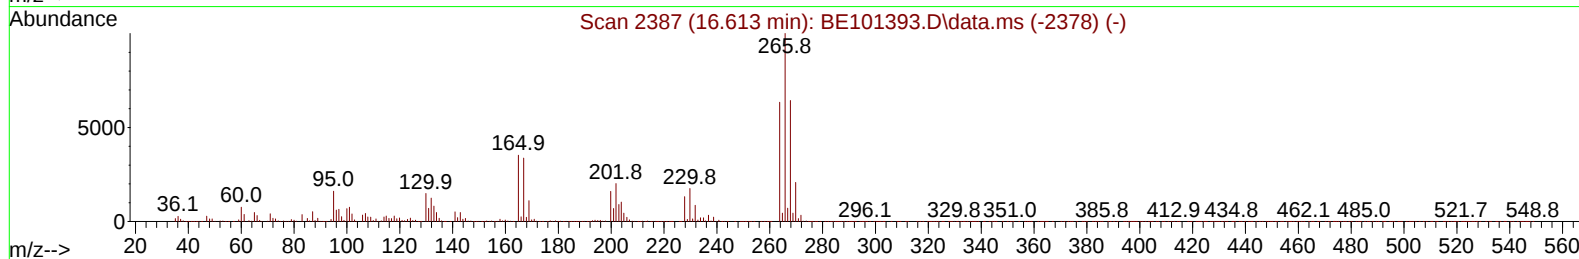
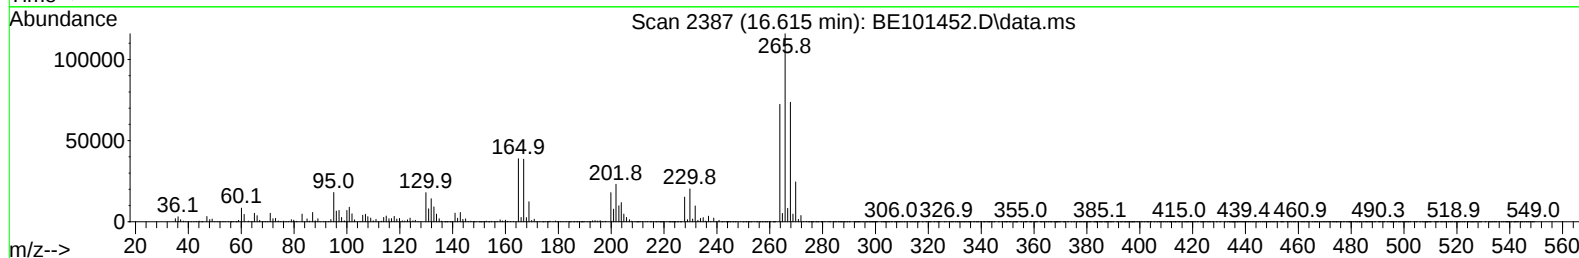


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101452.D
Acq On : 4 Nov 2024 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 19:28:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

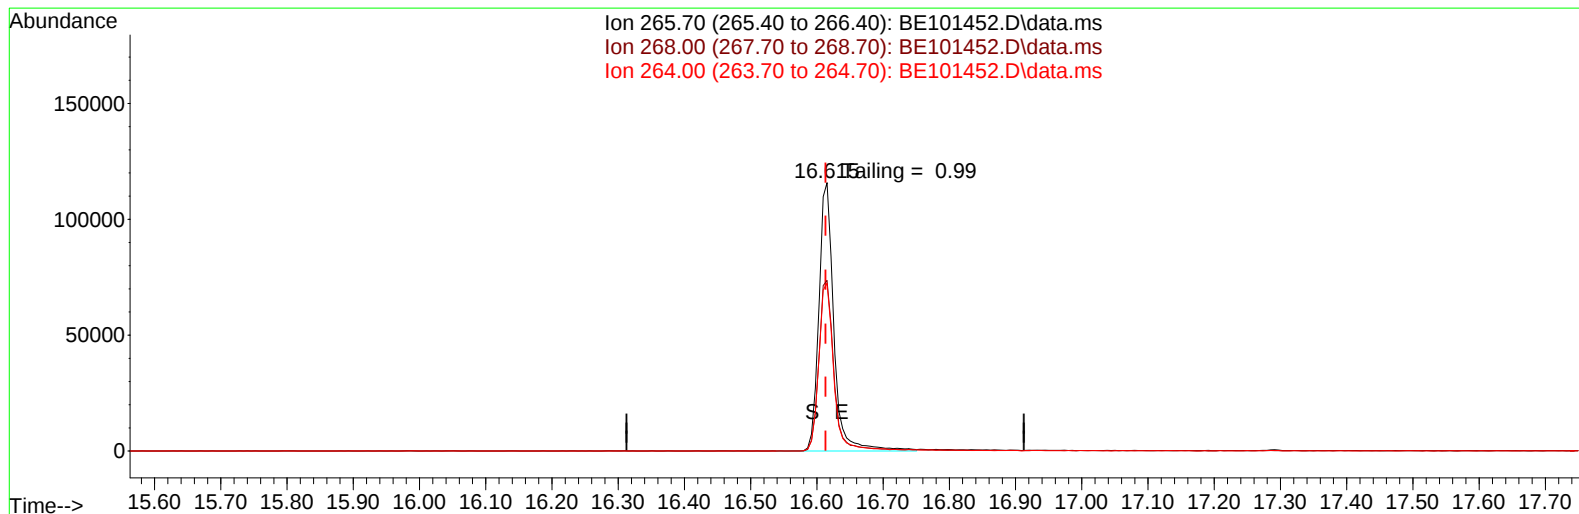

TIC: BE101452.D\data.ms

(70) Pentachlorophenol (C)




16.615min (+ 0.003) 502373.06 ng

response 175435

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.57
264.00	63.40	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101452.D
Acq On : 4 Nov 2024 12:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 19:28:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

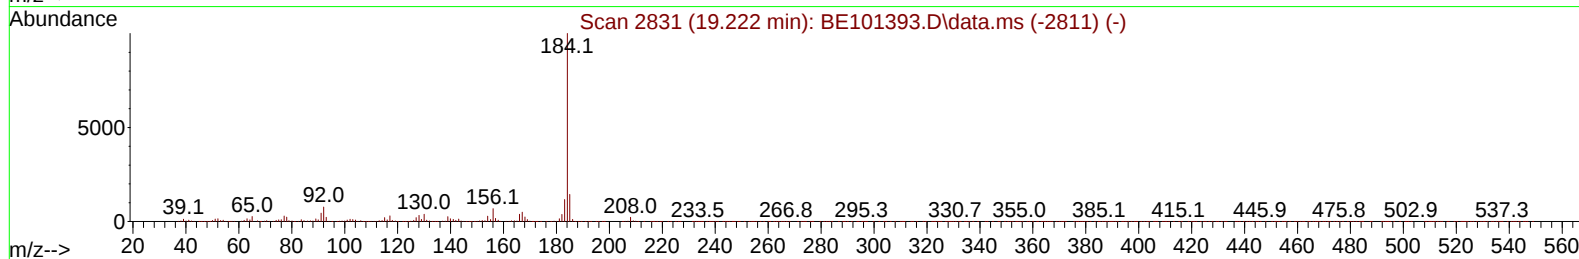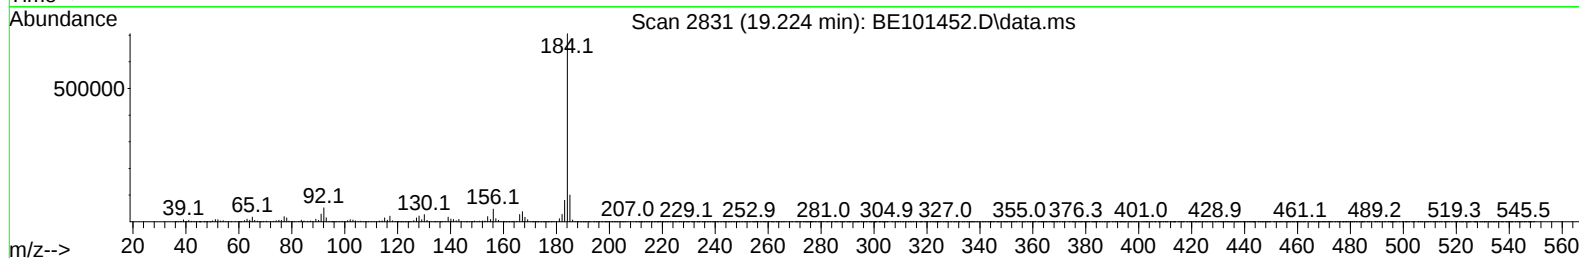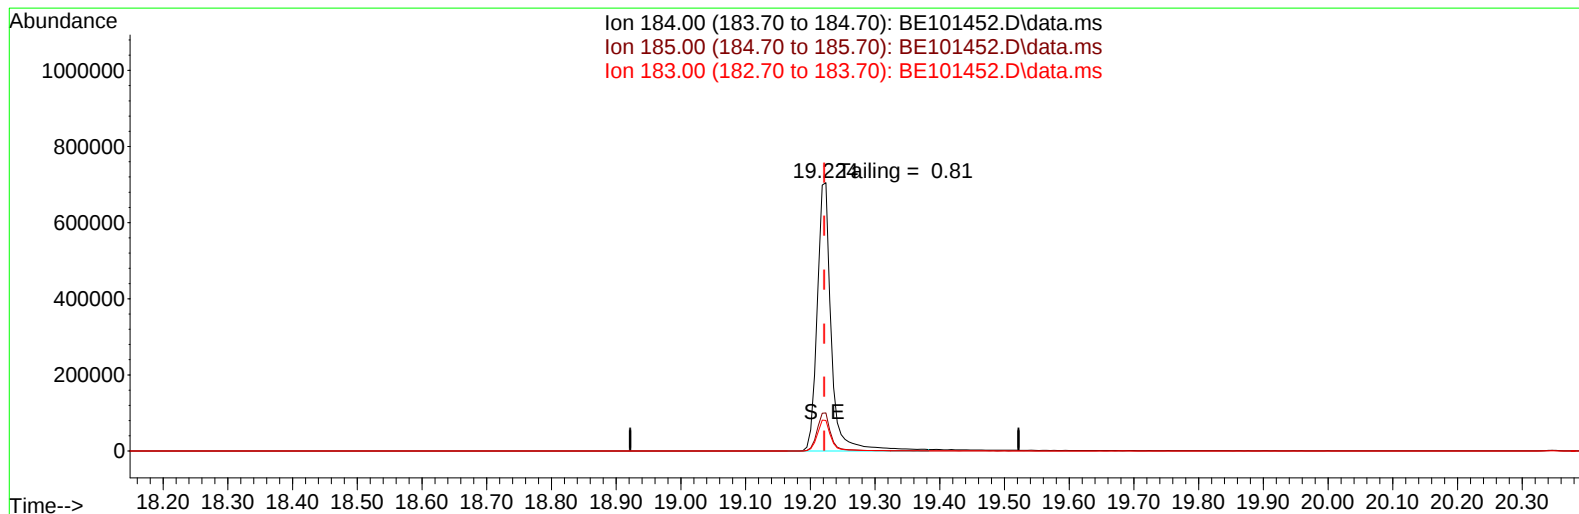

TIC: BE101452.D\data.ms

(77) Benzidine

19.224min (+ 0.003) 969740.64 ng m

response 1070765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	11.60	11.43
0.00	0.00	0.00