

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
 Data File : BE101454.D
 Acq On : 4 Nov 2024 13:25
 Operator : RC/JU
 Sample : PB164593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164593BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.323	458	465	492	rBV	1140970	1930114	33.78%	8.180%
2	6.951	734	742	766	rBV	971928	1927709	33.74%	8.170%
3	7.567	841	847	856	rBV	282569	459483	8.04%	1.947%
4	8.784	1046	1054	1066	rBV	700945	1207306	21.13%	5.117%
5	10.341	1311	1319	1331	rBV	371781	643539	11.26%	2.727%
6	12.802	1730	1738	1755	rBV	1953596	3002582	52.55%	12.725%
7	14.177	1965	1972	1981	rBV	560327	878867	15.38%	3.725%
8	15.687	2221	2229	2250	rBV	1808476	2714592	47.51%	11.505%
9	16.915	2432	2438	2451	rBV	720842	1125552	19.70%	4.770%
10	19.512	2873	2880	2894	rBV	4259678	5713582	100.00%	24.215%
11	21.075	3141	3146	3157	rBV	1332540	1727696	30.24%	7.322%
12	23.367	3529	3536	3548	rVB	1114622	2264302	39.63%	9.596%




Sum of corrected areas: 23595324

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101454.D
Acq On : 4 Nov 2024 13:25
Operator : RC/JU
Sample : PB164593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164593BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

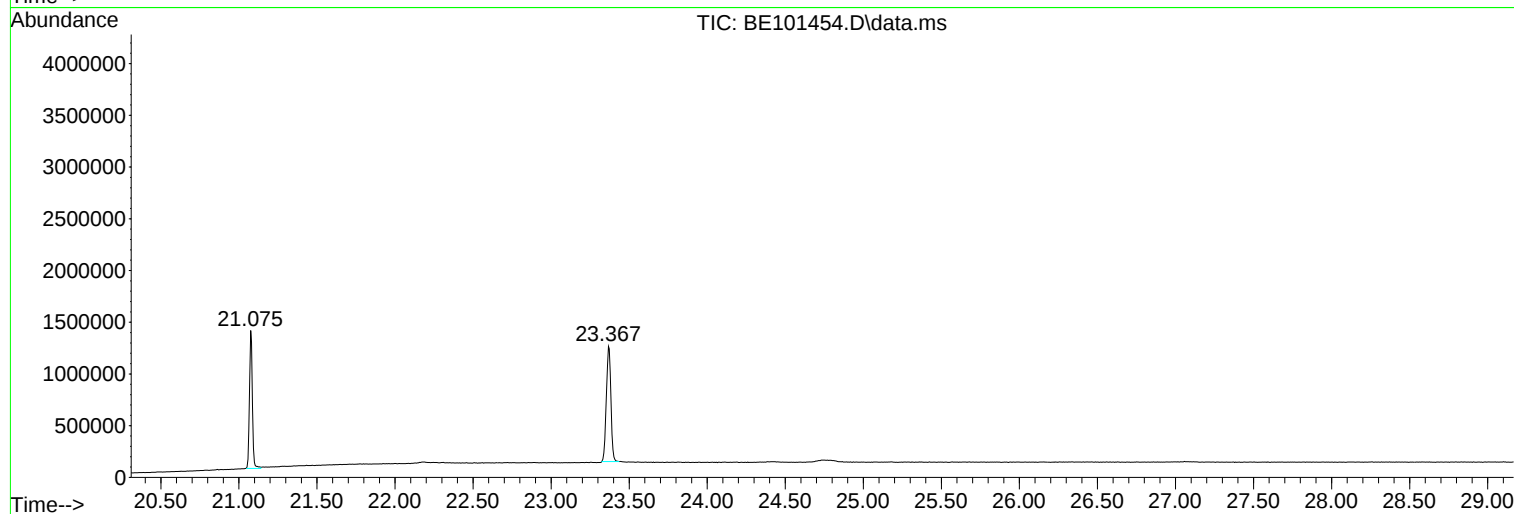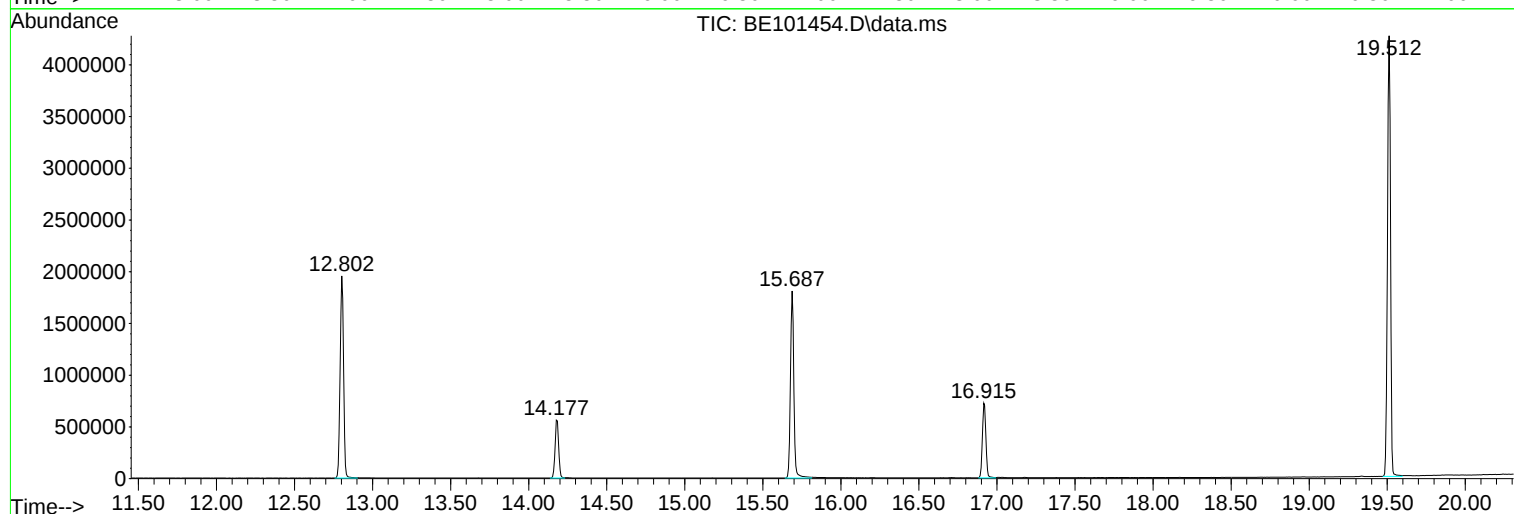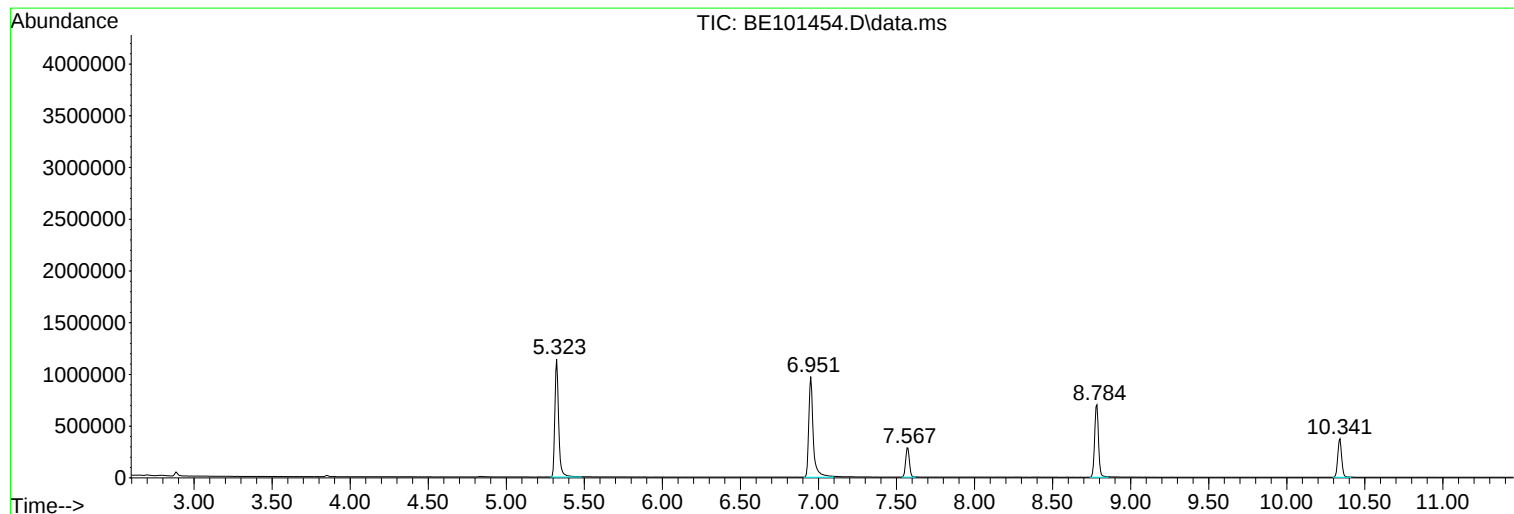

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101454.D
Acq On : 4 Nov 2024 13:25
Operator : RC/JU
Sample : PB164593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164593BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101454.D
Acq On : 4 Nov 2024 13:25
Operator : RC/JU
Sample : PB164593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164593BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------