

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
 Data File : BE101469.D
 Acq On : 4 Nov 2024 23:25
 Operator : RC/JU
 Sample : P4667-09 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-F-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.876	45	49	61	rVB	131238	193952	10.59%	2.123%
2	5.320	459	465	485	rBV	121067	220386	12.03%	2.412%
3	6.947	736	742	763	rBV	102512	235354	12.85%	2.576%
4	7.570	837	848	857	rBV	267101	427678	23.34%	4.681%
5	8.780	1046	1054	1065	rBV	82580	149014	8.13%	1.631%
6	10.337	1311	1319	1332	rBV	385735	668690	36.50%	7.318%
7	11.601	1529	1534	1540	rBV	13064	21169	1.16%	0.232%
8	12.799	1731	1738	1745	rBV	279687	427115	23.31%	4.675%
9	12.864	1745	1749	1756	rVB	17489	28853	1.57%	0.316%
10	13.522	1850	1861	1866	rBV7	8250	23240	1.27%	0.254%
11	14.180	1965	1973	1982	rBV	644536	973376	53.13%	10.653%
12	15.549	2202	2206	2211	rBV	18180	23605	1.29%	0.258%
13	15.684	2223	2229	2236	rBV	242648	362420	19.78%	3.966%
14	15.749	2236	2240	2246	rVB3	12193	24994	1.36%	0.274%
15	16.918	2432	2439	2445	rBV	819139	1221238	66.66%	13.366%
16	19.327	2847	2849	2854	rVB	22494	25069	1.37%	0.274%
17	19.503	2874	2879	2884	rBV	604339	752403	41.07%	8.235%
18	21.078	3142	3147	3152	rBV	1169995	1526551	83.33%	16.707%
19	23.369	3531	3537	3546	rVB	940138	1831997	100.00%	20.050%




Sum of corrected areas: 9137104

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101469.D
Acq On : 4 Nov 2024 23:25
Operator : RC/JU
Sample : P4667-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

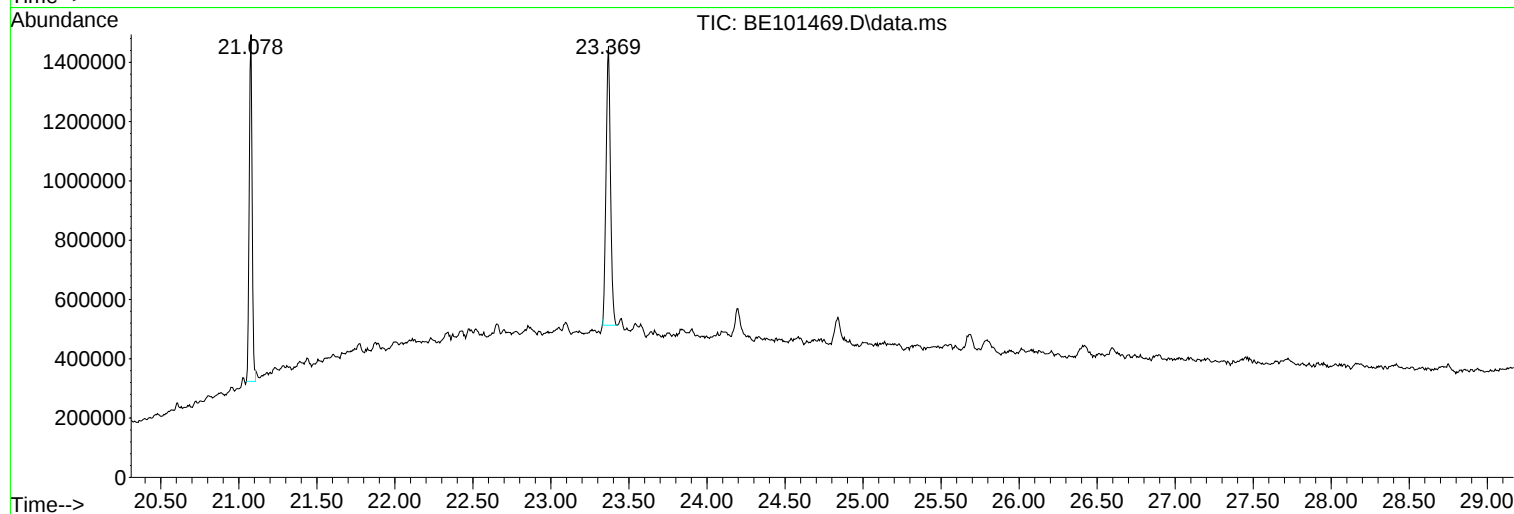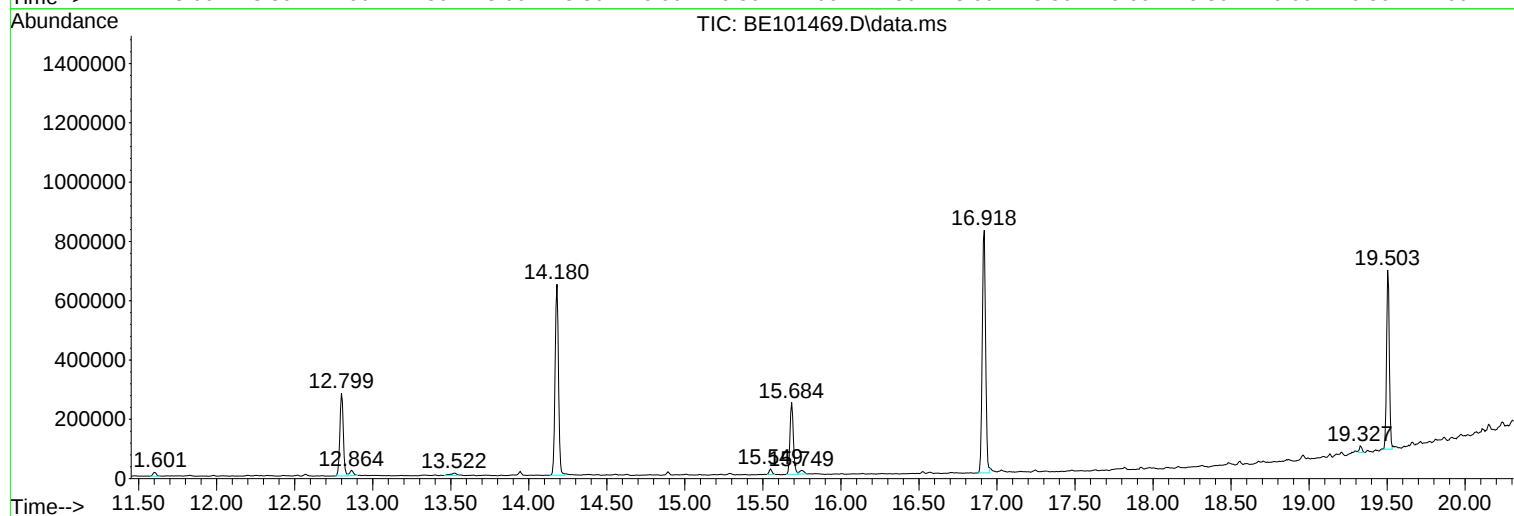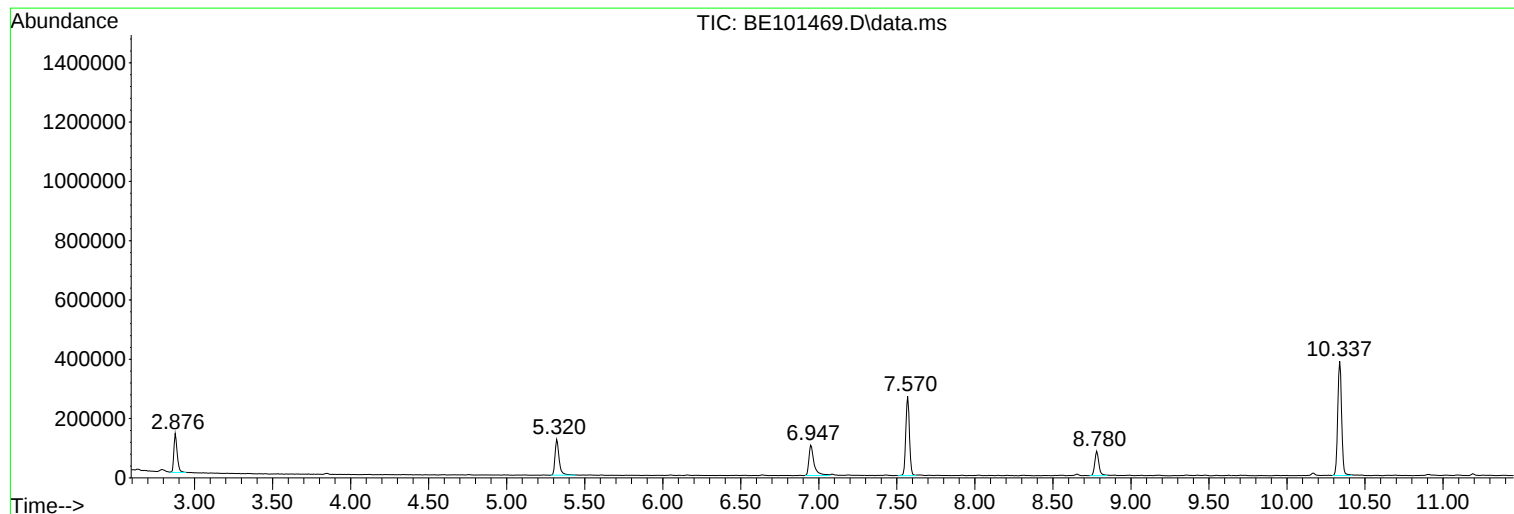

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101469.D
Acq On : 4 Nov 2024 23:25
Operator : RC/JU
Sample : P4667-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10










Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.876	9.07 ng	193952	1,4-Dichlorobenzene-d4	7.570

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	64
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	14
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

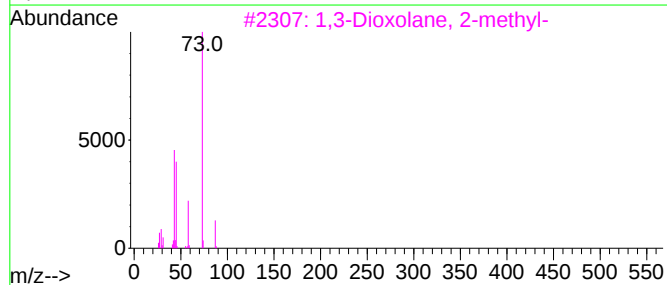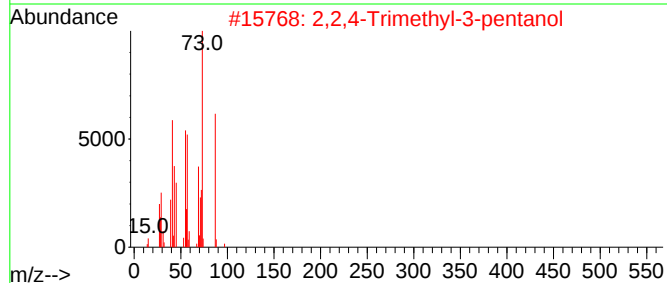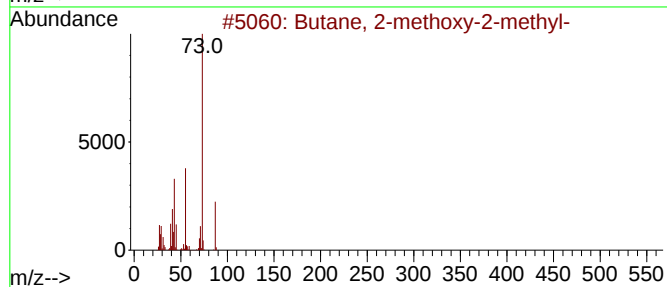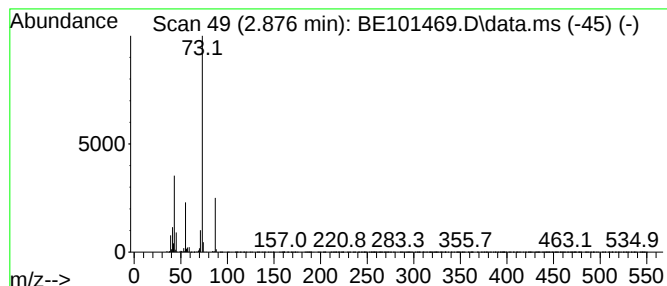

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110424\
Data File : BE101469.D
Acq On : 4 Nov 2024 23:25
Operator : RC/JU
Sample : P4667-09 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-F-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.876	9.1	ng	193952	1	7.570	427678	20.0