

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110515\
 Data File : BE091063.D
 Acq On : 5 Nov 2015 10:52
 Operator : UM/NP
 Sample : PB86441BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK41

Quant Time: Nov 06 05:43:24 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 06 05:41:53 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	4846	0.40	ng/ul	0.00
4) Naphthalene-d8	9.57	136	26736	0.40	ng/ul	0.00
8) Acenaphthene-d10	13.41	164	16303	0.40	ng/ul	0.00
12) Phenanthrene-d10	16.22	188	2390520	0.40	ng/ul	0.09
18) Chrysene-d12	20.29	240	34528	0.40	ng/ul	0.00
22) Perylene-d12	22.07	264	2693823	0.40	ng/ul	-0.12
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.91	96	36835	10.57	ng/uL	-0.04
6) 2-Methylnaphthalene-d10	11.08	152	12259	0.34	ng/ul	0.00
16) Fluoranthene-d10	18.13	212	30397	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
11) Fluorene	14.40	166	4246	0.06	ng/ul#	8
19) Pyrene	18.52	202	17092	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110515\
Data File : BE091063.D
Acq On : 5 Nov 2015 10:52
Operator : UM/NP
Sample : PB86441BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK41

Quant Time: Nov 06 05:43:24 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE102715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 06 05:41:53 2015
Response via : Initial Calibration

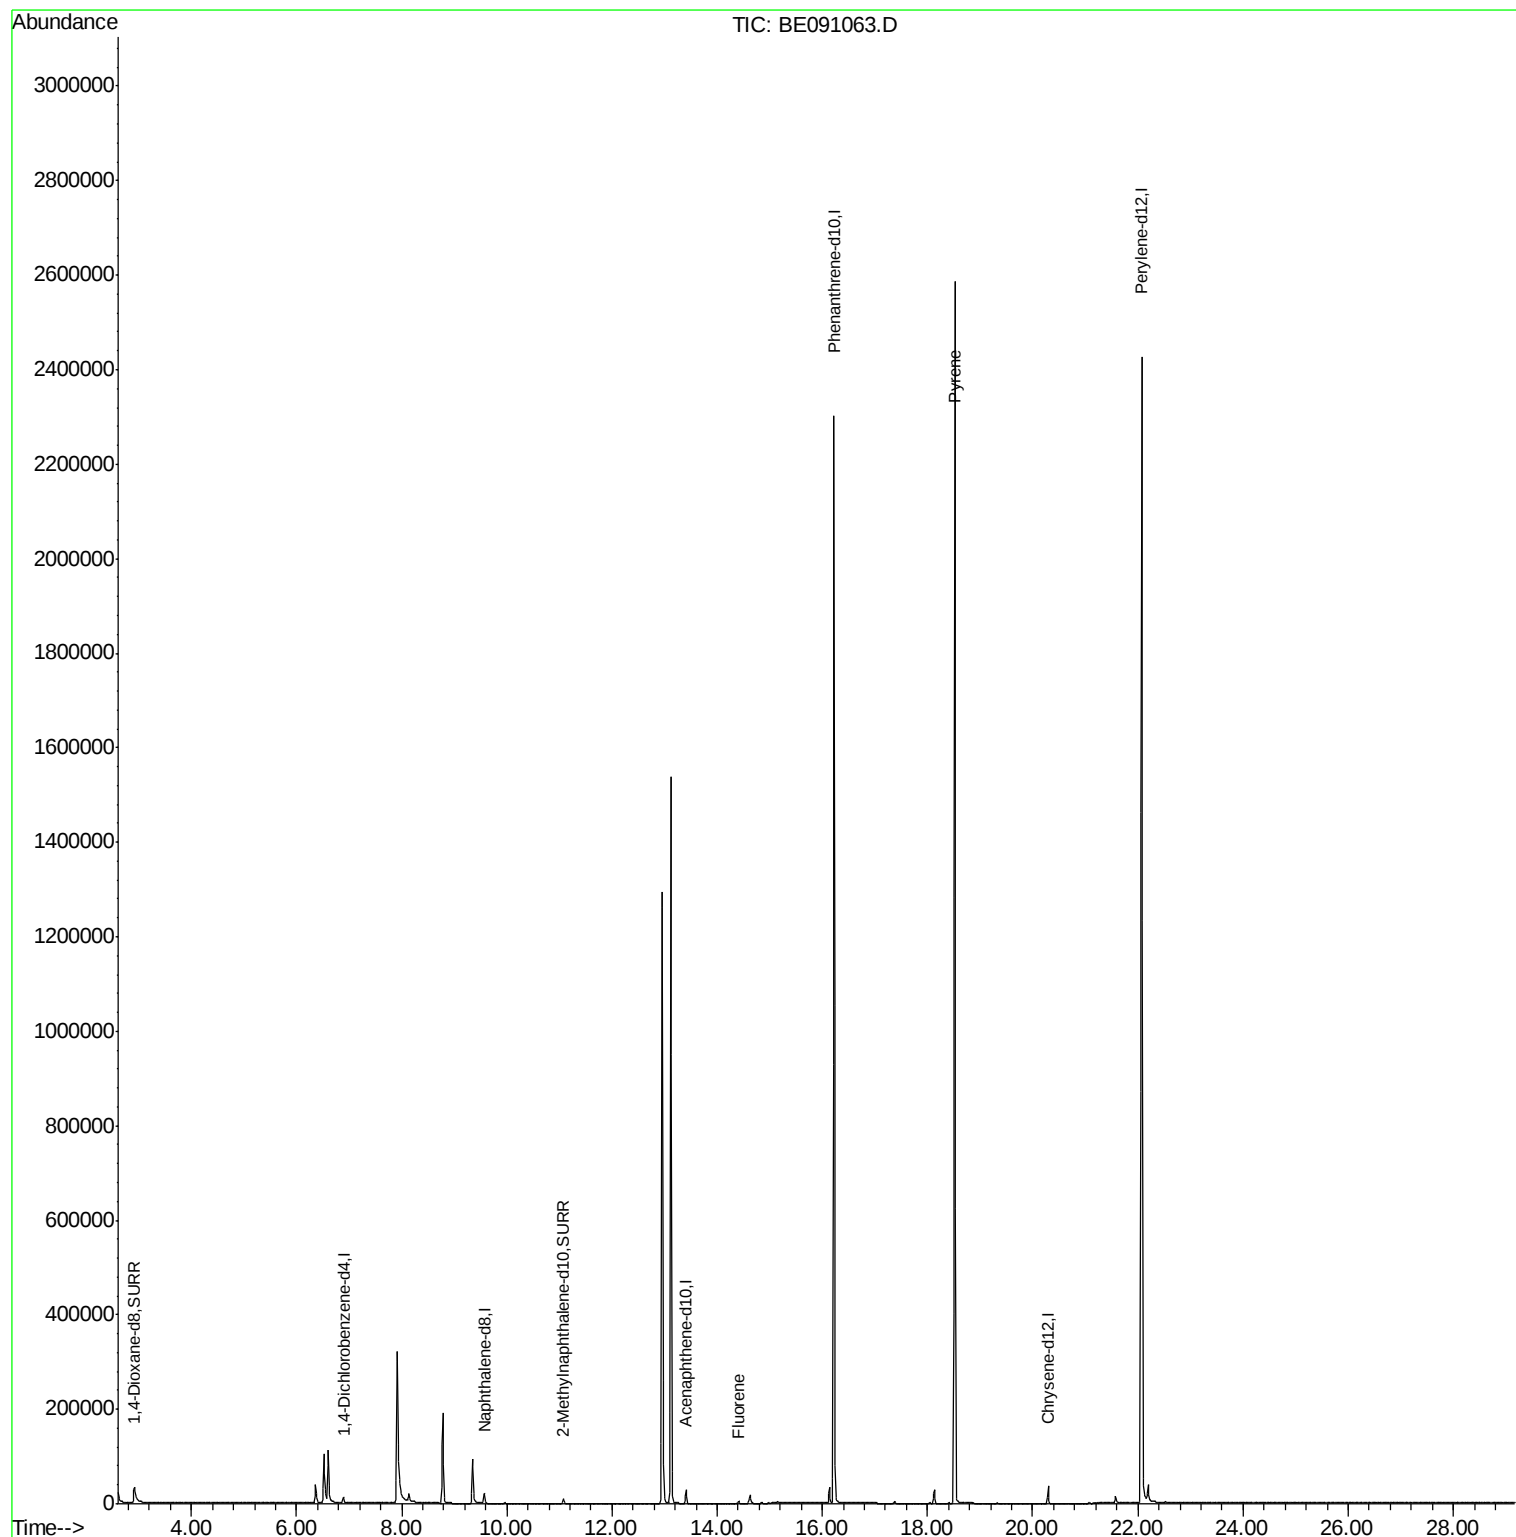

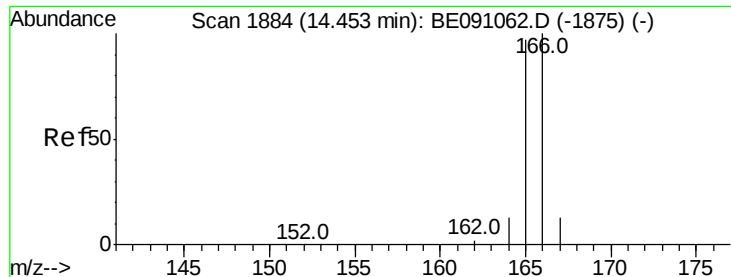

#11

Fluorene

Concen: 0.06 ng/ul

RT: 14.40 min Scan# 1877

Delta R.T. -0.05 min

Lab File: BE091063.D

Acq: 5 Nov 2015 10:52

Instrument :

BNA_E

ClientSampleId :

SBLK41





Tot Ion:166 Resp: 4246

Ion Ratio Lower Upper

166 100

165 9.6 87.6 131.4#

167 40.8 11.1 16.7#

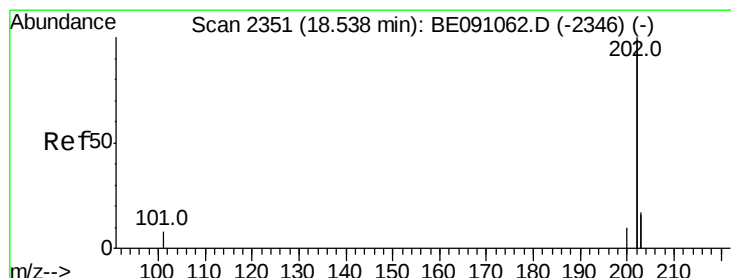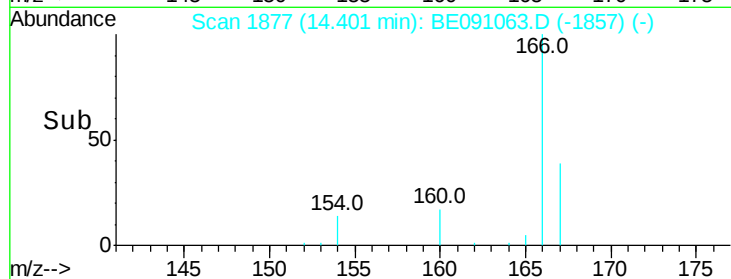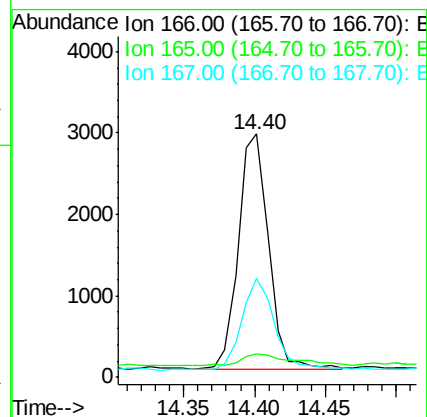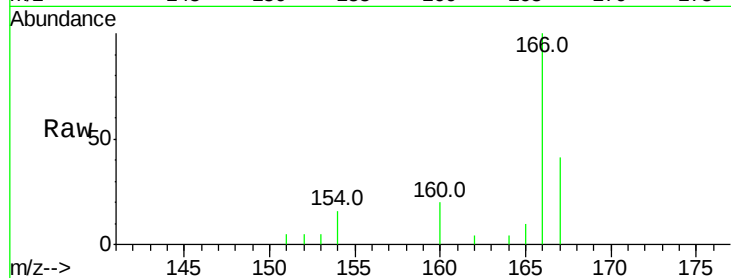

#19

Pyrene

Concen: 0.04 ng/ul

RT: 18.52 min Scan# 2348

Delta R.T. -0.02 min

Lab File: BE091063.D

Acq: 5 Nov 2015 10:52

Tgt Ion:202 Resp: 17092

Ion Ratio Lower Upper

202 100

200 1.5 18.0 27.0#

203 192.2 13.8 20.6#

