

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
 Data File : BE101480.D
 Acq On : 5 Nov 2024 15:43
 Operator : RC/JU
 Sample : P4640-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 MH-3

Quant Time: Nov 05 15:39:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	61100	20.000	ng	0.00
21) Naphthalene-d8	10.337	136	270587	20.000	ng	0.00
39) Acenaphthene-d10	14.179	164	192190	20.000	ng	0.00
64) Phenanthrene-d10	16.917	188	452958	20.000	ng	0.00
76) Chrysene-d12	21.077	240	526766	20.000	ng	0.00
86) Perylene-d12	23.369	264	691787	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.319	112	472752	135.610	ng	0.00
7) Phenol-d6	6.947	99	596595	123.420	ng	0.00
23) Nitrobenzene-d5	8.780	82	366797	85.142	ng	0.00
42) 2,4,6-Tribromophenol	15.689	330	450448	133.725	ng	0.00
45) 2-Fluorobiphenyl	12.799	172	955878	84.230	ng	0.00
79) Terphenyl-d14	19.508	244	2163078	94.509	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101480.D
Acq On : 5 Nov 2024 15:43
Operator : RC/JU
Sample : P4640-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
MH-3

Quant Time: Nov 05 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

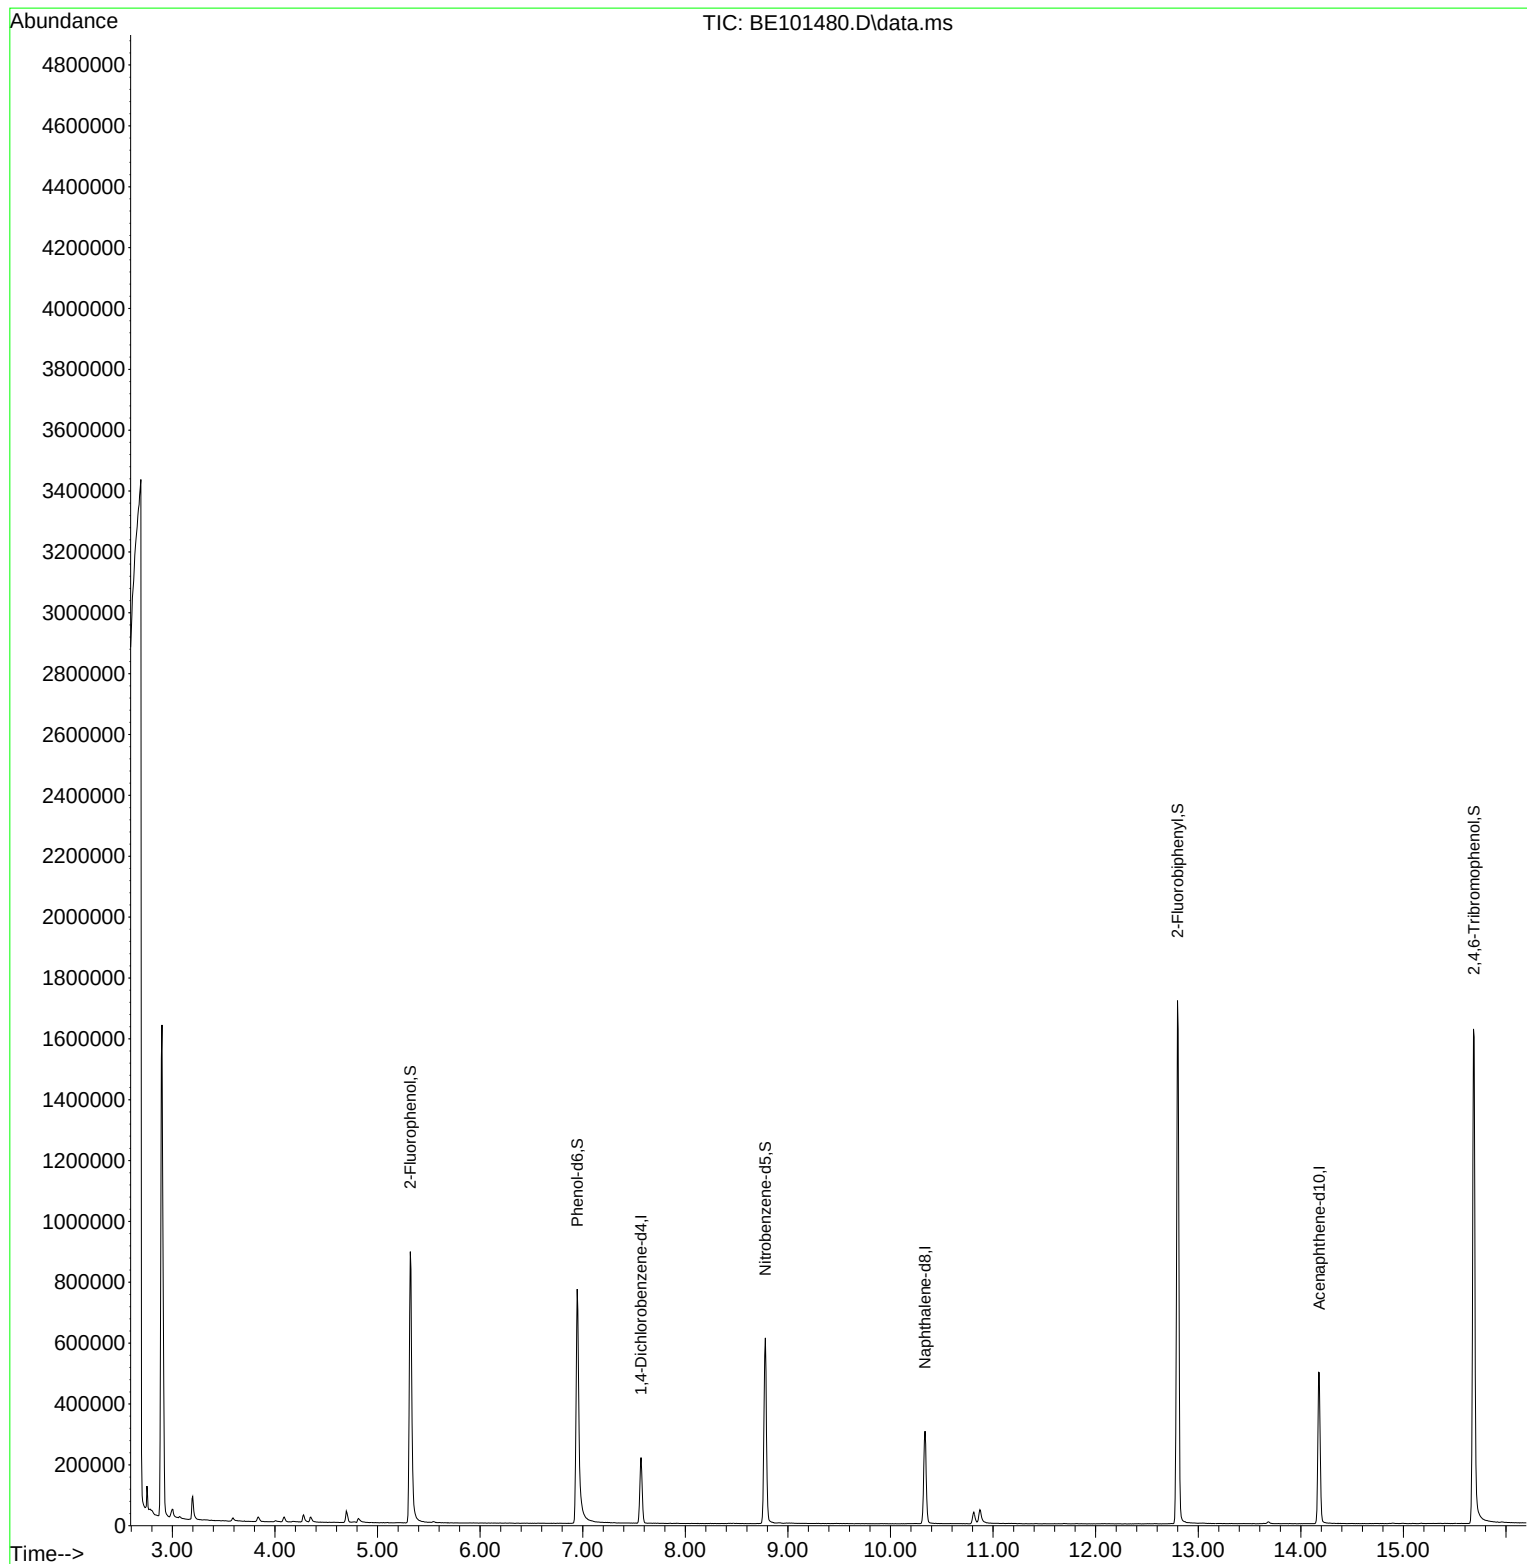

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101480.D
Acq On : 5 Nov 2024 15:43
Operator : RC/JU
Sample : P4640-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
MH-3

Quant Time: Nov 05 15:39:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

