

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
 Data File : BE101487.D
 Acq On : 5 Nov 2024 19:51
 Operator : RC/JU
 Sample : P4645-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Z-02-WC

Quant Time: Nov 06 00:03:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 29 01:26:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.570	152	57420	20.000	ng	0.00
21) Naphthalene-d8	10.337	136	236071	20.000	ng	0.00
39) Acenaphthene-d10	14.180	164	166348	20.000	ng	0.00
64) Phenanthrene-d10	16.917	188	407988	20.000	ng	0.00
76) Chrysene-d12	21.077	240	521310	20.000	ng	0.00
86) Perylene-d12	23.363	264	667650	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.325	112	427695	130.548	ng	0.00
7) Phenol-d6	6.947	99	491297	108.150	ng	0.00
23) Nitrobenzene-d5	8.780	82	347113	92.353	ng	0.00
42) 2,4,6-Tribromophenol	15.690	330	442355	151.723	ng	0.00
45) 2-Fluorobiphenyl	12.799	172	873658	88.944	ng	0.00
79) Terphenyl-d14	19.509	244	2215215	97.800	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101487.D
Acq On : 5 Nov 2024 19:51
Operator : RC/JU
Sample : P4645-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-02-WC

Quant Time: Nov 06 00:03:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

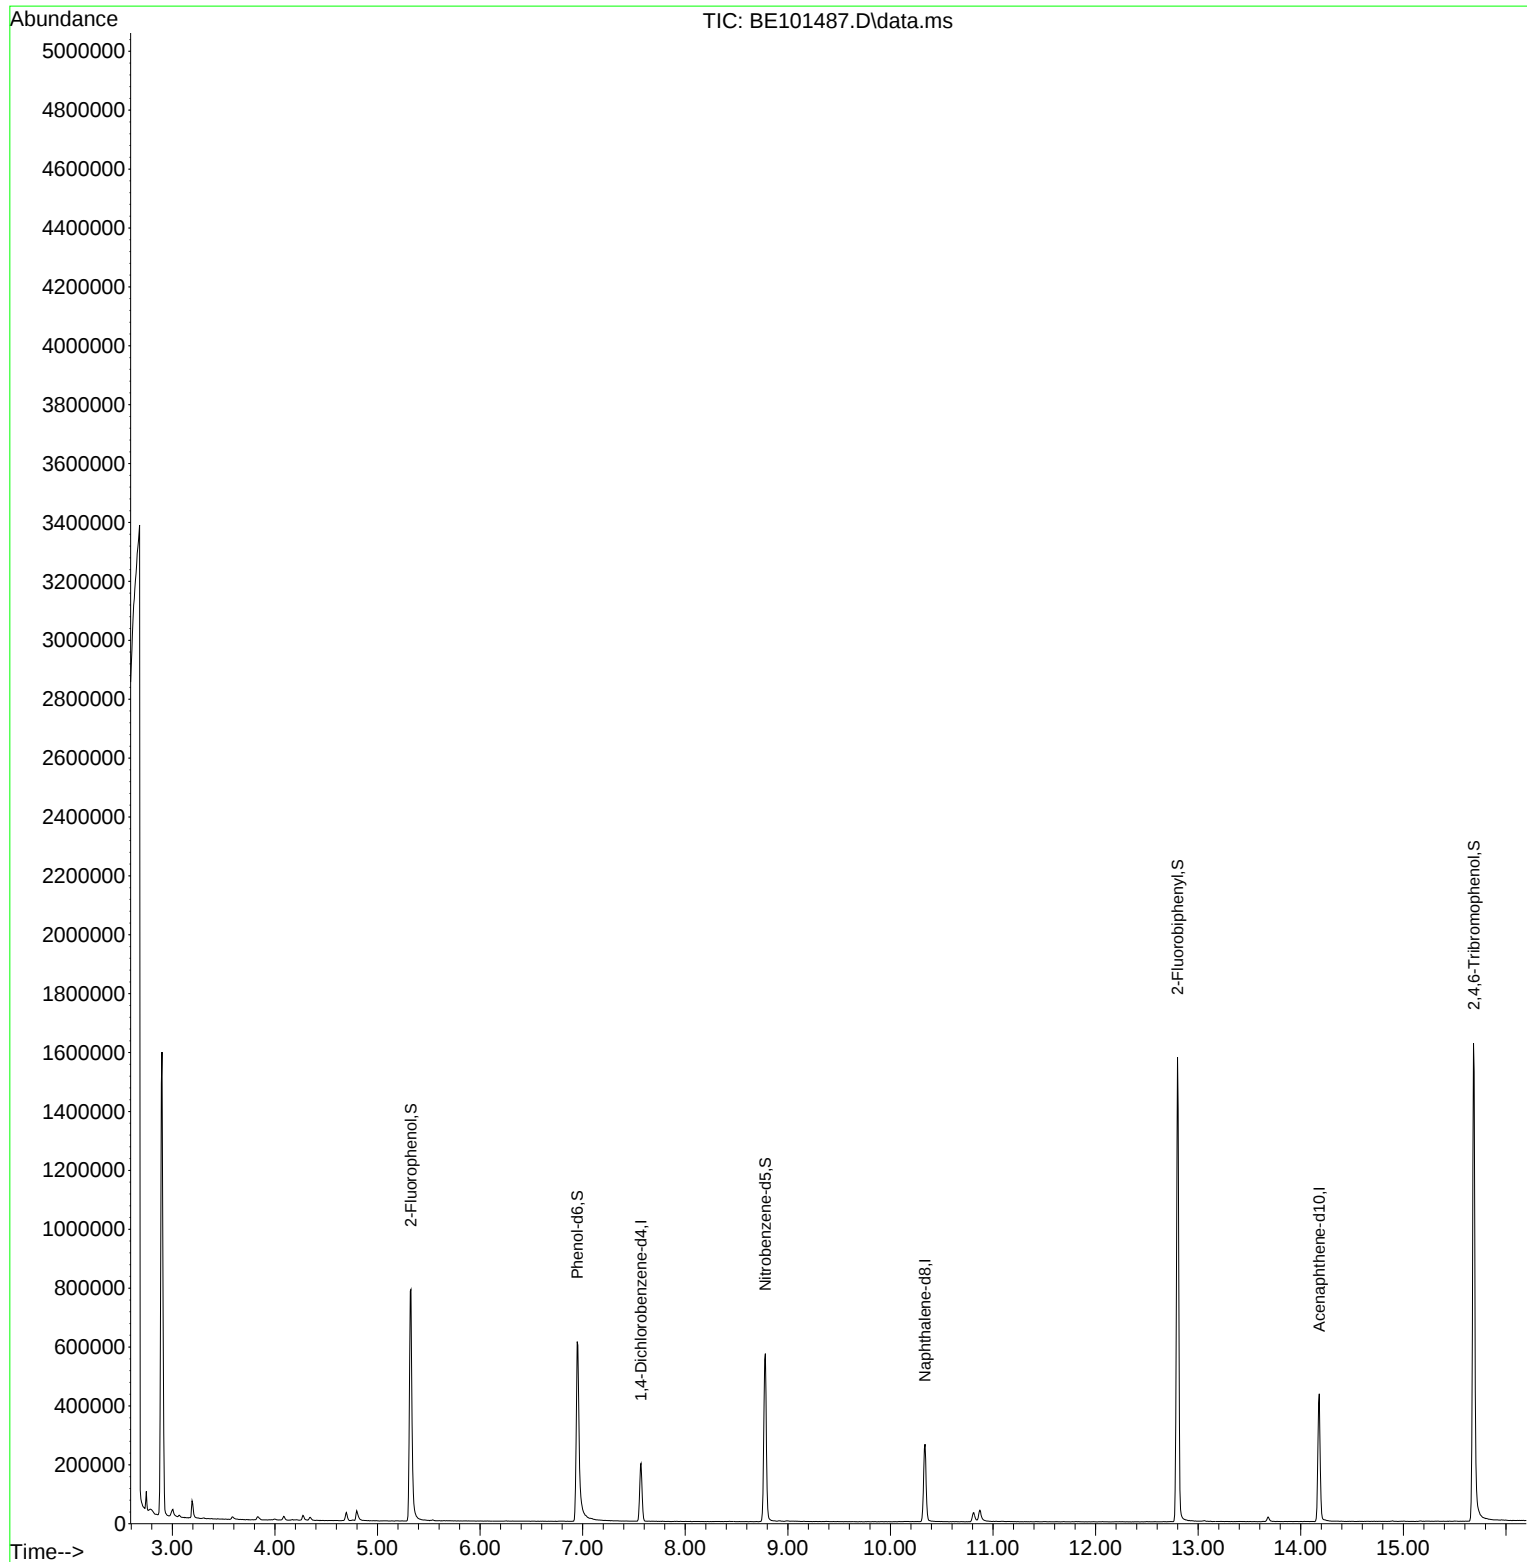

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101487.D
Acq On : 5 Nov 2024 19:51
Operator : RC/JU
Sample : P4645-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Z-02-WC

Quant Time: Nov 06 00:03:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

