
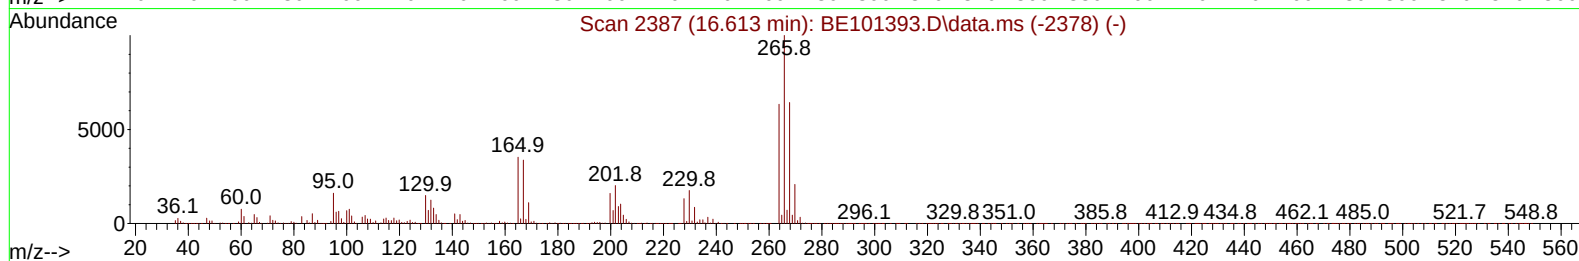
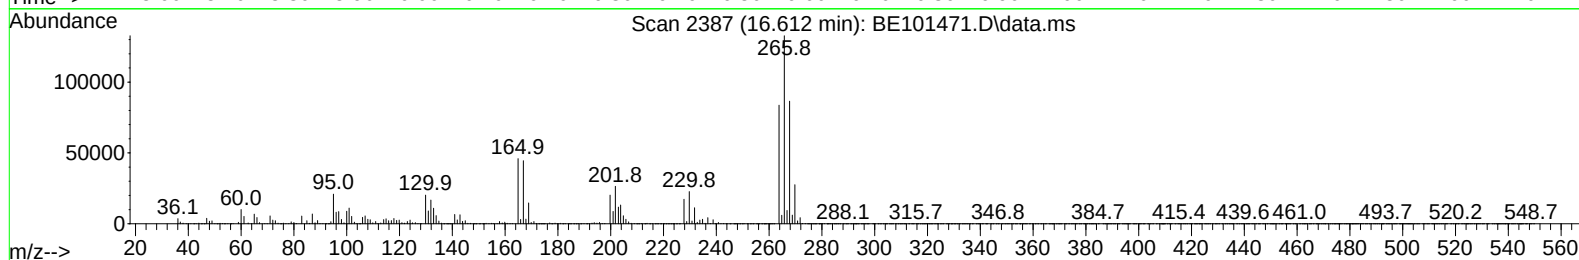


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101471.D
Acq On : 5 Nov 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 10:41:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

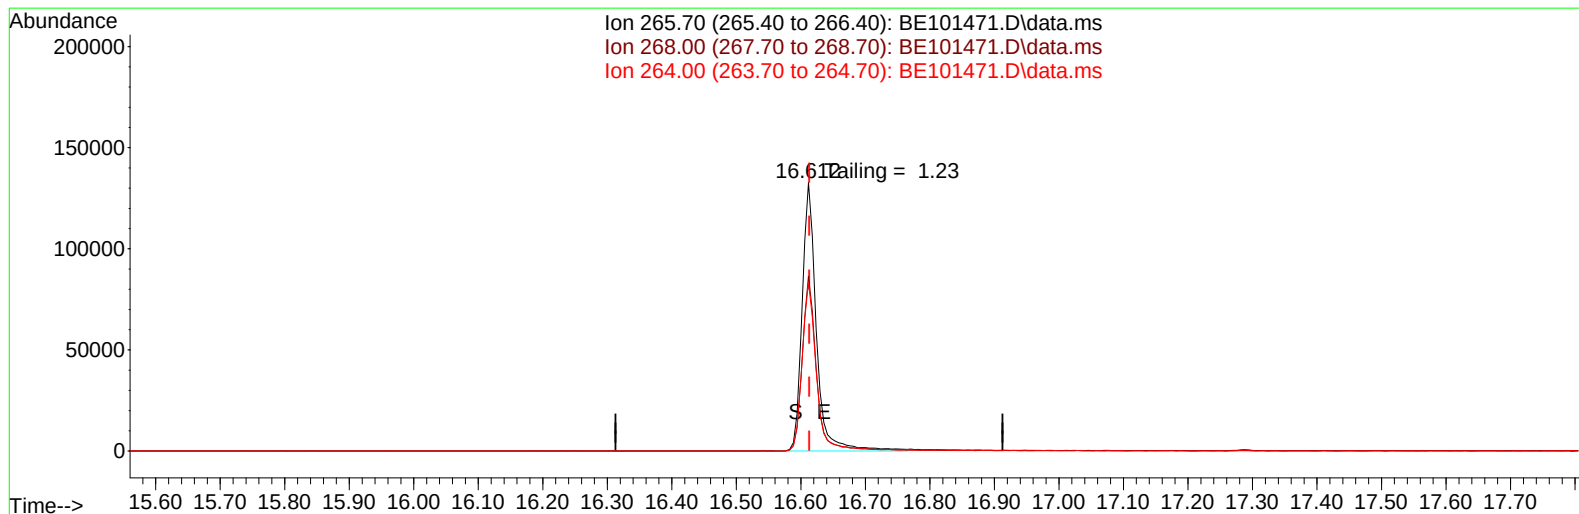

TIC: BE101471.D\data.ms

(70) Pentachlorophenol (C)




16.612min (-0.001) 1236265.89 ng

response 206048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.18
264.00	63.40	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101471.D
Acq On : 5 Nov 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 10:41:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

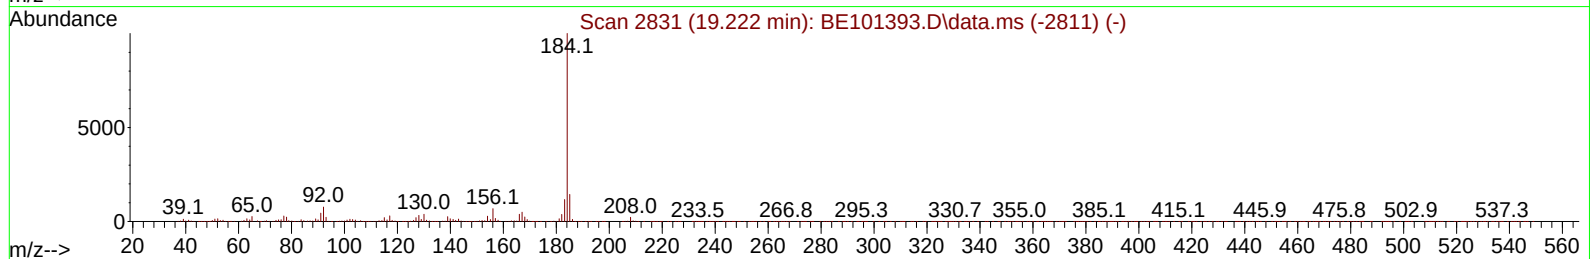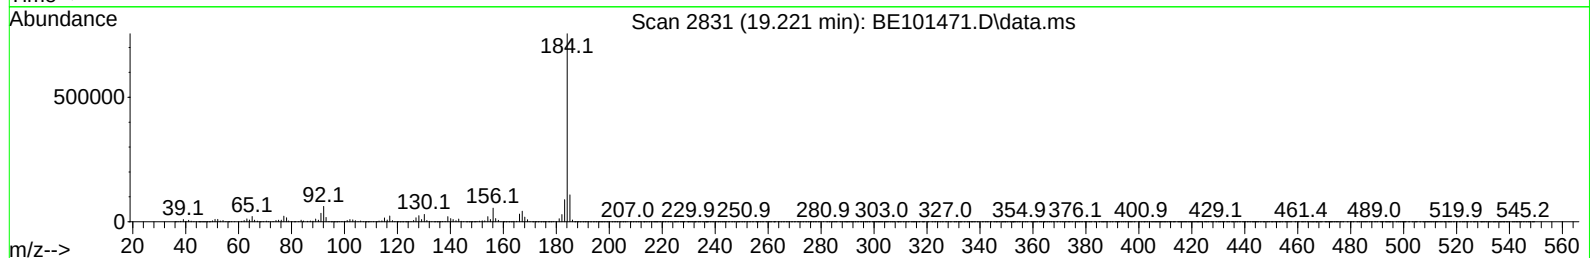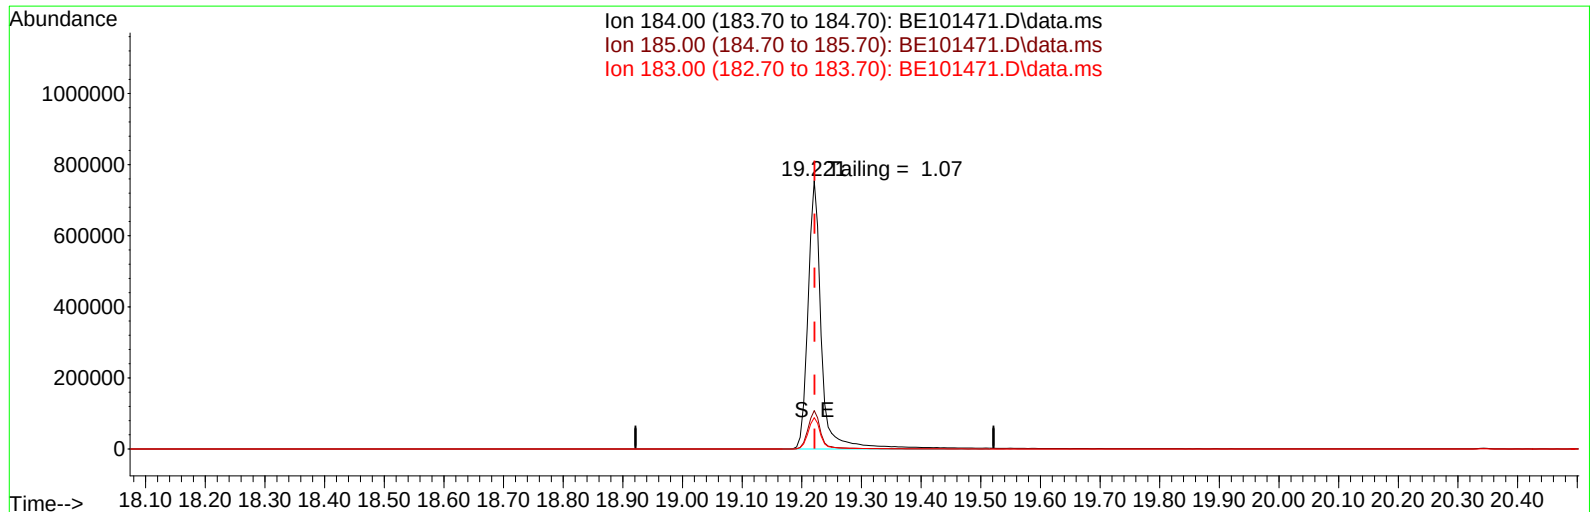

TIC: BE101471.D\data.ms

(77) Benzidine**19.221min (-0.001) 1366074.03 ng****response 1196307**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.33
183.00	11.60	11.71
0.00	0.00	0.00