

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101485.D
Acq On : 5 Nov 2024 18:39
Operator : RC/JU
Sample : P4643-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-9

Quant Time: Nov 06 00:03:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.567	152	60079	20.000	ng	0.00
21) Naphthalene-d8	10.334	136	257146	20.000	ng	0.00
39) Acenaphthene-d10	14.176	164	178286	20.000	ng	0.00
64) Phenanthrene-d10	16.914	188	428544	20.000	ng	0.00
76) Chrysene-d12	21.074	240	503216	20.000	ng	0.00
86) Perylene-d12	23.366	264	647563	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.322	112	478894	139.706	ng	0.00
7) Phenol-d6	6.944	99	573620	120.684	ng	0.00
23) Nitrobenzene-d5	8.777	82	387212	94.578	ng	0.00
42) 2,4,6-Tribromophenol	15.686	330	473043	151.384	ng	0.00
45) 2-Fluorobiphenyl	12.802	172	991641	94.196	ng	0.00
79) Terphenyl-d14	19.511	244	2259698	103.352	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101485.D
Acq On : 5 Nov 2024 18:39
Operator : RC/JU
Sample : P4643-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-9


Quant Time: Nov 06 00:03:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration

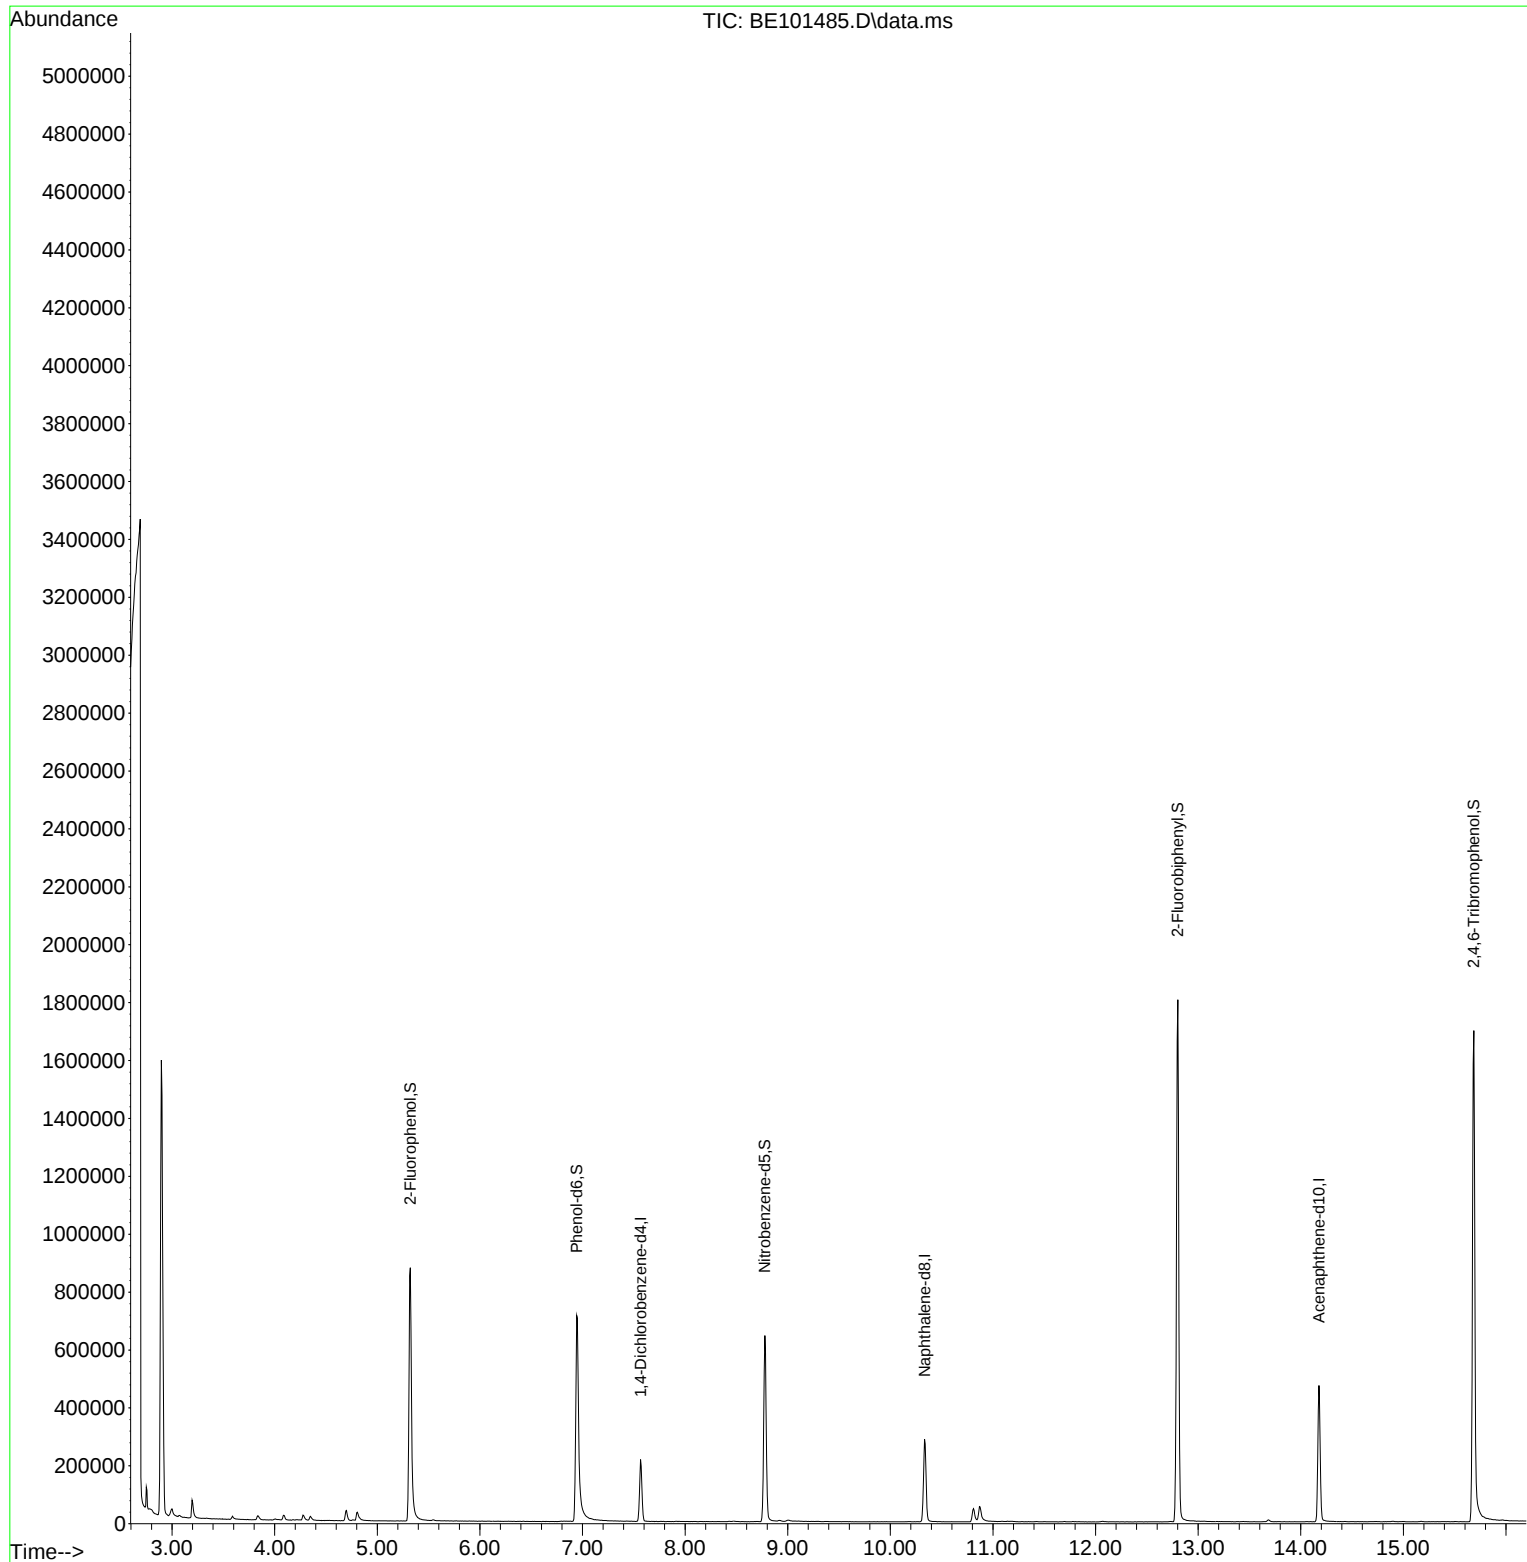


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101485.D
Acq On : 5 Nov 2024 18:39
Operator : RC/JU
Sample : P4643-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TP-9

Quant Time: Nov 06 00:03:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 29 01:26:30 2024
Response via : Initial Calibration




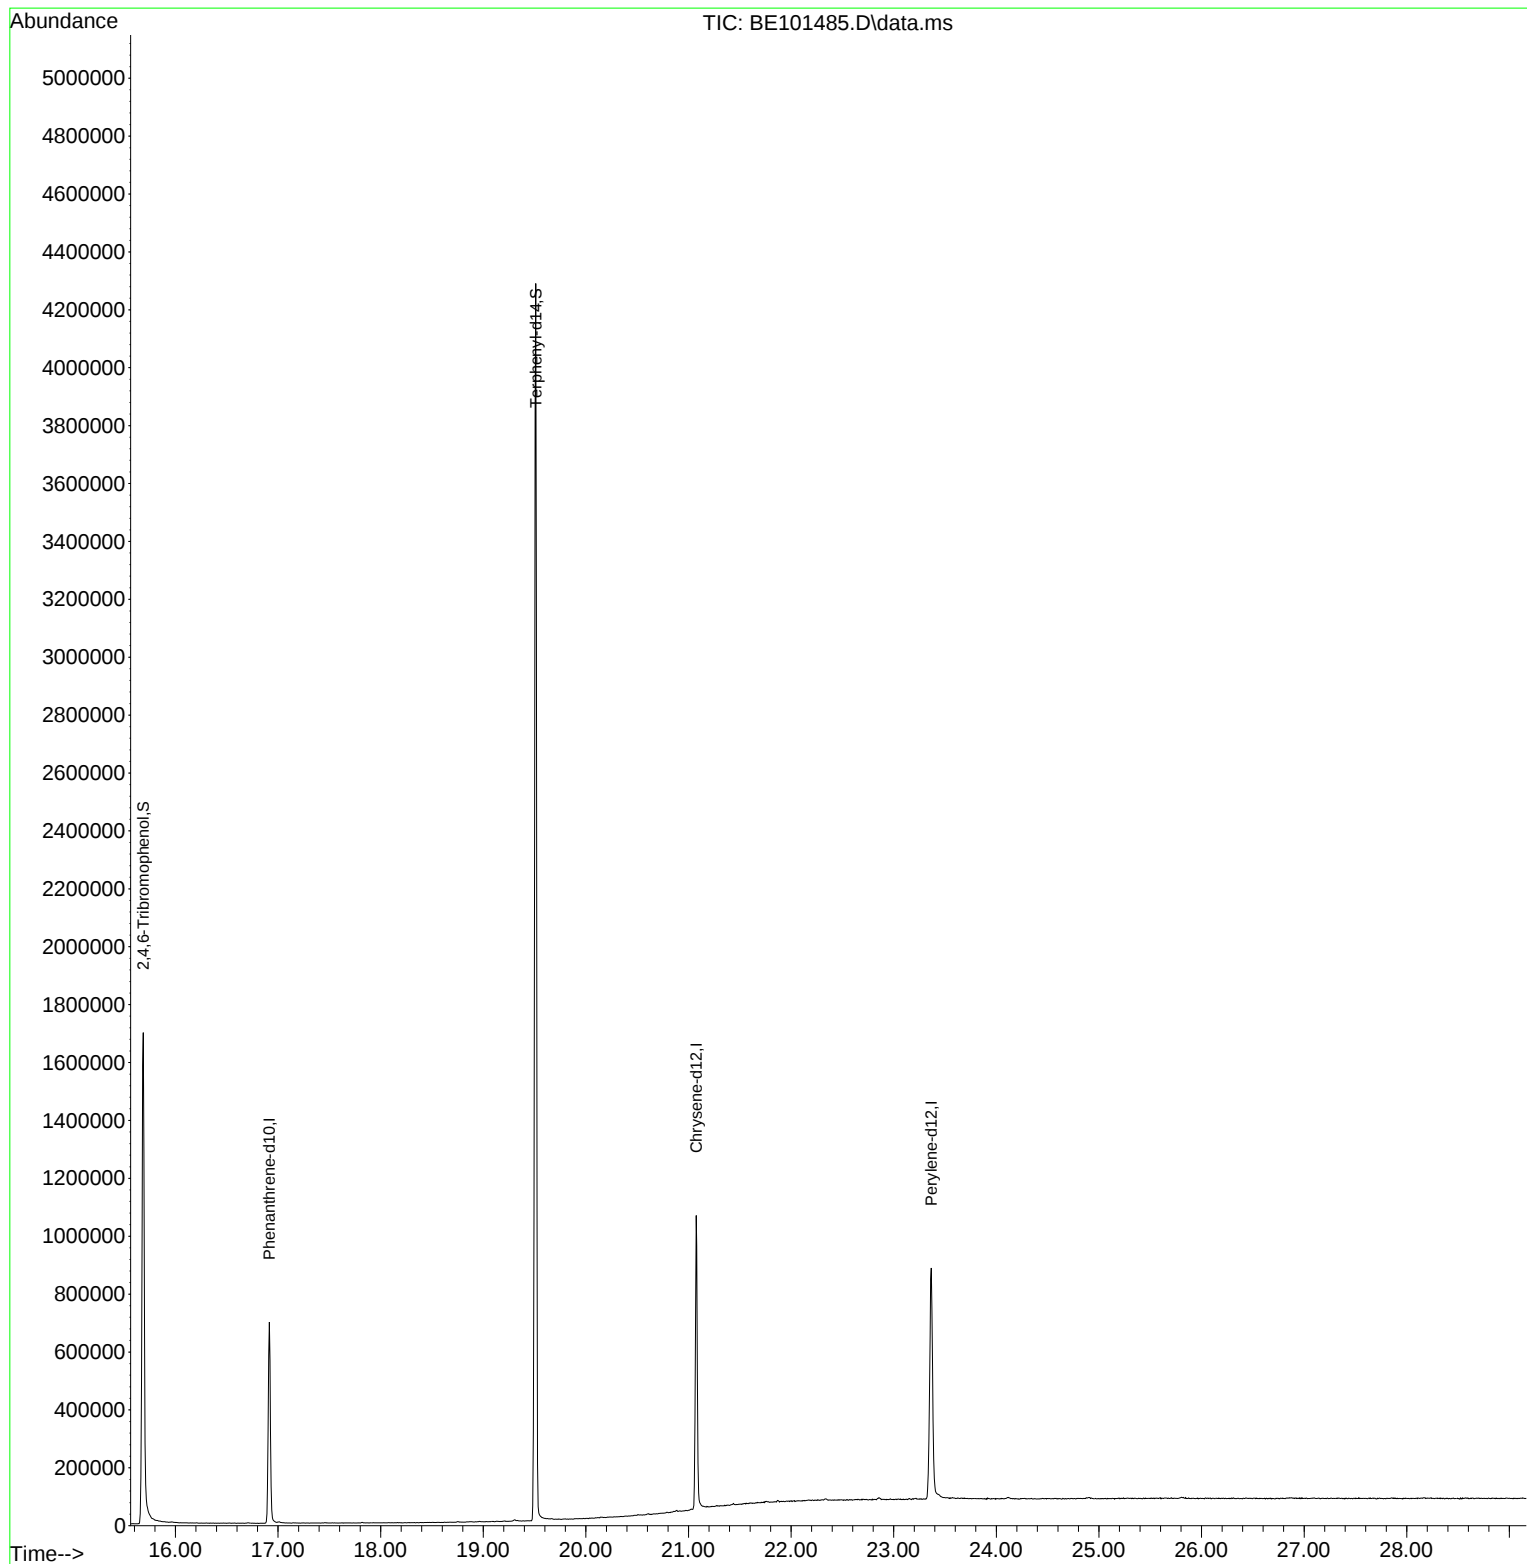


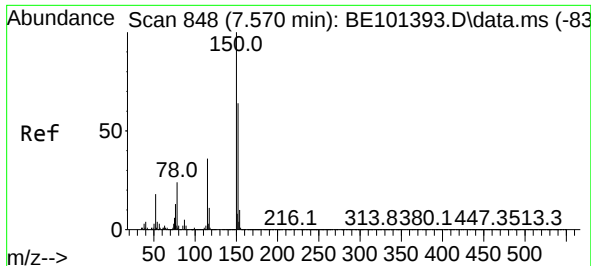

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.567 min Scan# 848
Delta R.T. -0.003 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39




Instrument :
BNA_E
ClientSampleId :
TP-9


Tgt Ion:152 Resp: 60079
Ion Ratio Lower Upper
152 100
150 157.0 124.2 186.4
115 56.7 45.3 67.9

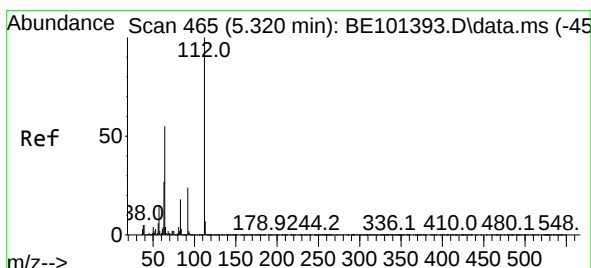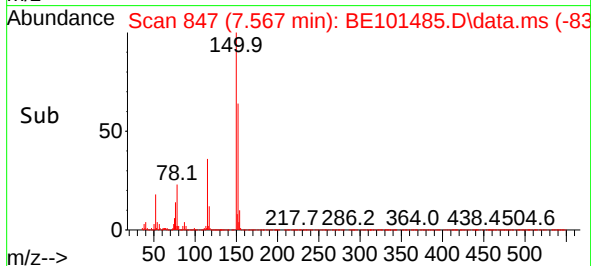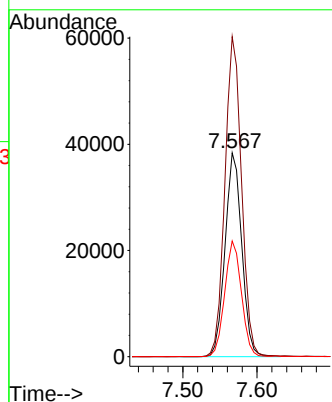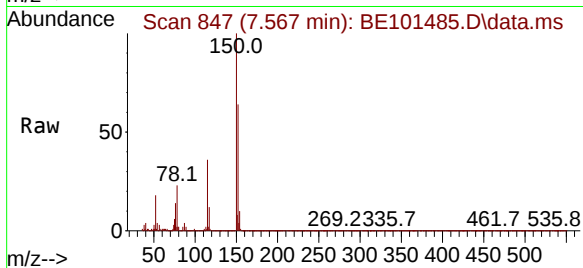

#5
2-Fluorophenol
Concen: 139.706 ng
RT: 5.322 min Scan# 465
Delta R.T. 0.002 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39

Tgt Ion:112 Resp: 478894
Ion Ratio Lower Upper
112 100
64 53.6 43.7 65.5
63 27.2 21.4 32.2


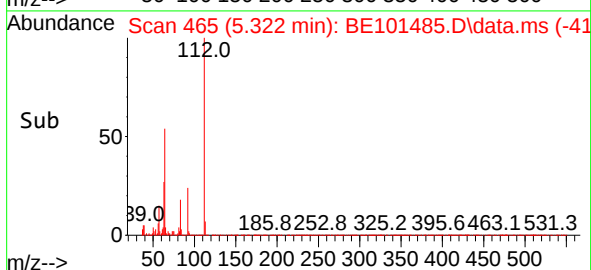
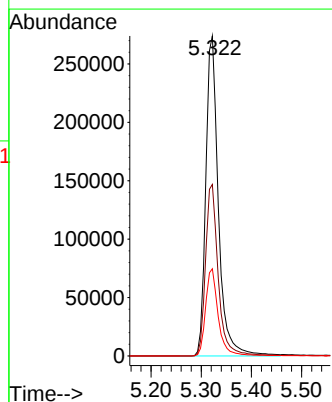
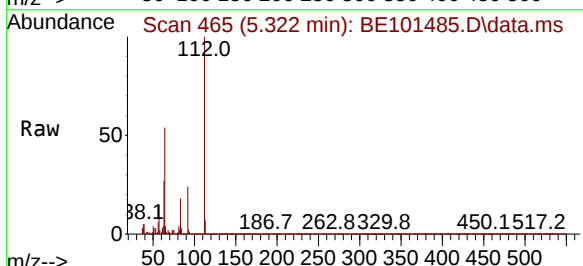


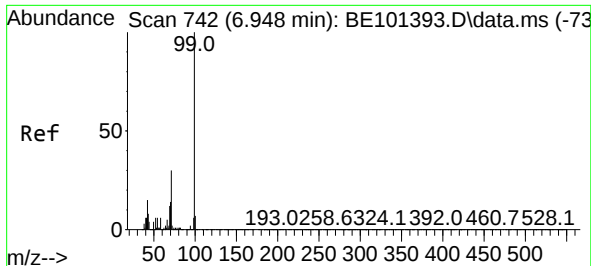

#7
Phenol-d6
Concen: 120.684 ng
RT: 6.944 min Scan# 741
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39




Instrument :
BNA_E
ClientSampleId :
TP-9


Tgt Ion: 99 Resp: 573620
Ion Ratio Lower Upper
99 100
42 16.1 12.3 18.5
71 30.1 23.8 35.8

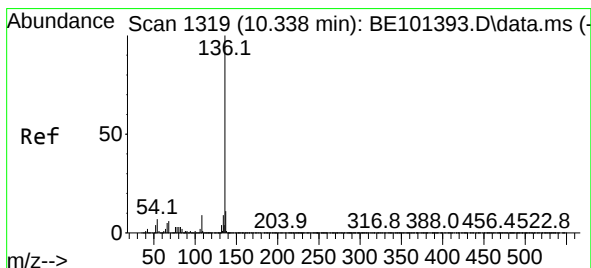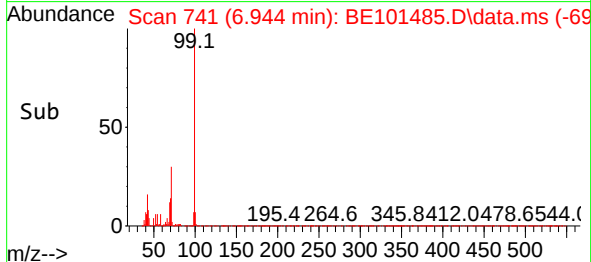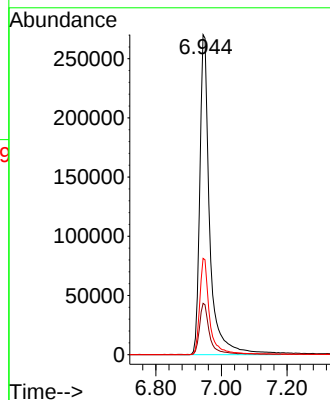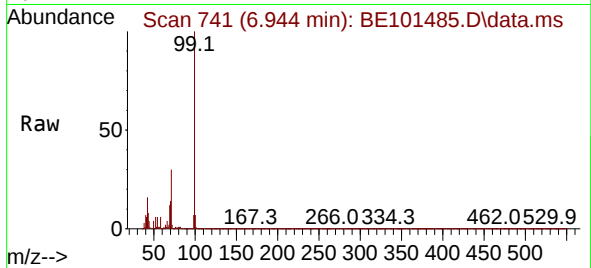

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.334 min Scan# 1318
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39

Tgt Ion:136 Resp: 257146
Ion Ratio Lower Upper
136 100
137 11.4 9.0 13.6
54 7.3 5.9 8.9
68 6.4 4.8 7.2


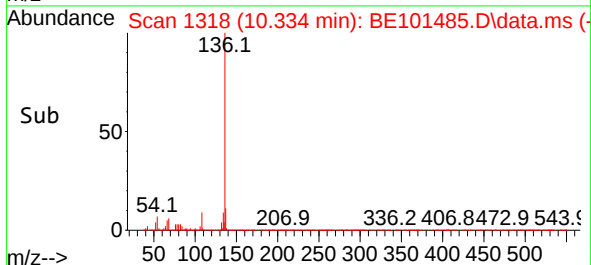
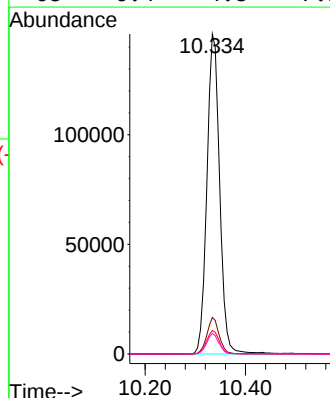
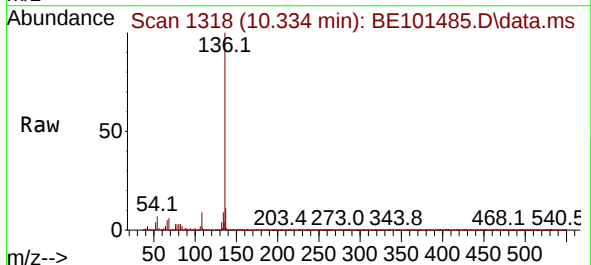


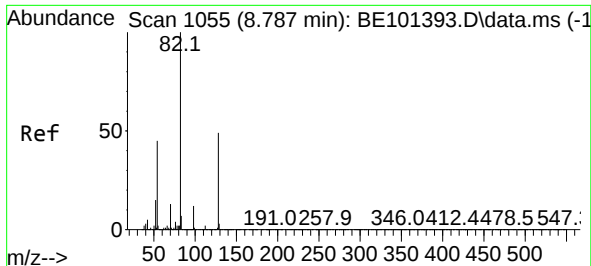

#23
Nitrobenzene-d5
Concen: 94.578 ng
RT: 8.777 min Scan# 1053
Delta R.T. -0.010 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39




Instrument :
BNA_E
ClientSampleId :
TP-9


Tgt Ion: 82 Resp: 387212
Ion Ratio Lower Upper
82 100
128 47.7 38.9 58.3
54 46.2 36.2 54.4

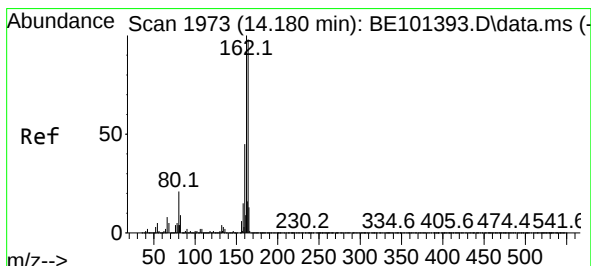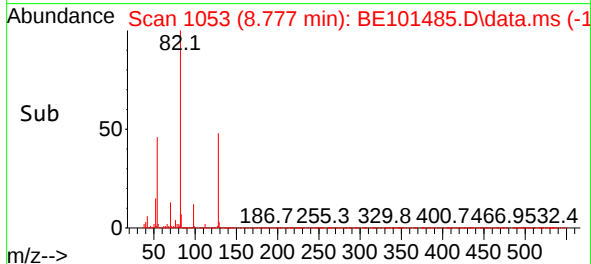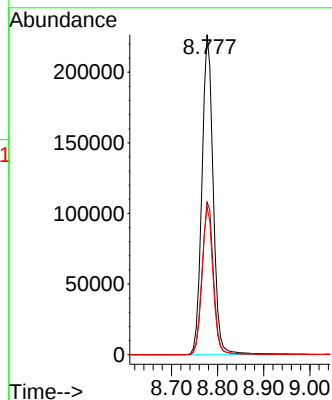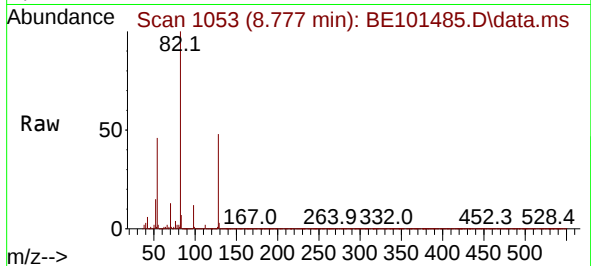

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.176 min Scan# 1972
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39

Tgt Ion: 164 Resp: 178286
Ion Ratio Lower Upper
164 100
162 103.7 81.3 121.9
160 46.4 36.4 54.6


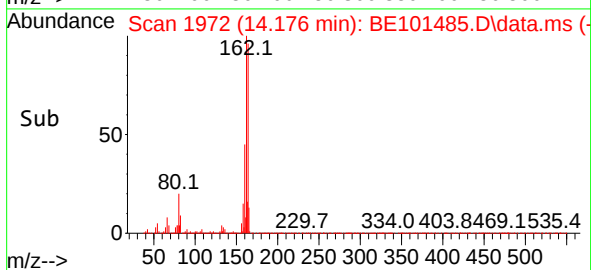
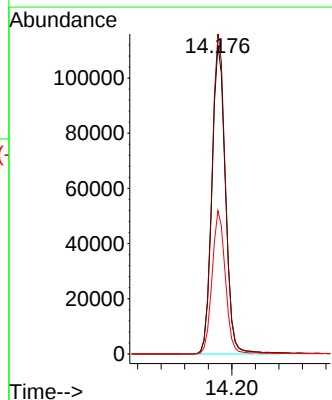
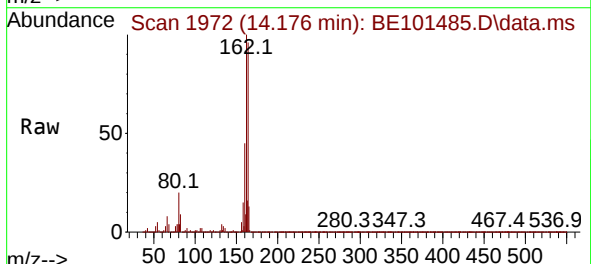


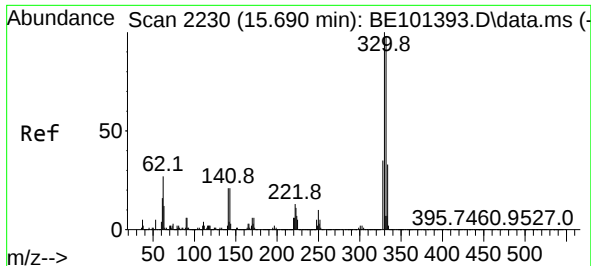

#42
2,4,6-Tribromophenol
Concen: 151.384 ng
RT: 15.686 min Scan# 21
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39




Instrument :
BNA_E
ClientSampleId :
TP-9


Tgt Ion:330 Resp: 473043
Ion Ratio Lower Upper
330 100
332 96.8 78.2 117.2
141 21.5 18.3 27.5

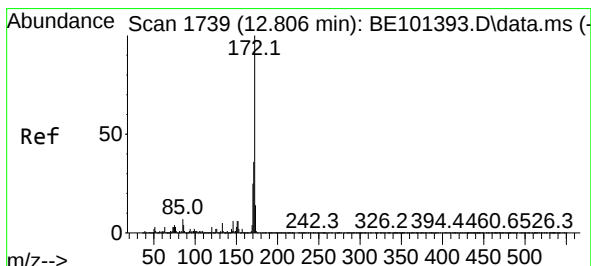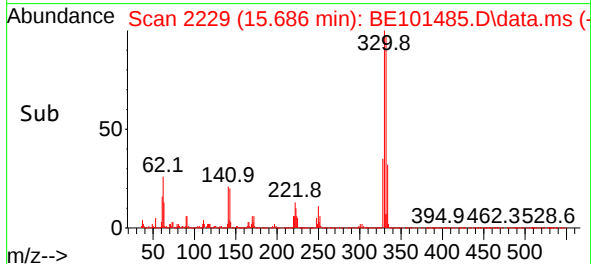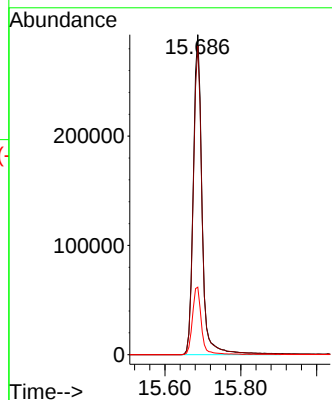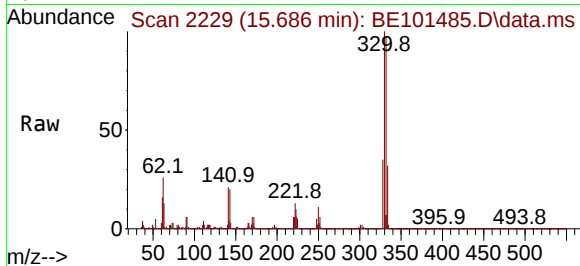

#45
2-Fluorobiphenyl
Concen: 94.196 ng
RT: 12.802 min Scan# 1738
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39

Tgt Ion:172 Resp: 991641
Ion Ratio Lower Upper
172 100
171 35.4 29.2 43.8
170 23.7 19.8 29.6


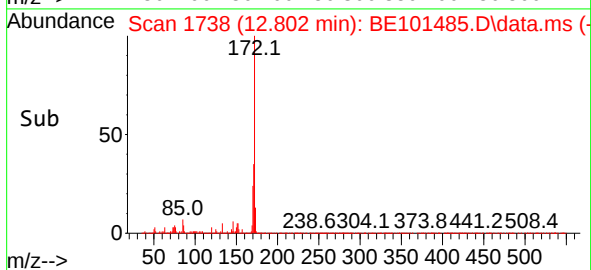
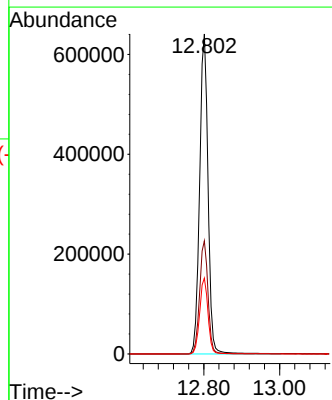
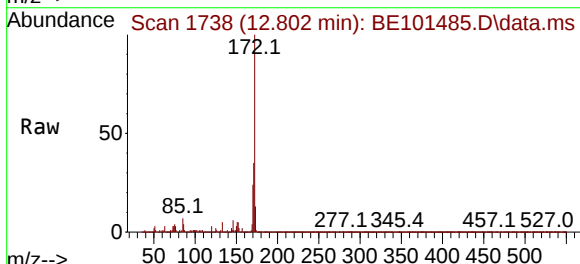


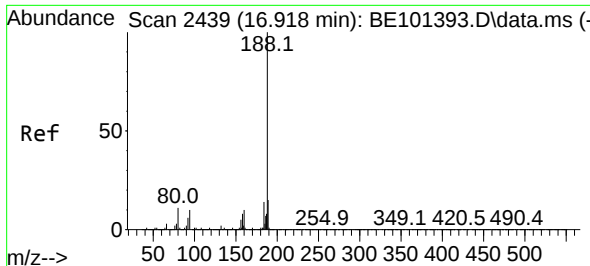

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.914 min Scan# 2438
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39




Instrument :
BNA_E
ClientSampleId :
TP-9


Tgt Ion:188 Resp: 428544
Ion Ratio Lower Upper
188 100
94 9.8 7.8 11.8
80 10.3 8.6 12.8

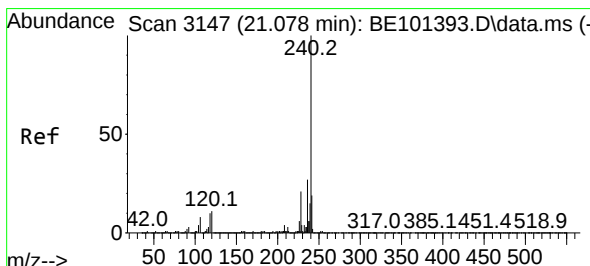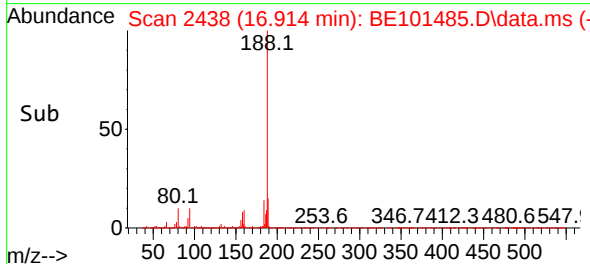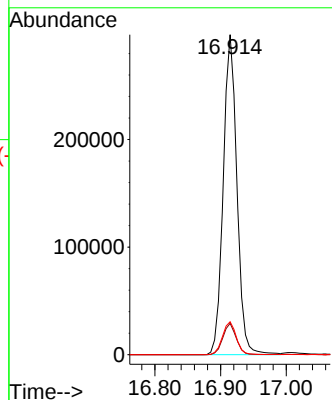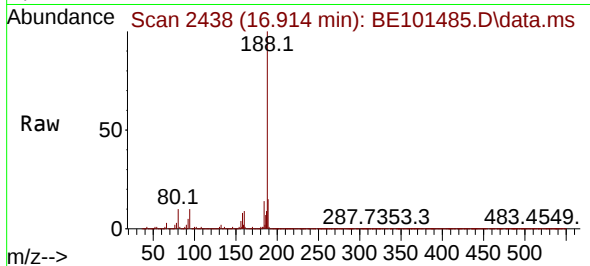

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.074 min Scan# 3146
Delta R.T. -0.004 min
Lab File: BE101485.D
Acq: 5 Nov 2024 18:39

Tgt Ion:240 Resp: 503216
Ion Ratio Lower Upper
240 100
120 10.6 9.0 13.4
236 26.6 21.4 32.0

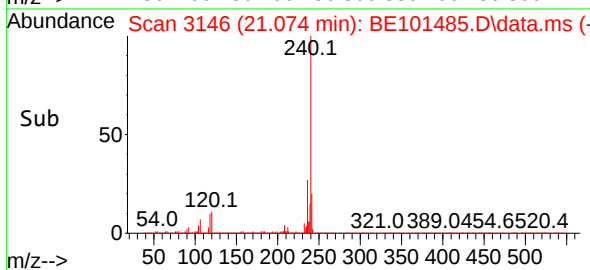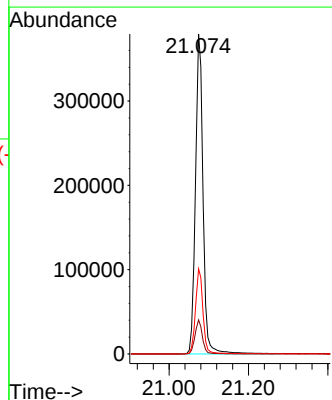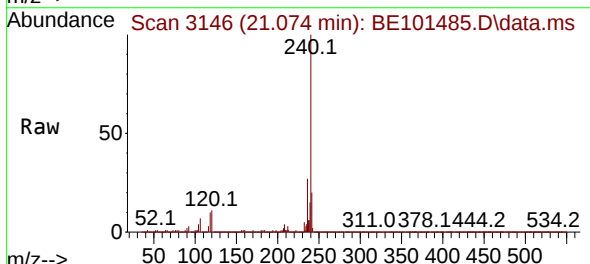

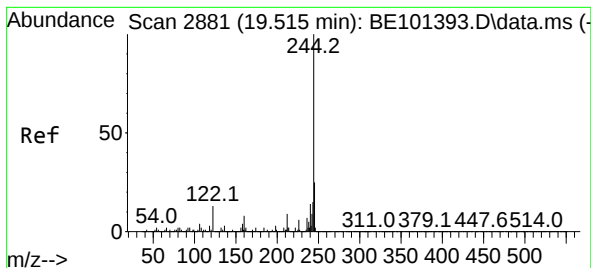

#79

Terphenyl-d14

Concen: 103.352 ng

RT: 19.511 min Scan# 21

Delta R.T. -0.004 min

Lab File: BE101485.D

Acq: 5 Nov 2024 18:39

Instrument :

BNA_E

ClientSampleId :

TP-9





Tgt Ion:244 Resp: 2259698

Ion Ratio Lower Upper

244 100

212 7.6 7.2 10.8

122 10.8 10.4 15.6

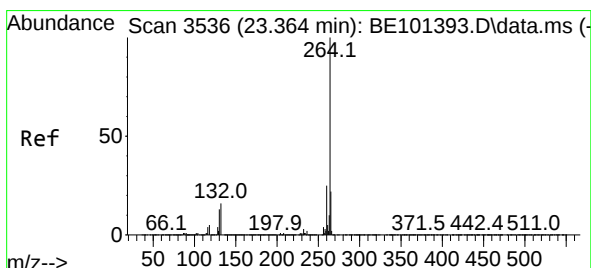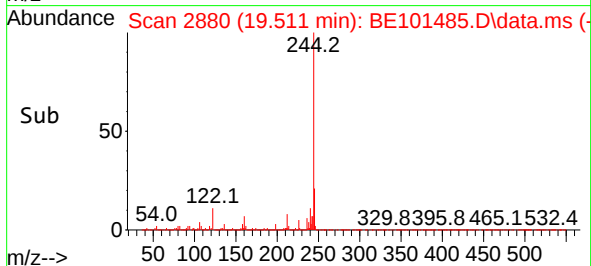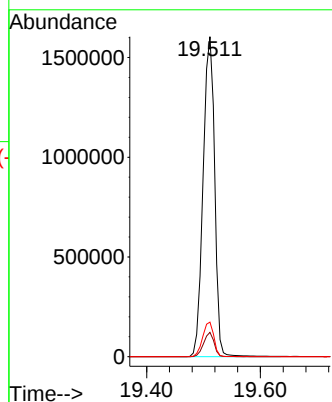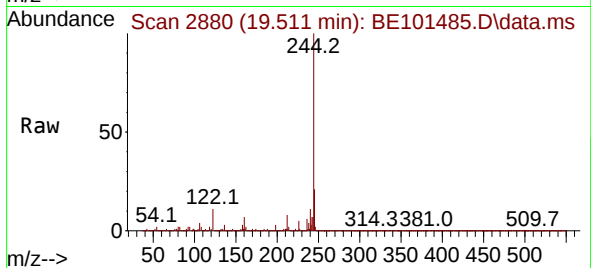

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.366 min Scan# 3536

Delta R.T. 0.002 min

Lab File: BE101485.D

Acq: 5 Nov 2024 18:39

Tgt Ion:264 Resp: 647563

Ion Ratio Lower Upper

264 100

260 24.4 19.8 29.8

265 21.8 17.6 26.4

