

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
 Data File : BE101473.D
 Acq On : 5 Nov 2024 11:33
 Operator : RC/JU
 Sample : PB164639BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164639BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BE101473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.319	458	465	487	rBV	1072647	1808503	32.59%	8.274%
2	6.947	734	742	772	rBV	896072	1819093	32.78%	8.323%
3	7.570	841	848	863	rVB	247616	386674	6.97%	1.769%
4	8.780	1045	1054	1076	rBV	681150	1158793	20.88%	5.302%
5	10.337	1307	1319	1340	rBV	312702	549762	9.91%	2.515%
6	12.805	1730	1739	1761	rBV	1917387	2938996	52.97%	13.446%
7	14.179	1966	1973	1990	rBV	488343	758412	13.67%	3.470%
8	15.689	2222	2230	2256	rBV	1642139	2649175	47.74%	12.120%
9	16.917	2432	2439	2452	rBV	677850	973284	17.54%	4.453%
10	19.514	2874	2881	2899	rBV	4042980	5548900	100.00%	25.387%
11	21.077	3141	3147	3158	rBV	1068283	1459064	26.29%	6.675%
12	23.369	3529	3537	3550	rBV	859561	1806694	32.56%	8.266%




Sum of corrected areas: 21857350

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101473.D
Acq On : 5 Nov 2024 11:33
Operator : RC/JU
Sample : PB164639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164639BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

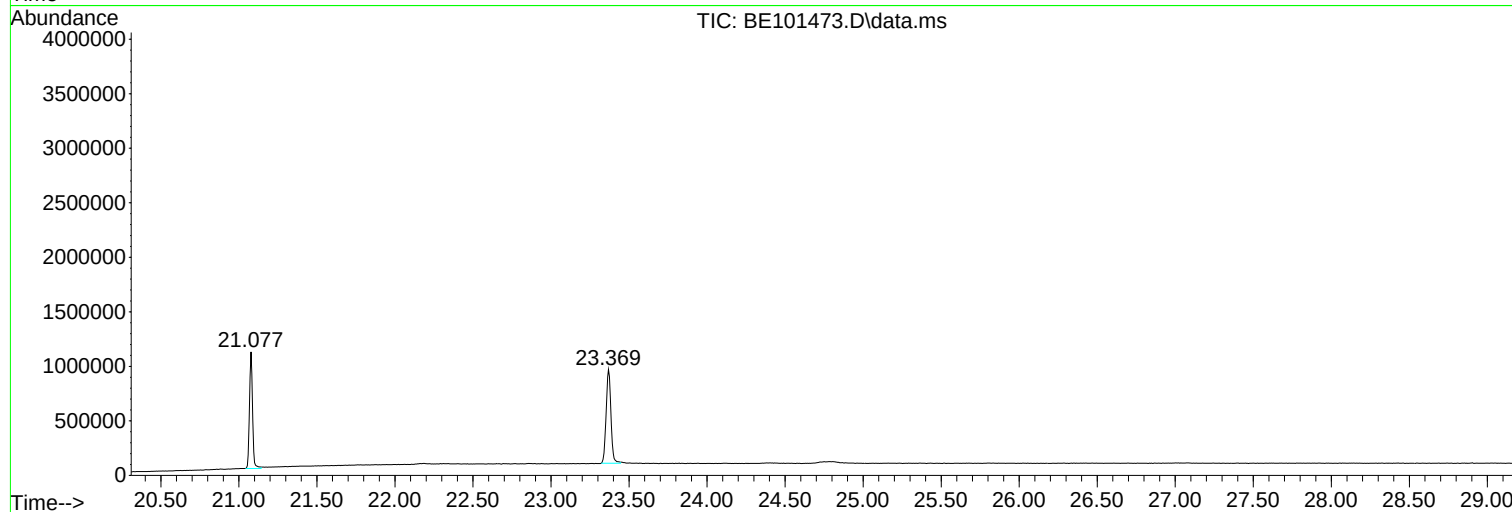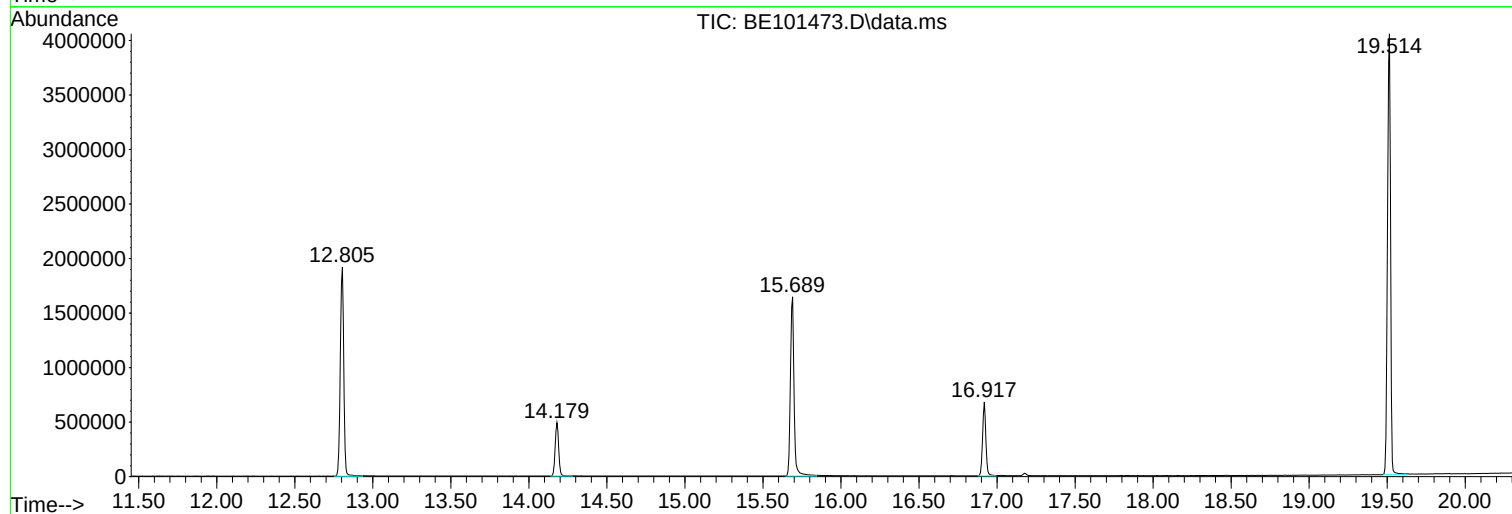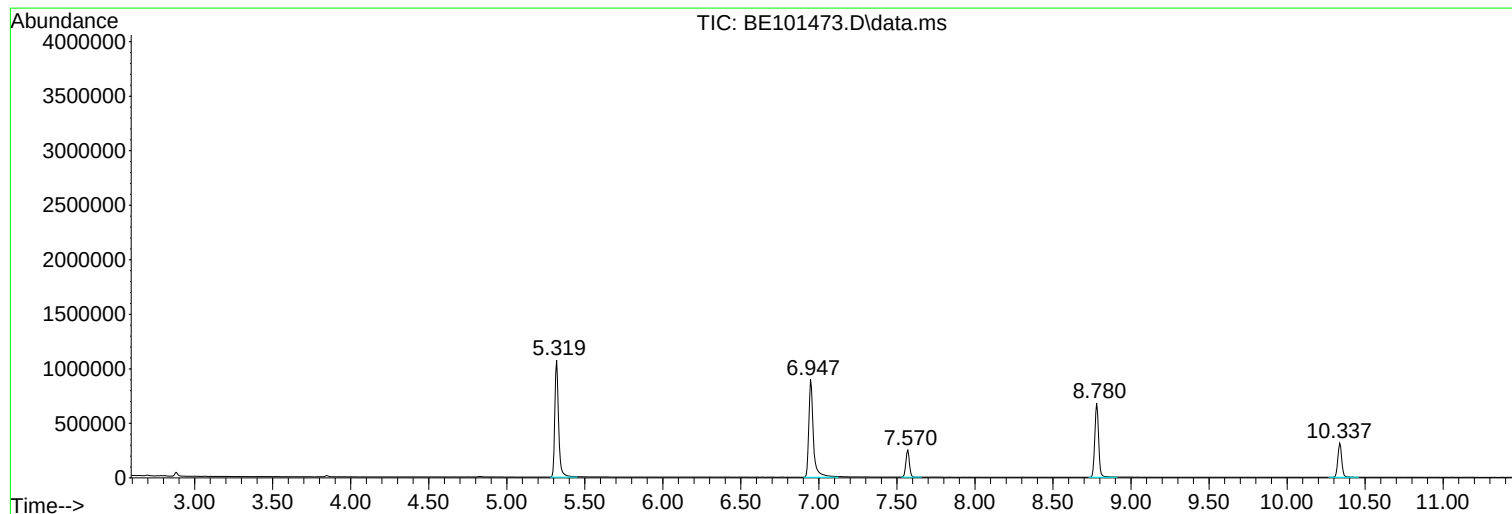

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101473.D
Acq On : 5 Nov 2024 11:33
Operator : RC/JU
Sample : PB164639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164639BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE110524\
Data File : BE101473.D
Acq On : 5 Nov 2024 11:33
Operator : RC/JU
Sample : PB164639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164639BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE102824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------