

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
 Data File : BE094748.D
 Acq On : 6 Nov 2017 12:05
 Operator : SJ/JU
 Sample : I5955-11
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-14(7-7.5)-101717

Quant Time: Nov 07 00:12:45 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 00:12:32 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1166	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.69	136	7242	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4254	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.44	240	8671	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	490060	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	2942	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	7152	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.65	202	1078	0.04	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE110617\
Data File : BE094748.D
Acq On : 6 Nov 2017 12:05
Operator : SJ/JU
Sample : I5955-11
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-14(7-7.5)-101717

Quant Time: Nov 07 00:12:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 00:12:32 2017
Response via : Initial Calibration

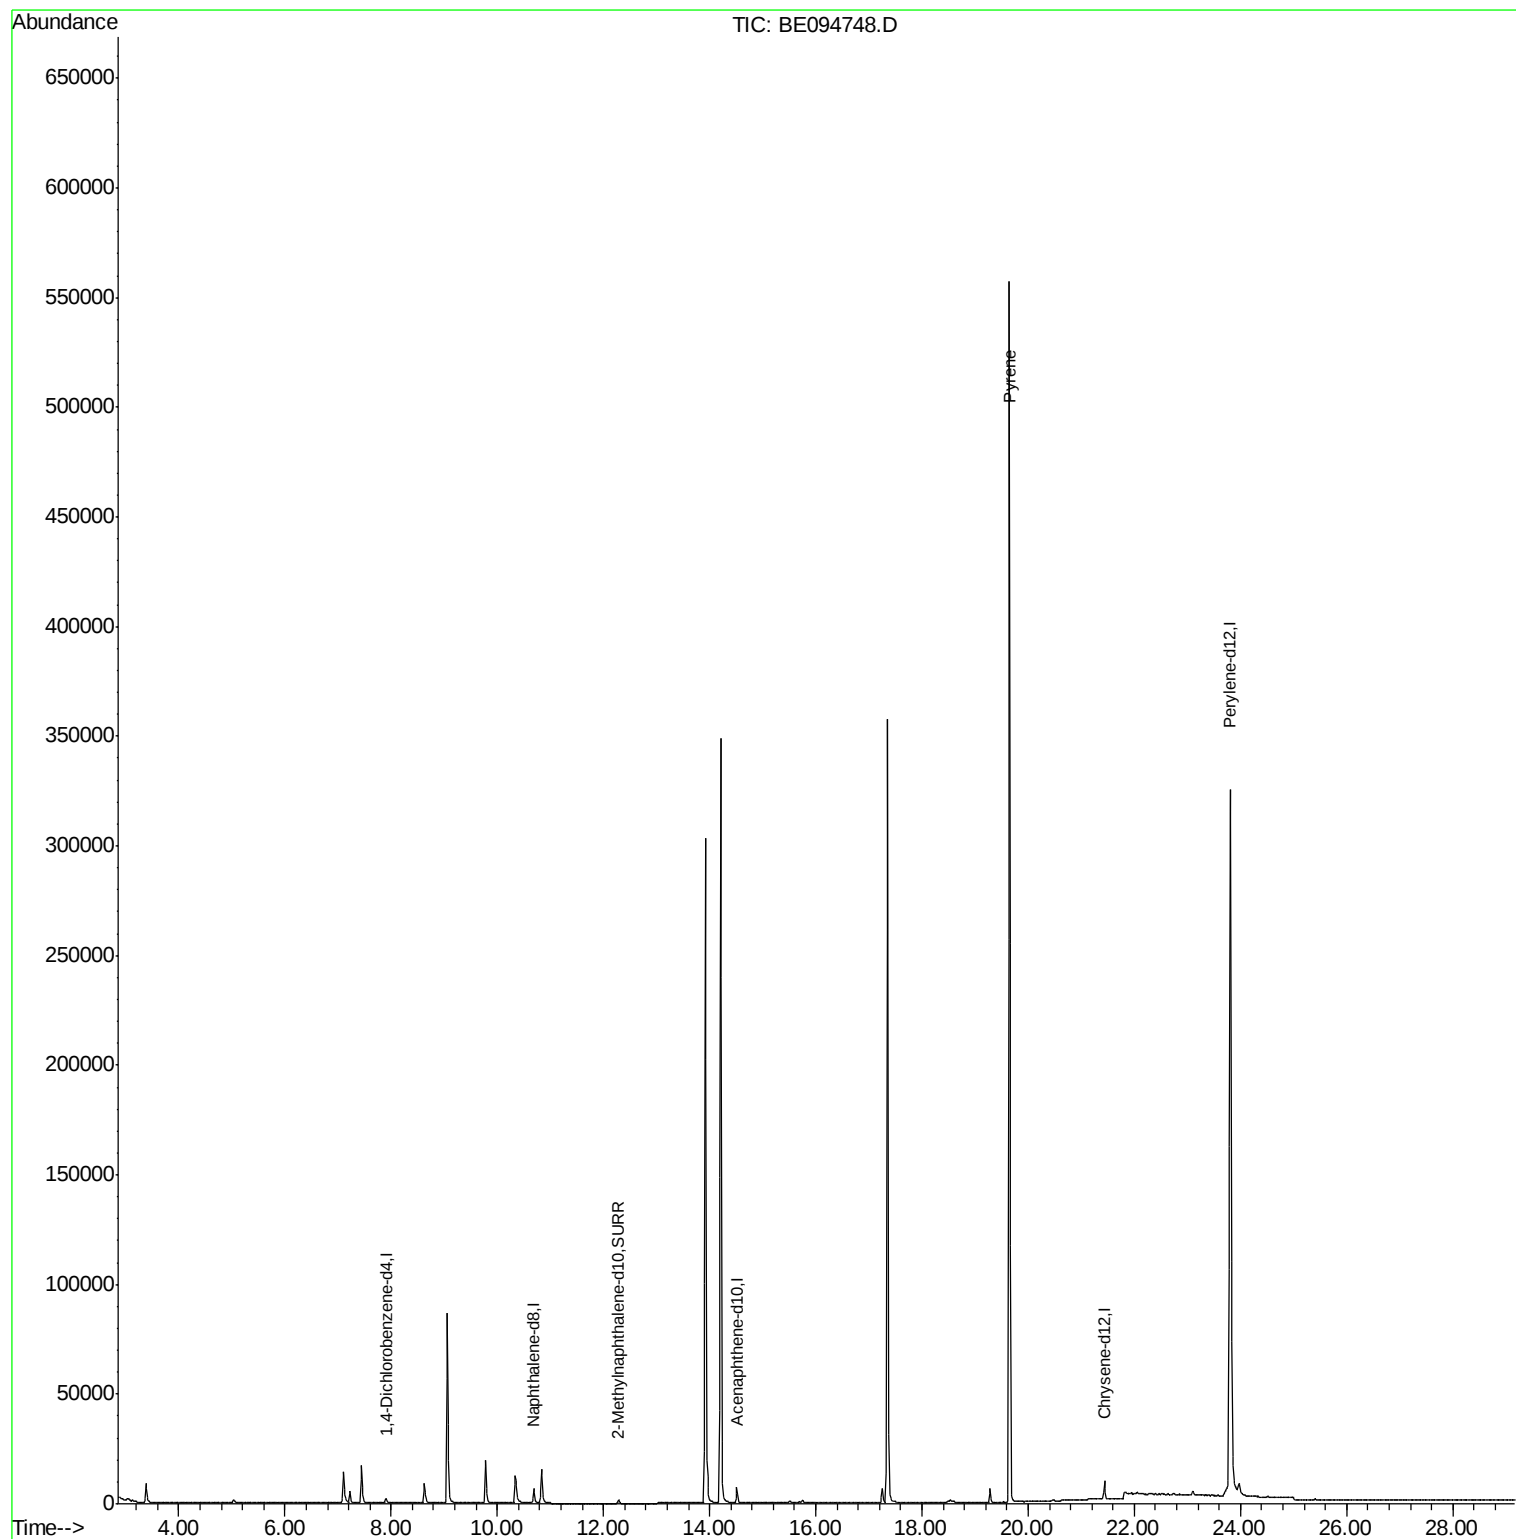

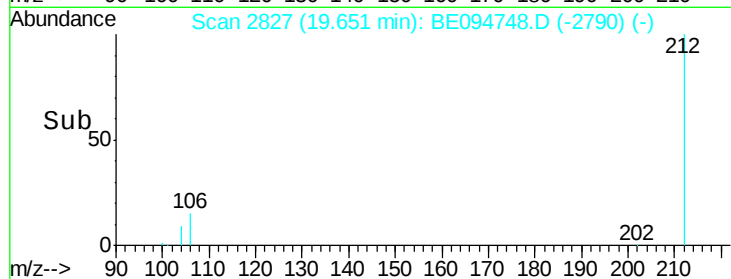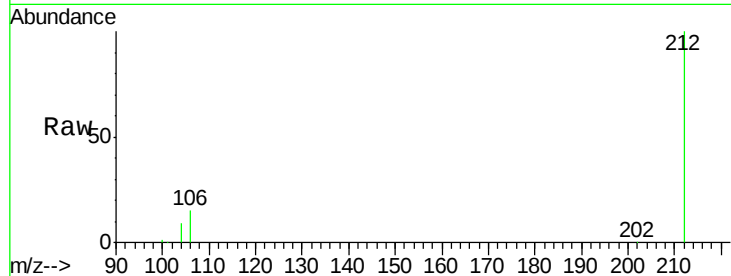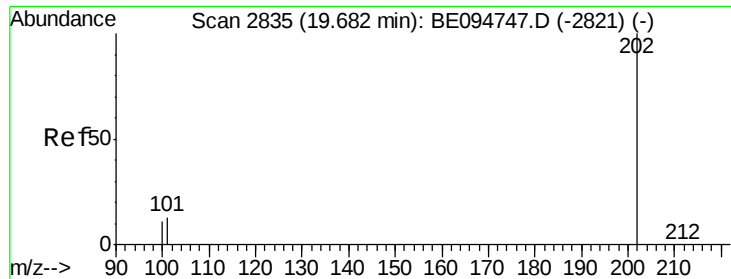

#17

Pvrene

Concen: 0.04 ng/ul

RT: 19.65 min Scan# 2827

Delta R.T. -0.03 min

Lab File: BE094748.D

Acq: 6 Nov 2017 12:05

Instrument :

BNA_E

ClientSampleId :

B-14(7-7.5)-101717

Tot Ion:202 Resp: 1078

Ion Ratio Lower Upper

202 100

101 137.3 18.2 27.4#

100 666.1 15.6 23.4#

